

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013019\
 Data File : FB019594.D
 Signal(s) : FID2B.CH
 Acq On : 30 Jan 2019 15:42
 Operator : MJ/SJ
 Sample : K1282-30MS
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 15 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jan 30 23:45:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
 Quant Title :
 QLast Update : Tue Jan 29 12:07:12 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.049	185686	15.885 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.900	525802	30.370 ng/ml
2) t 2,2,4-Trimethylpentane	7.662	487673	29.407 ng/ml
3) t n-Heptane	8.003	150937	9.366 ng/ml
4) t Benzene	8.140	184140	9.763 ng/ml
6) t Toluene	10.896	507044	28.986 ng/ml
7) t Ethylbenzene	13.348	206991	9.432 ng/ml
8) t m-Xylene	13.482	435452	19.026 ng/ml
9) t O-Xylene	14.214	432785	19.377 ng/ml
10) t 1,2,4-Trimethylbenzene	16.500	438609	18.930 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013019\
Data File : FB019594.D
Signal(s) : FID2B.CH
Acq On : 30 Jan 2019 15:42
Operator : MJ/SJ
Sample : K1282-30MS
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 15 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jan 30 23:45:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
Quant Title :
QLast Update : Tue Jan 29 12:07:12 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

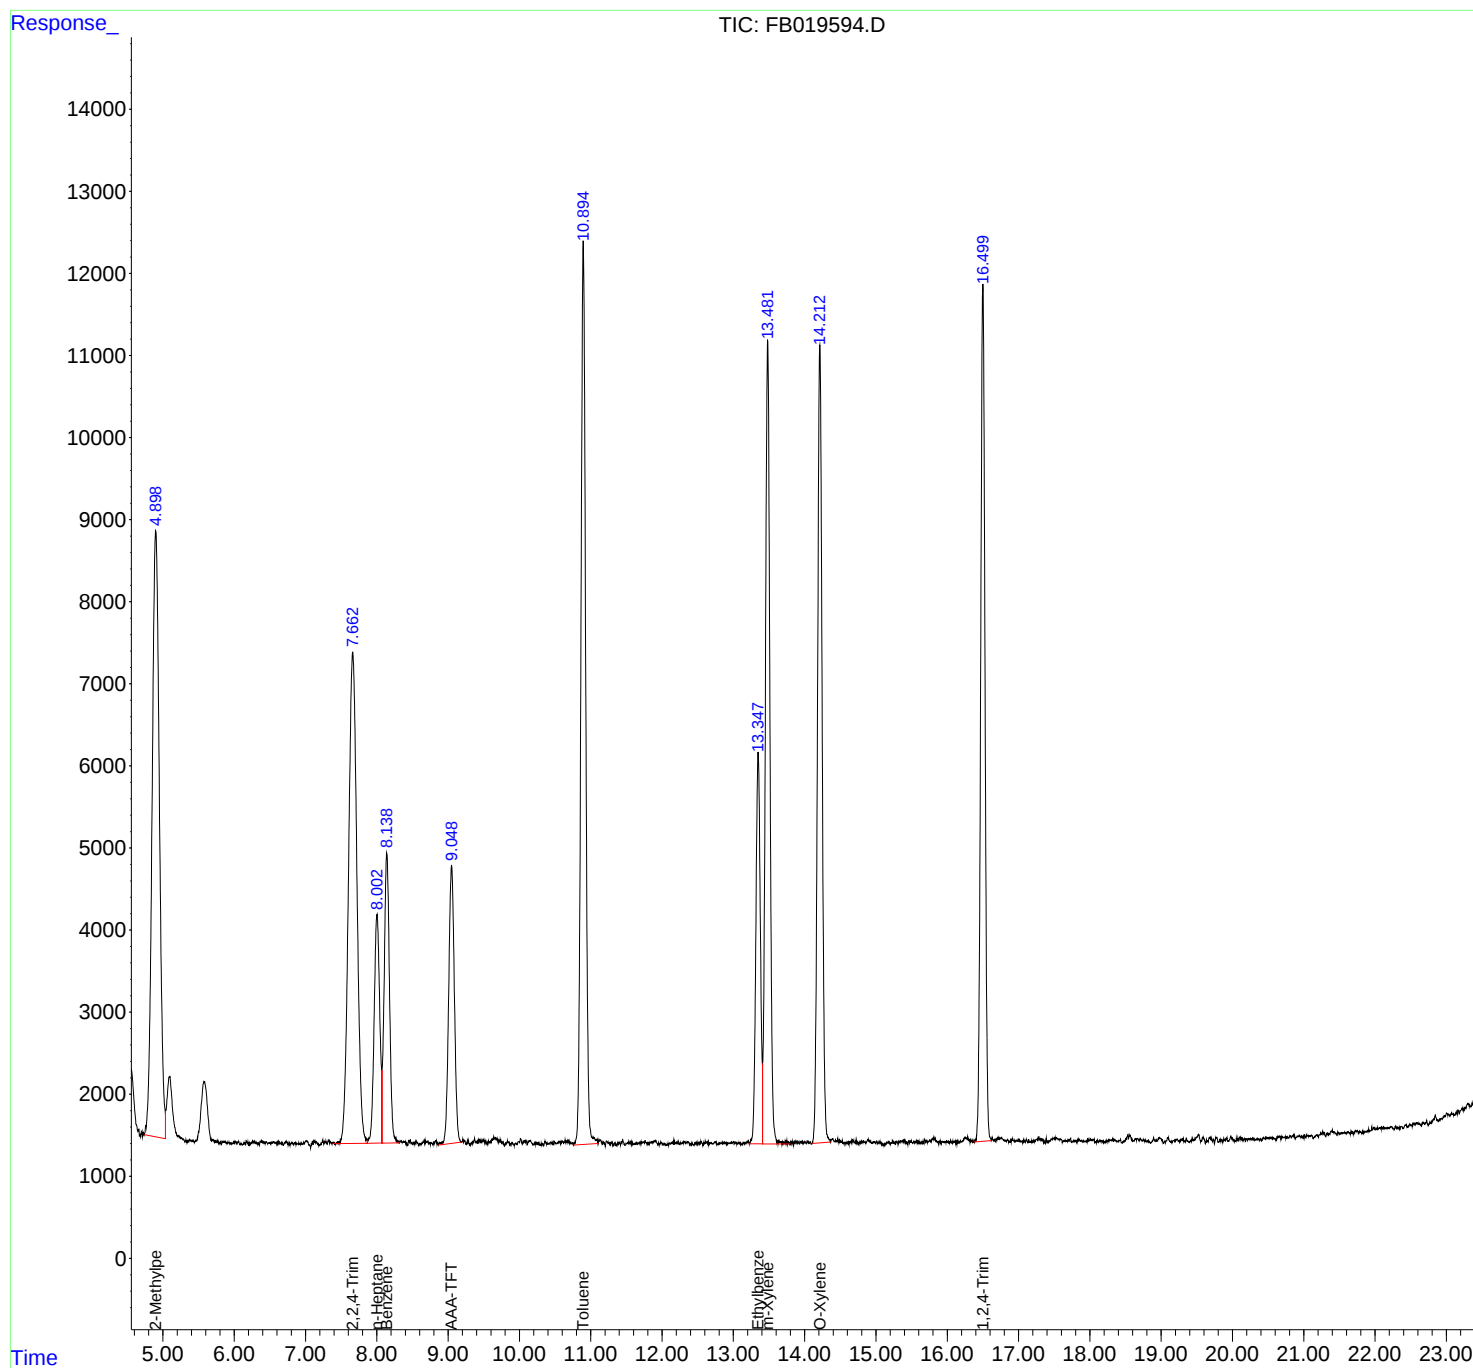

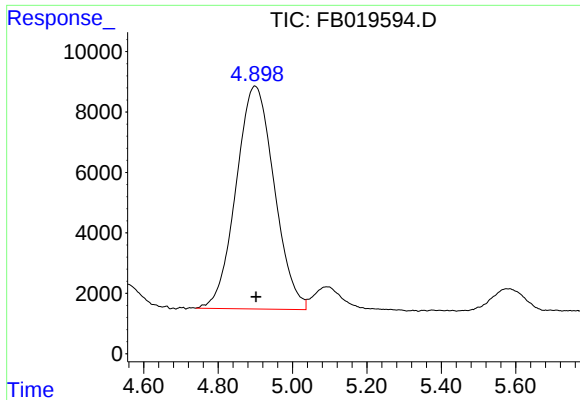


#1 2-Methylpentane

R.T.: 4.900 min
Delta R.T.: -0.002 min
Response: 525802
Conc: 30.37 ng/ml

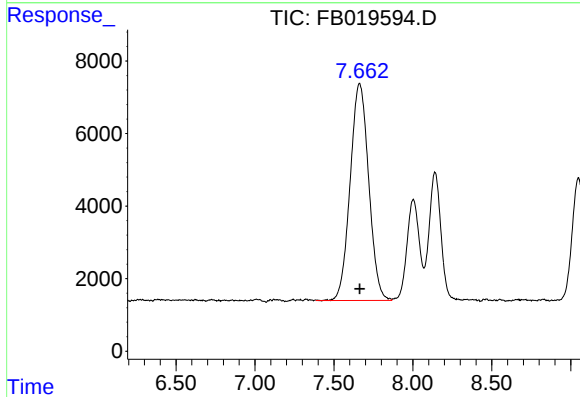


#2 2,2,4-Trimethylpentane

R.T.: 7.662 min
Delta R.T.: -0.002 min
Response: 487673
Conc: 29.41 ng/ml

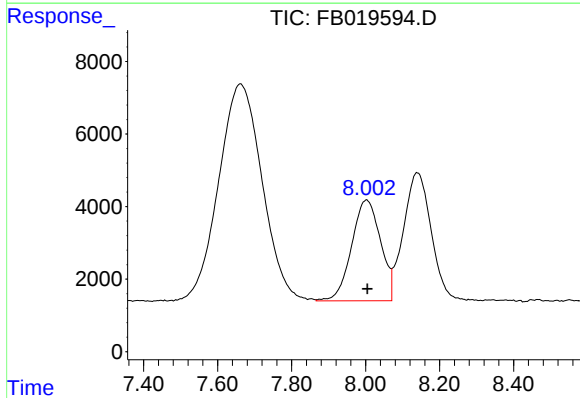


#3 n-Heptane

R.T.: 8.003 min
Delta R.T.: -0.002 min
Response: 150937
Conc: 9.37 ng/ml

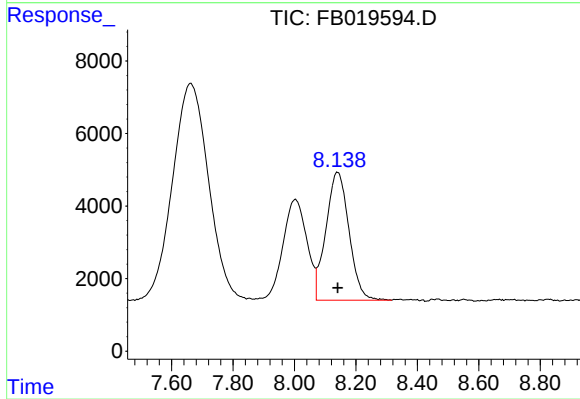


#4 Benzene

R.T.: 8.140 min
Delta R.T.: 0.000 min
Response: 184140
Conc: 9.76 ng/ml

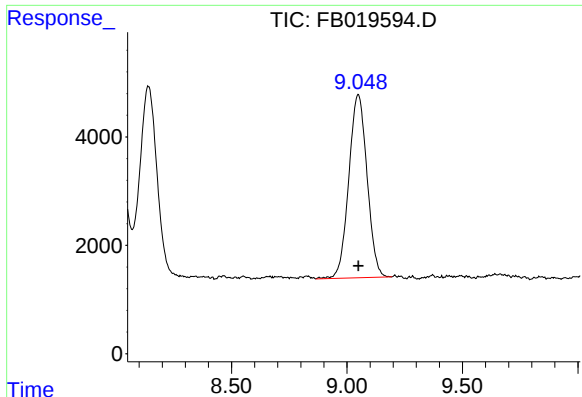


#5 AAA-TFT

R.T.: 9.049 min
Delta R.T.: 0.000 min
Response: 185686
Conc: 15.88 ng/ml

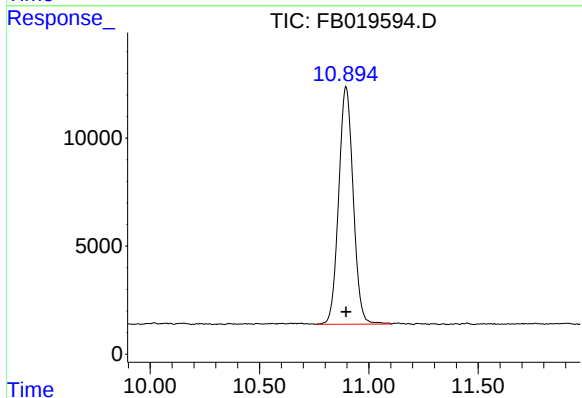


#6 Toluene

R.T.: 10.896 min
Delta R.T.: 0.000 min
Response: 507044
Conc: 28.99 ng/ml

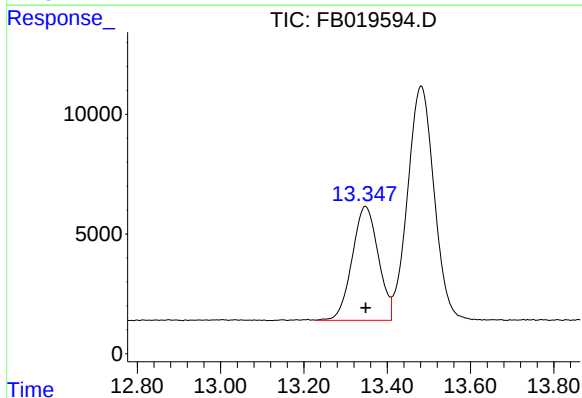


#7 Ethylbenzene

R.T.: 13.348 min
Delta R.T.: 0.000 min
Response: 206991
Conc: 9.43 ng/ml

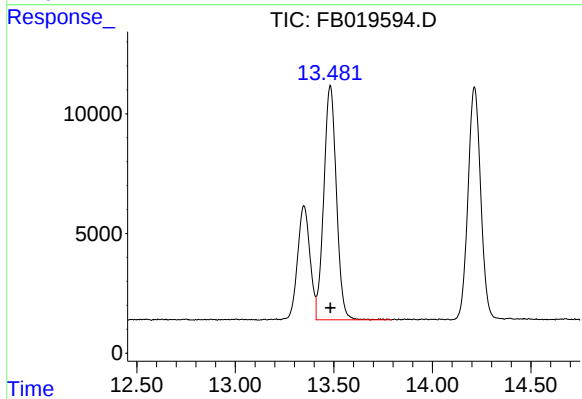


#8 m-Xylene

R.T.: 13.482 min
Delta R.T.: 0.000 min
Response: 435452
Conc: 19.03 ng/ml

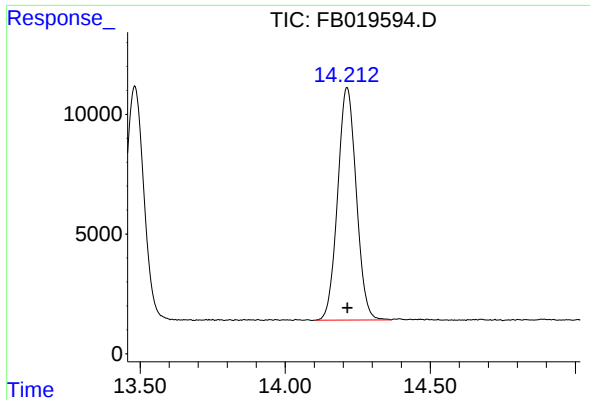

#9 O-Xylene

R.T.: 14.214 min
Delta R.T.: 0.000 min
Response: 432785
Conc: 19.38 ng/ml

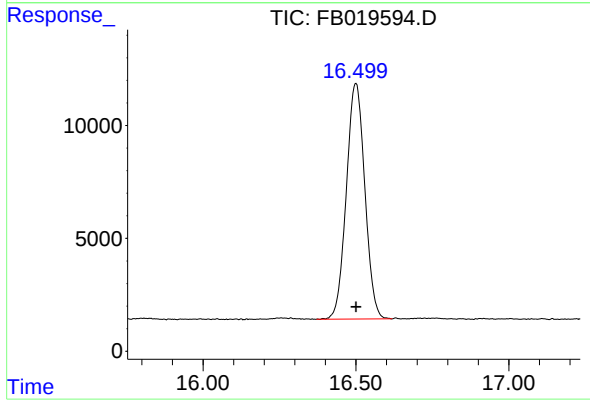

#10 1,2,4-Trimethylbenzene

R.T.: 16.500 min
Delta R.T.: 0.000 min
Response: 438609
Conc: 18.93 ng/ml