

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013020\
 Data File : FB023579.D
 Signal(s) : FID2B.CH
 Acq On : 30 Jan 2020 10:36
 Operator : DD/AJ
 Sample : VBF0130W1
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jan 31 00:33:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
 Quant Title :
 QLast Update : Thu Jan 16 11:42:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	488554	20.568 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.684	14913	0.472 ng/ml
2) t 2,2,4-Trimethylpentane	7.404	1914	0.056 ng/ml
3) t n-Heptane	7.761	801	0.024 ng/ml
6) t Toluene	10.628	6633	0.168 ng/ml
7) t Ethylbenzene	13.056	747	0.020 ng/ml
8) t m-Xylene	13.192	3680	0.103 ng/ml
9) t O-Xylene	13.926	2091	0.061 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	6249	0.214 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013020\
Data File : FB023579.D
Signal(s) : FID2B.CH
Acq On : 30 Jan 2020 10:36
Operator : DD/AJ
Sample : VBF0130W1
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 31 00:33:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
Quant Title :
QLast Update : Thu Jan 16 11:42:55 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

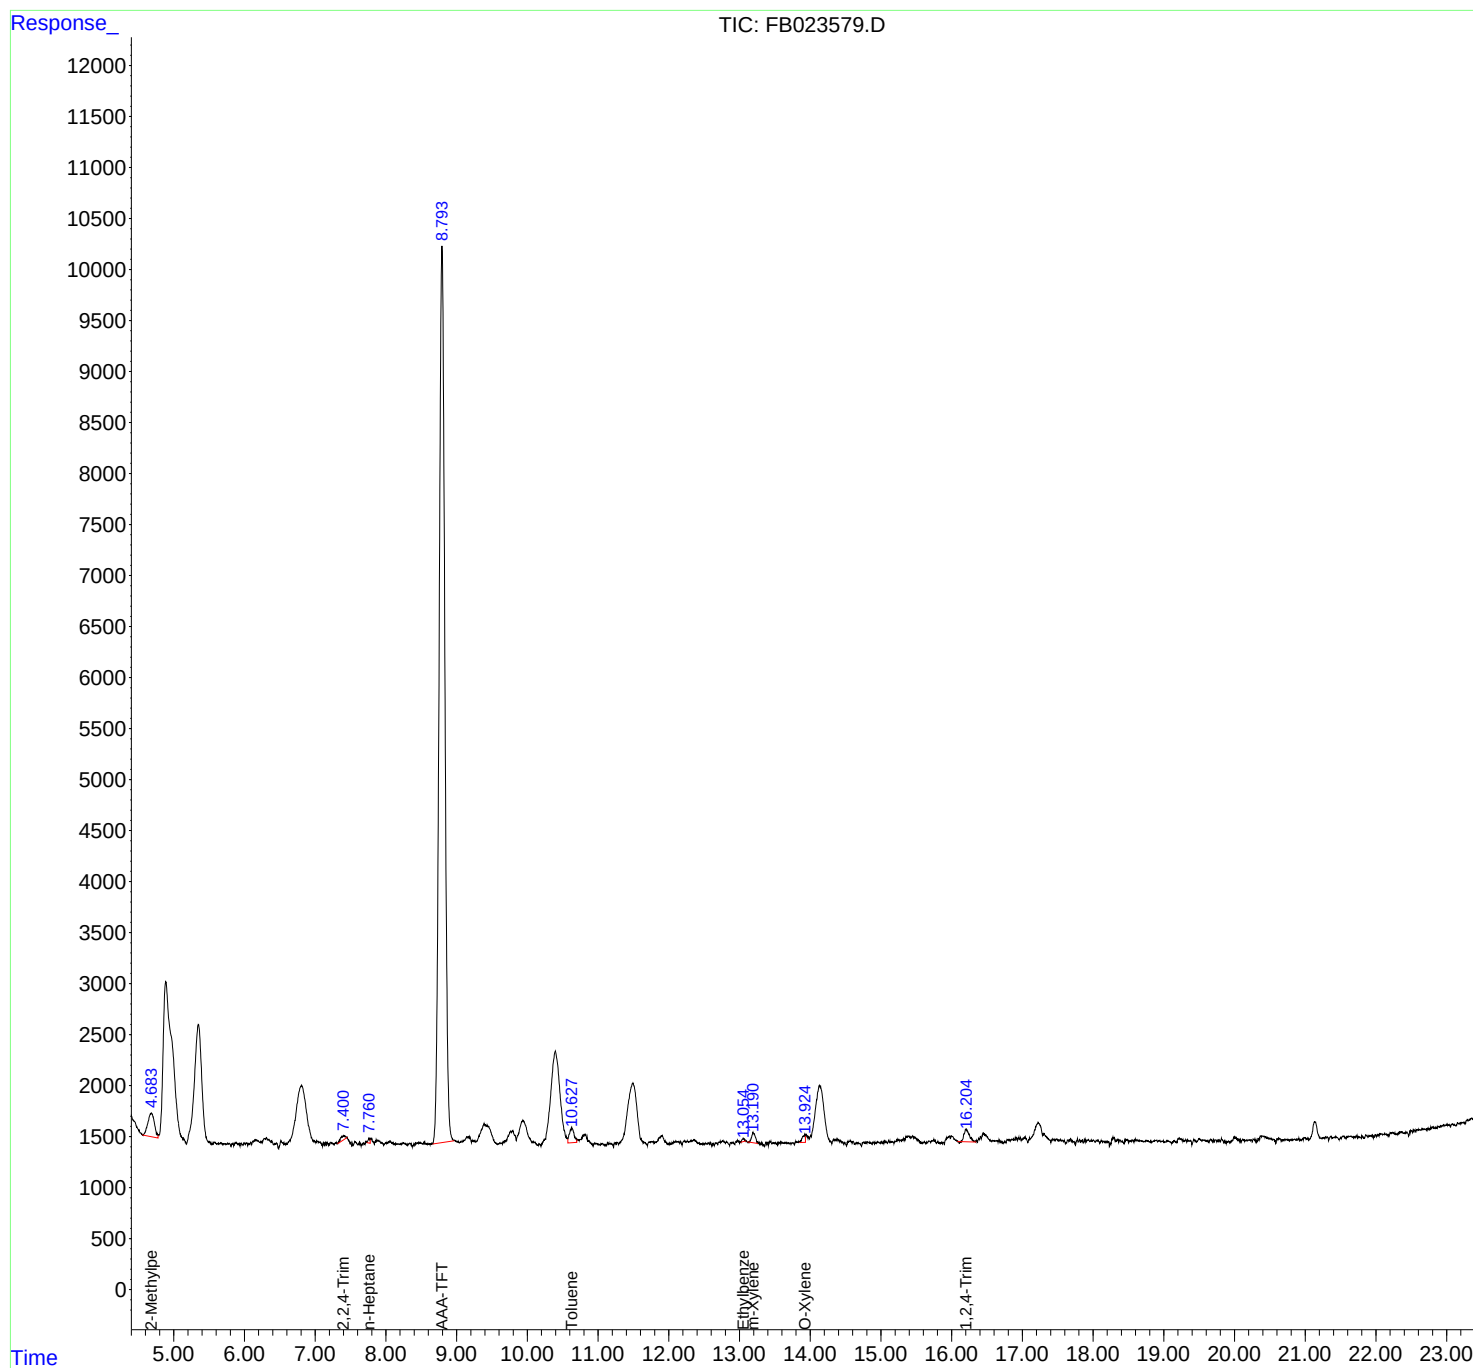


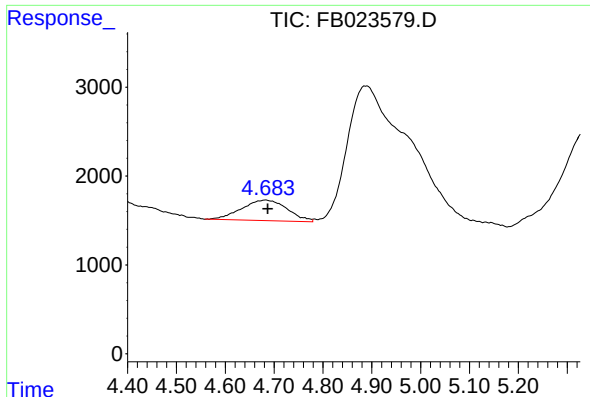

#1 2-Methylpentane


R.T.: 4.684 min
Delta R.T.: -0.003 min
Response: 14913
Conc: 0.47 ng/ml

Instrument :
FID_B
ClientSampleId :

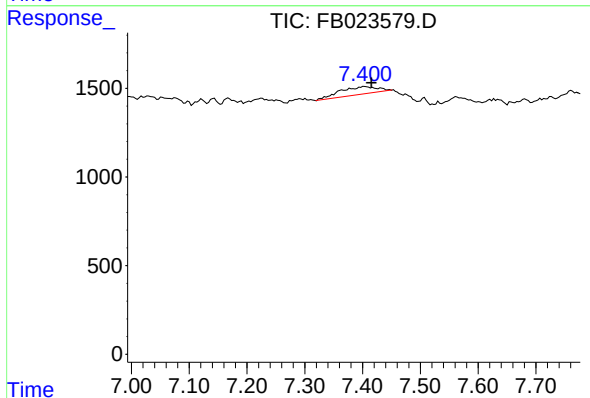


#2 2,2,4-Trimethylpentane

R.T.: 7.404 min
Delta R.T.: -0.012 min
Response: 1914
Conc: 0.06 ng/ml

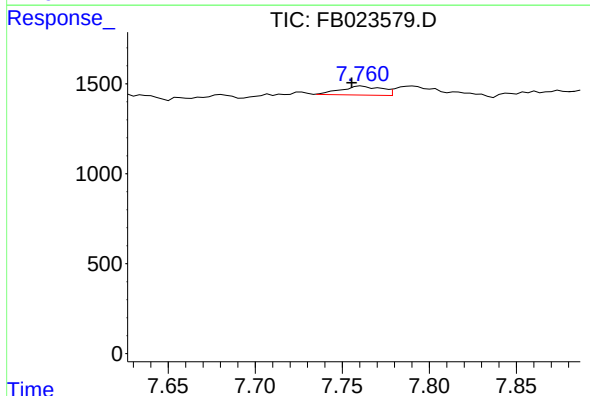


#3 n-Heptane

R.T.: 7.761 min
Delta R.T.: 0.006 min
Response: 801
Conc: 0.02 ng/ml

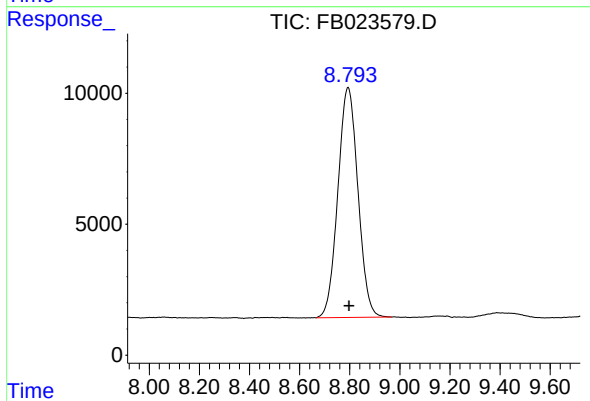

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: -0.003 min
Response: 488554
Conc: 20.57 ng/ml

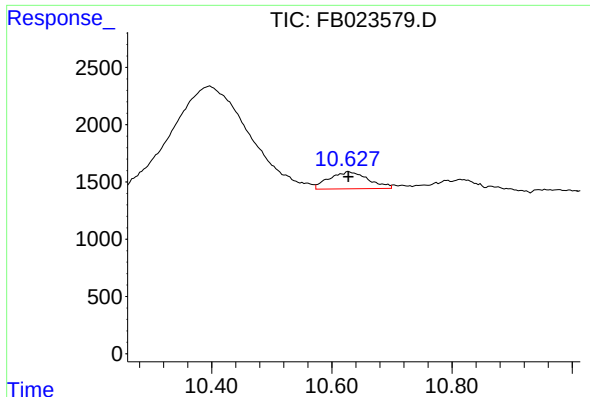

#6 Toluene


R.T.: 10.628 min
Delta R.T.: 0.000 min
Response: 6633
Conc: 0.17 ng/ml

Instrument :
FID_B
ClientSampleId :

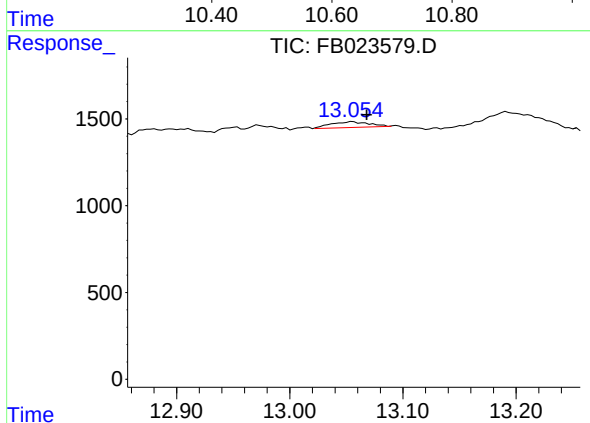


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: -0.012 min
Response: 747
Conc: 0.02 ng/ml

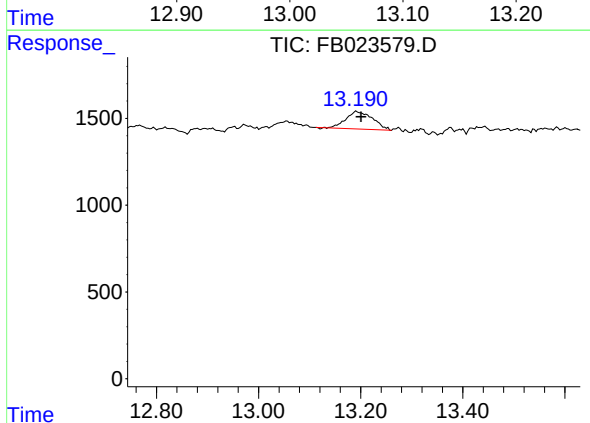


#8 m-Xylene

R.T.: 13.192 min
Delta R.T.: -0.009 min
Response: 3680
Conc: 0.10 ng/ml

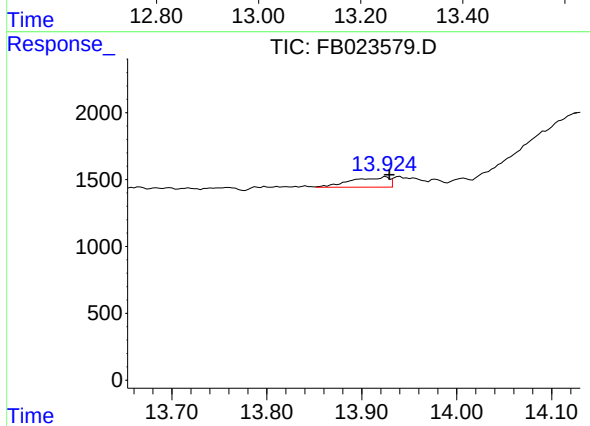

#9 O-Xylene

R.T.: 13.926 min
Delta R.T.: -0.003 min
Response: 2091
Conc: 0.06 ng/ml

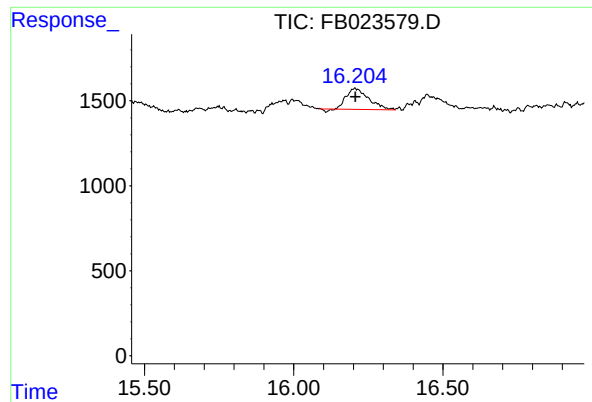

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: 0.000 min
Response: 6249
Conc: 0.21 ng/ml

Instrument :
FID_B
ClientSampleId :