

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013020\
 Data File : FB023581.D
 Signal(s) : FID2B.CH
 Acq On : 30 Jan 2020 12:00
 Operator : DD/AJ
 Sample : L1004-17
 Misc : 5.08g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jan 31 00:34:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
 Quant Title :
 QLast Update : Thu Jan 16 11:42:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	486086	20.464 ng/ml
Target Compounds			
6) t Toluene	10.624	31920	0.808 ng/ml
7) t Ethylbenzene	13.069	16395	0.439 ng/ml
8) t m-Xylene	13.195	99382	2.795 ng/ml
9) t O-Xylene	13.924	30598	0.886 ng/ml
10) t 1,2,4-Trimethylbenzene	16.211	24267	0.830 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013020\
Data File : FB023581.D
Signal(s) : FID2B.CH
Acq On : 30 Jan 2020 12:00
Operator : DD/AJ
Sample : L1004-17
Misc : 5.08g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 31 00:34:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
Quant Title :
QLast Update : Thu Jan 16 11:42:55 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

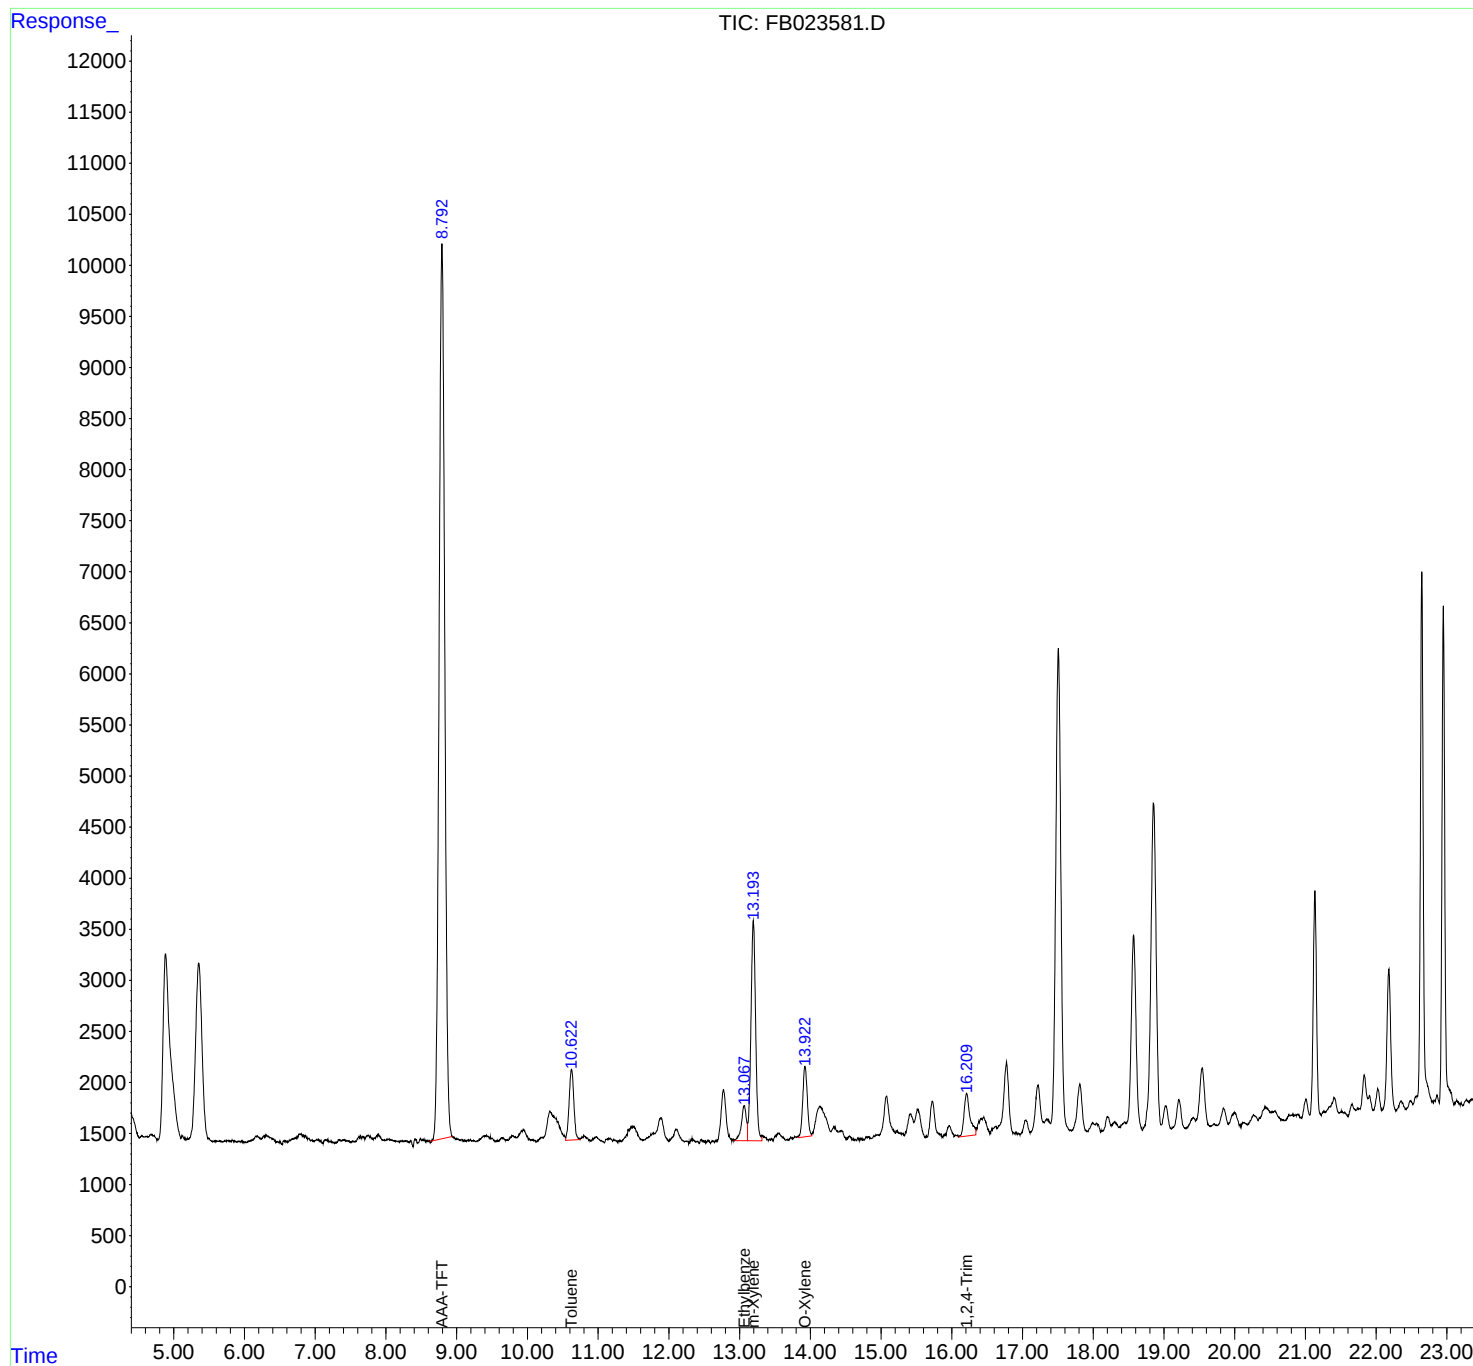


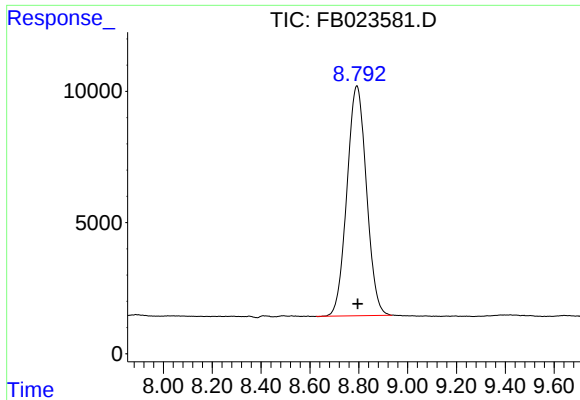

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: -0.004 min
Response: 486086
Conc: 20.46 ng/ml

Instrument :
FID_B
ClientSampleId :

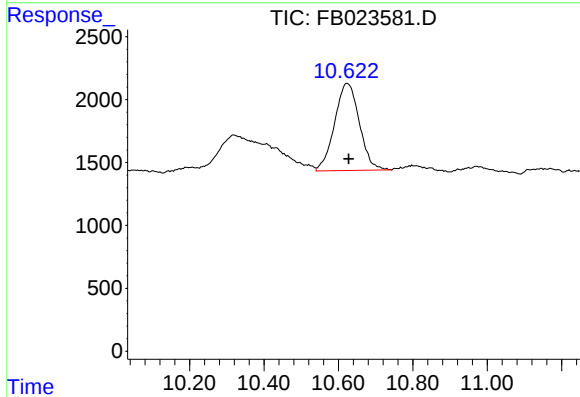


#6 Toluene

R.T.: 10.624 min
Delta R.T.: -0.004 min
Response: 31920
Conc: 0.81 ng/ml

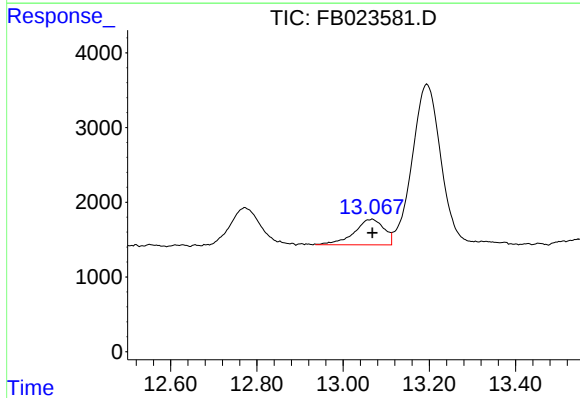


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: 0.000 min
Response: 16395
Conc: 0.44 ng/ml

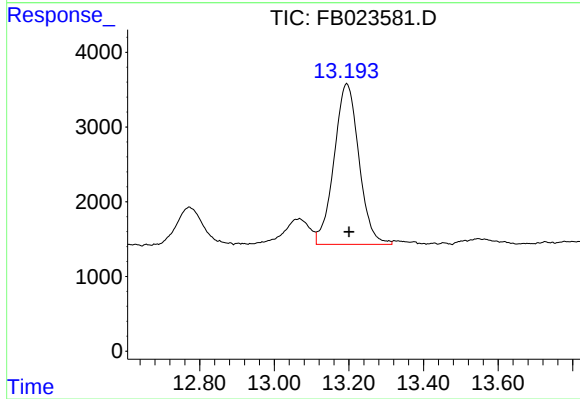

#8 m-Xylene


R.T.: 13.195 min
Delta R.T.: -0.006 min
Response: 99382
Conc: 2.79 ng/ml

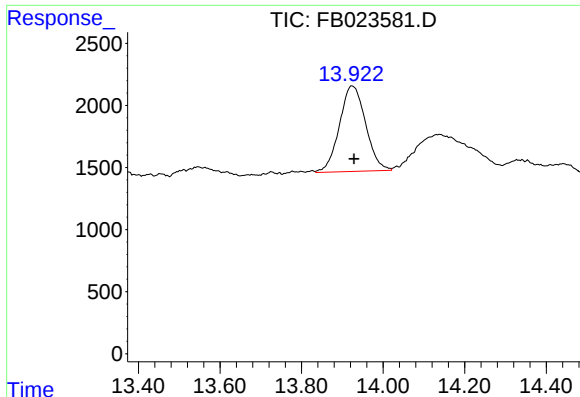

#9 O-Xylene

R.T.: 13.924 min
Delta R.T.: -0.004 min
Response: 30598
Conc: 0.89 ng/ml

Instrument :
FID_B
ClientSampleId :

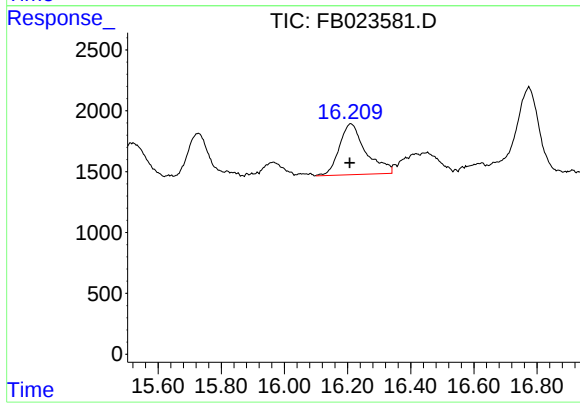

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min
Delta R.T.: 0.004 min
Response: 24267
Conc: 0.83 ng/ml