

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013020\
 Data File : FB023583.D
 Signal(s) : FID2B.CH
 Acq On : 30 Jan 2020 13:01
 Operator : DD/AJ
 Sample : L1014-12MS
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jan 31 00:34:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
 Quant Title :
 QLast Update : Thu Jan 16 11:42:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	485957	20.458 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.686	648282	20.515 ng/ml
2) t 2,2,4-Trimethylpentane	7.413	492780	14.513 ng/ml
3) t n-Heptane	7.753	166016	4.958 ng/ml
4) t Benzene	7.888	385753	9.446 ng/ml
6) t Toluene	10.625	1101947	27.884 ng/ml
7) t Ethylbenzene	13.065	311346	8.336 ng/ml
8) t m-Xylene	13.198	594474	16.717 ng/ml
9) t O-Xylene	13.926	575671	16.660 ng/ml
10) t 1,2,4-Trimethylbenzene	16.205	461874	15.796 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013020\
Data File : FB023583.D
Signal(s) : FID2B.CH
Acq On : 30 Jan 2020 13:01
Operator : DD/AJ
Sample : L1014-12MS
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 31 00:34:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
Quant Title :
QLast Update : Thu Jan 16 11:42:55 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

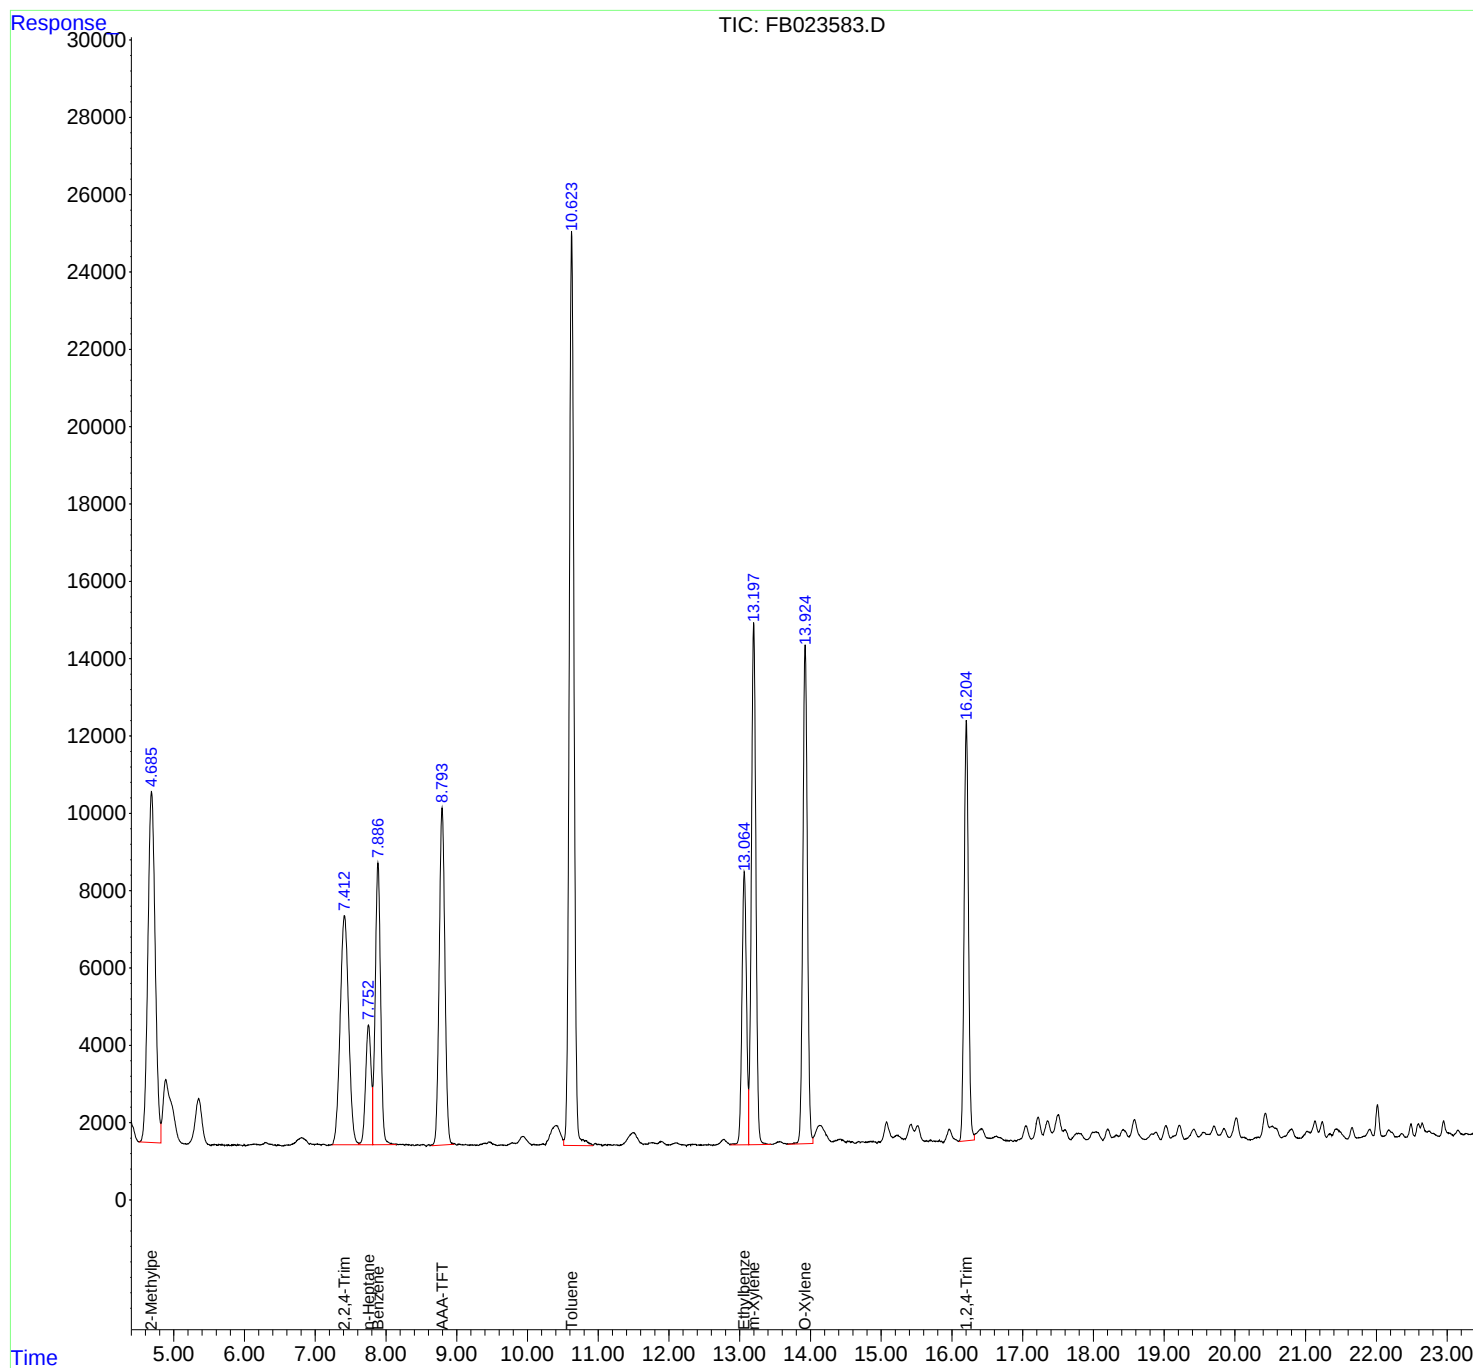


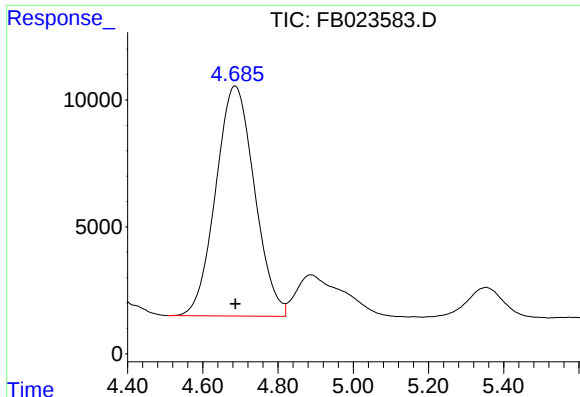

#1 2-Methylpentane


R.T.: 4.686 min
Delta R.T.: 0.000 min
Response: 648282
Conc: 20.51 ng/ml

Instrument :
FID_B
ClientSampleId :

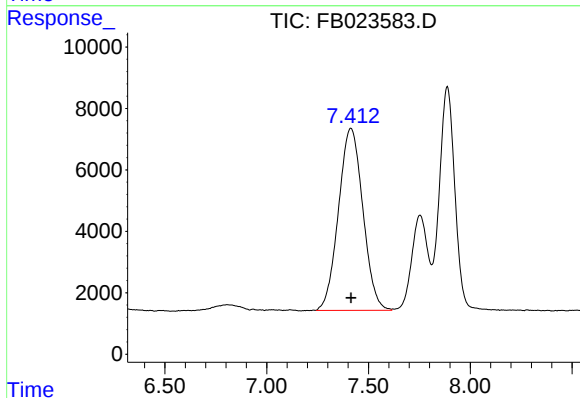


#2 2,2,4-Trimethylpentane

R.T.: 7.413 min
Delta R.T.: -0.002 min
Response: 492780
Conc: 14.51 ng/ml

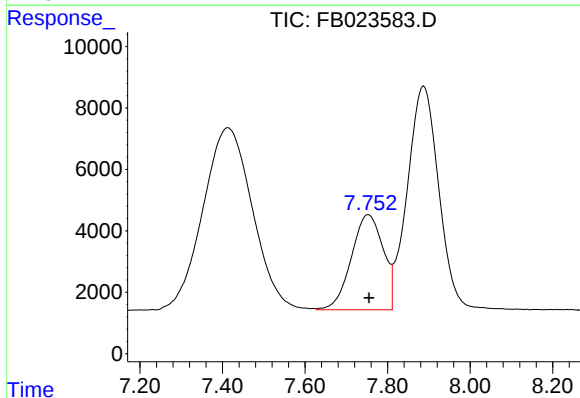


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: -0.002 min
Response: 166016
Conc: 4.96 ng/ml

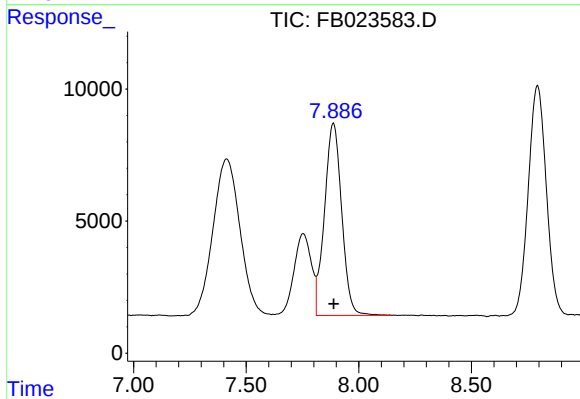

#4 Benzene


R.T.: 7.888 min
Delta R.T.: -0.002 min
Response: 385753
Conc: 9.45 ng/ml

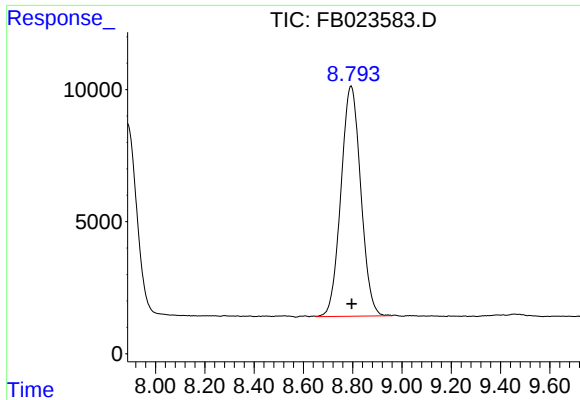

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: -0.003 min
Response: 485957
Conc: 20.46 ng/ml

Instrument :
FID_B
ClientSampleId :

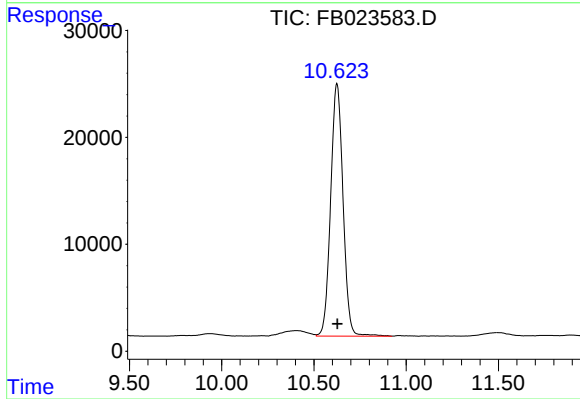


#6 Toluene

R.T.: 10.625 min
Delta R.T.: -0.002 min
Response: 1101947
Conc: 27.88 ng/ml

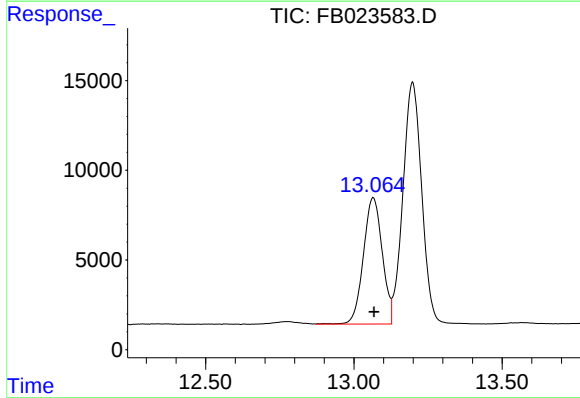


#7 Ethylbenzene

R.T.: 13.065 min
Delta R.T.: -0.003 min
Response: 311346
Conc: 8.34 ng/ml

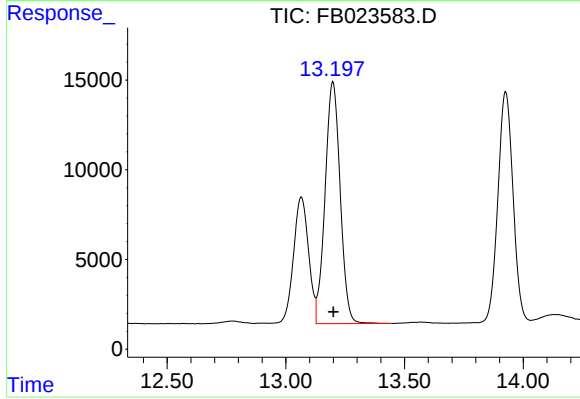

#8 m-Xylene


R.T.: 13.198 min
Delta R.T.: -0.002 min
Response: 594474
Conc: 16.72 ng/ml

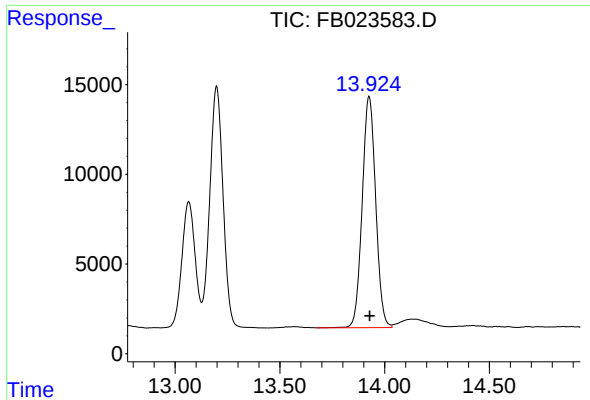

#9 O-Xylene

R.T.: 13.926 min
Delta R.T.: -0.003 min
Response: 575671
Conc: 16.66 ng/ml

Instrument :
FID_B
ClientSampleId :

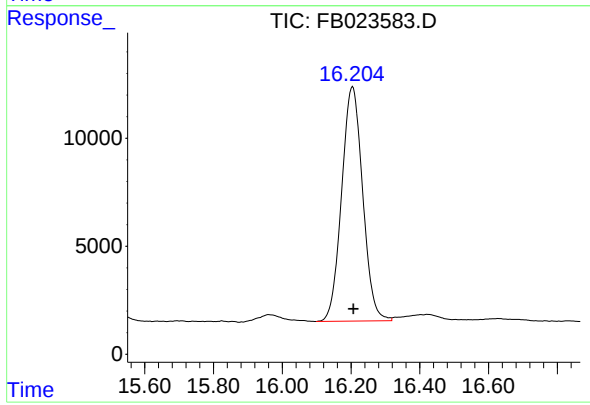

#10 1,2,4-Trimethylbenzene

R.T.: 16.205 min
Delta R.T.: -0.002 min
Response: 461874
Conc: 15.80 ng/ml