

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013020\
 Data File : FB023584.D
 Signal(s) : FID2B.CH
 Acq On : 30 Jan 2020 13:31
 Operator : DD/AJ
 Sample : L1014-12MSD
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 OR-03-012920MSD

Integration File: Calibration.e
 Quant Time: Jan 31 00:34:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
 Quant Title :
 QLast Update : Thu Jan 16 11:42:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	406153	17.099 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	531118	16.807 ng/ml
2) t 2,2,4-Trimethylpentane	7.412	408190	12.022 ng/ml
3) t n-Heptane	7.755	132843	3.967 ng/ml
4) t Benzene	7.888	345969	8.472 ng/ml
6) t Toluene	10.626	989998	25.052 ng/ml
7) t Ethylbenzene	13.065	292344	7.828 ng/ml
8) t m-Xylene	13.198	554679	15.598 ng/ml
9) t O-Xylene	13.926	544575	15.760 ng/ml
10) t 1,2,4-Trimethylbenzene	16.205	425204	14.541 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013020\
Data File : FB023584.D
Signal(s) : FID2B.CH
Acq On : 30 Jan 2020 13:31
Operator : DD/AJ
Sample : L1014-12MSD
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
OR-03-012920MSD

Integration File: Calibration.e
Quant Time: Jan 31 00:34:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
Quant Title :
QLast Update : Thu Jan 16 11:42:55 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

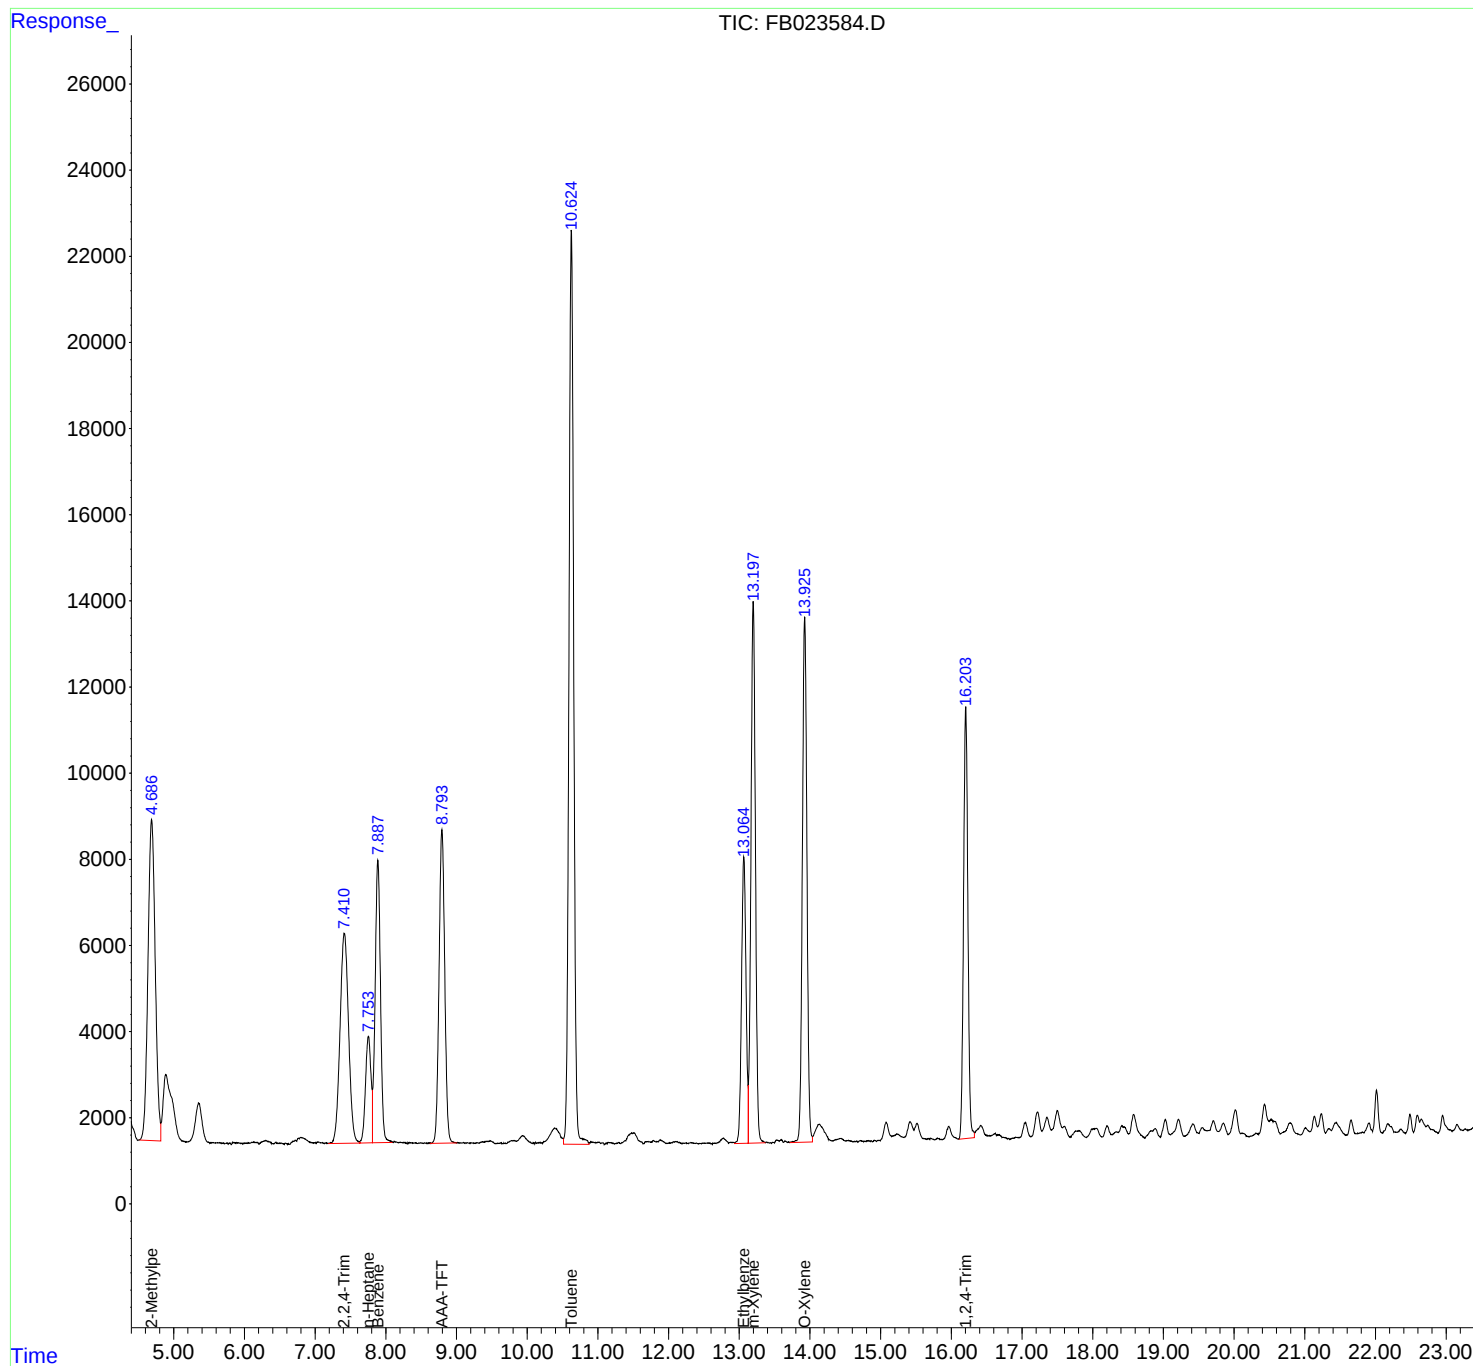


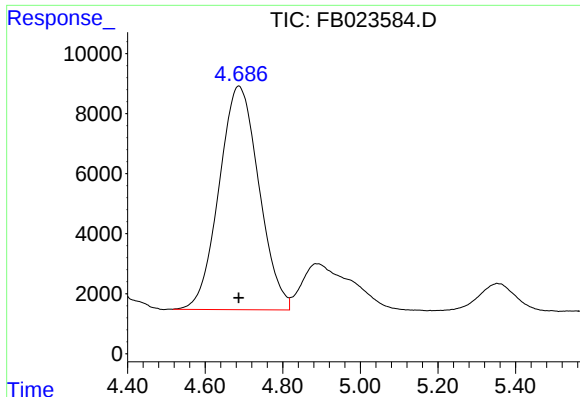

#1 2-Methylpentane


R.T.: 4.688 min
Delta R.T.: 0.000 min
Response: 531118
Conc: 16.81 ng/ml

Instrument :
FID_B
ClientSampleId :
OR-03-012920MSD

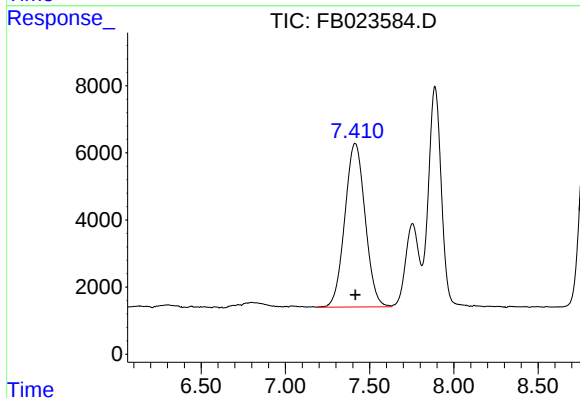


#2 2,2,4-Trimethylpentane

R.T.: 7.412 min
Delta R.T.: -0.003 min
Response: 408190
Conc: 12.02 ng/ml

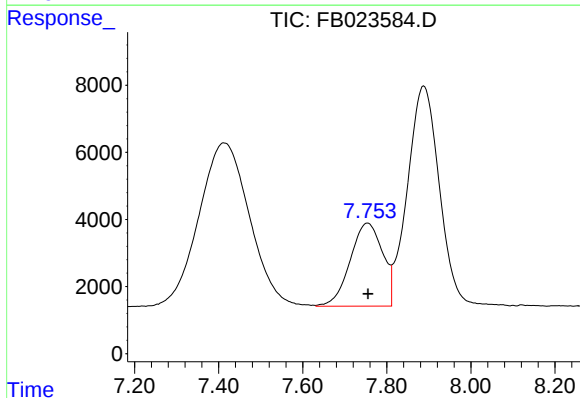


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.000 min
Response: 132843
Conc: 3.97 ng/ml

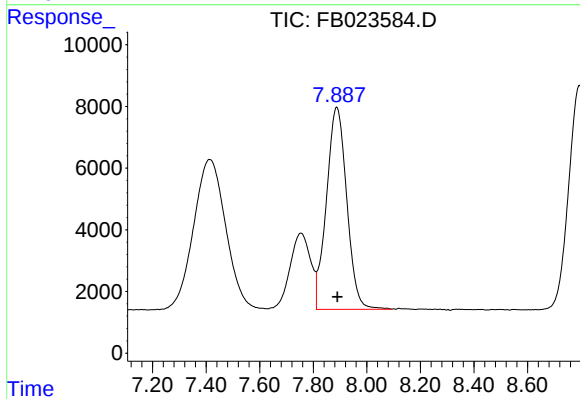

#4 Benzene


R.T.: 7.888 min
Delta R.T.: -0.001 min
Response: 345969
Conc: 8.47 ng/ml

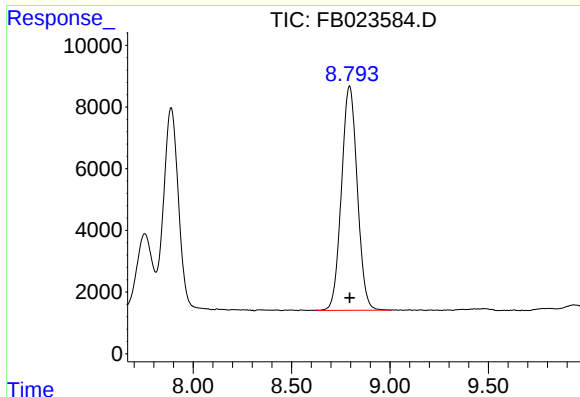

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: -0.002 min
Response: 406153
Conc: 17.10 ng/ml

Instrument :
FID_B
ClientSampleId :
OR-03-012920MSD

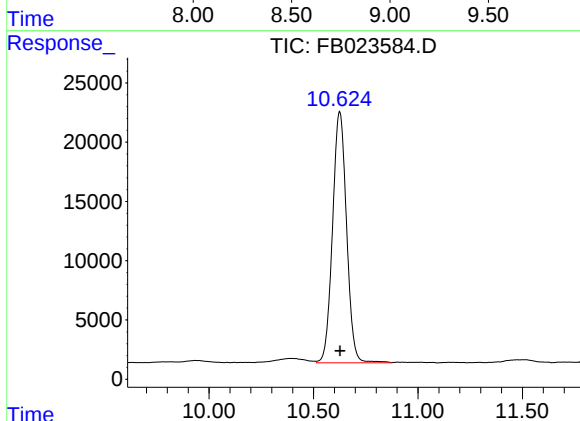


#6 Toluene

R.T.: 10.626 min
Delta R.T.: -0.002 min
Response: 989998
Conc: 25.05 ng/ml

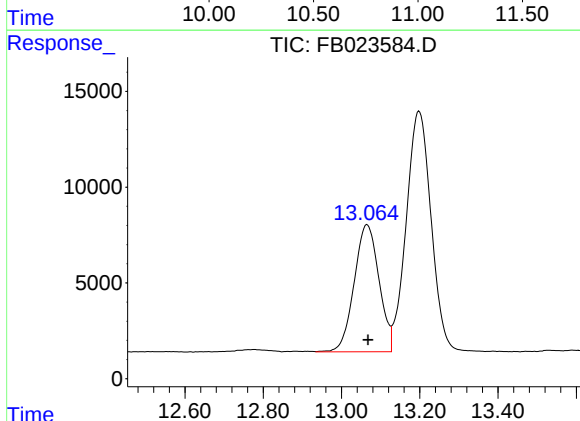


#7 Ethylbenzene

R.T.: 13.065 min
Delta R.T.: -0.003 min
Response: 292344
Conc: 7.83 ng/ml

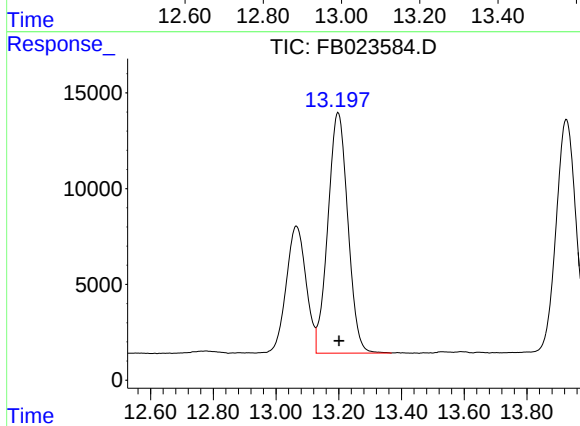

#8 m-Xylene


R.T.: 13.198 min
Delta R.T.: -0.002 min
Response: 554679
Conc: 15.60 ng/ml

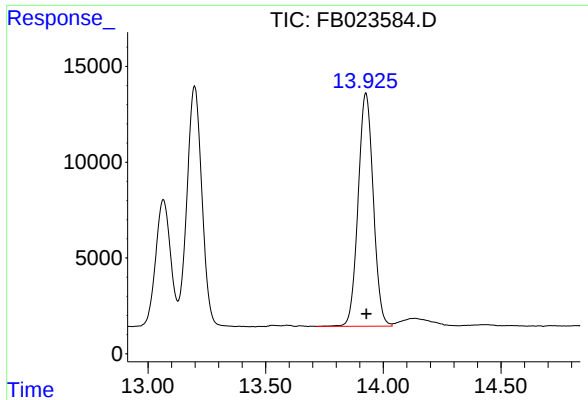

#9 O-Xylene

R.T.: 13.926 min
Delta R.T.: -0.003 min
Response: 544575
Conc: 15.76 ng/ml

Instrument :
FID_B
ClientSampleId :
OR-03-012920MSD

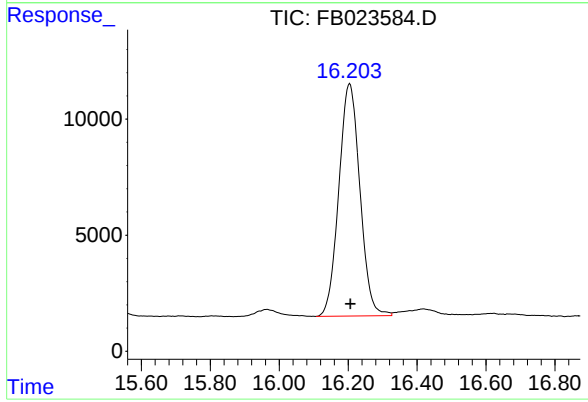

#10 1,2,4-Trimethylbenzene

R.T.: 16.205 min
Delta R.T.: -0.002 min
Response: 425204
Conc: 14.54 ng/ml