

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013020\
 Data File : FB023588.D
 Signal(s) : FID2B.CH
 Acq On : 30 Jan 2020 15:31
 Operator : DD/AJ
 Sample : L1161-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2020

Integration File: Calibration.e
 Quant Time: Jan 31 00:35:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
 Quant Title :
 QLast Update : Thu Jan 16 11:42:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	466981	19.659 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.684	53253	1.685 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	55567	1.637 ng/ml
3) t n-Heptane	7.756	16447	0.491 ng/ml
4) t Benzene	7.890	22030	0.539 ng/ml
6) t Toluene	10.628	69326	1.754 ng/ml
7) t Ethylbenzene	13.069	21378	0.572 ng/ml
8) t m-Xylene	13.200	41038	1.154 ng/ml
9) t O-Xylene	13.928	41458	1.200 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	39210	1.341 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013020\
Data File : FB023588.D
Signal(s) : FID2B.CH
Acq On : 30 Jan 2020 15:31
Operator : DD/AJ
Sample : L1161-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020

Integration File: Calibration.e
Quant Time: Jan 31 00:35:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
Quant Title :
QLast Update : Thu Jan 16 11:42:55 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

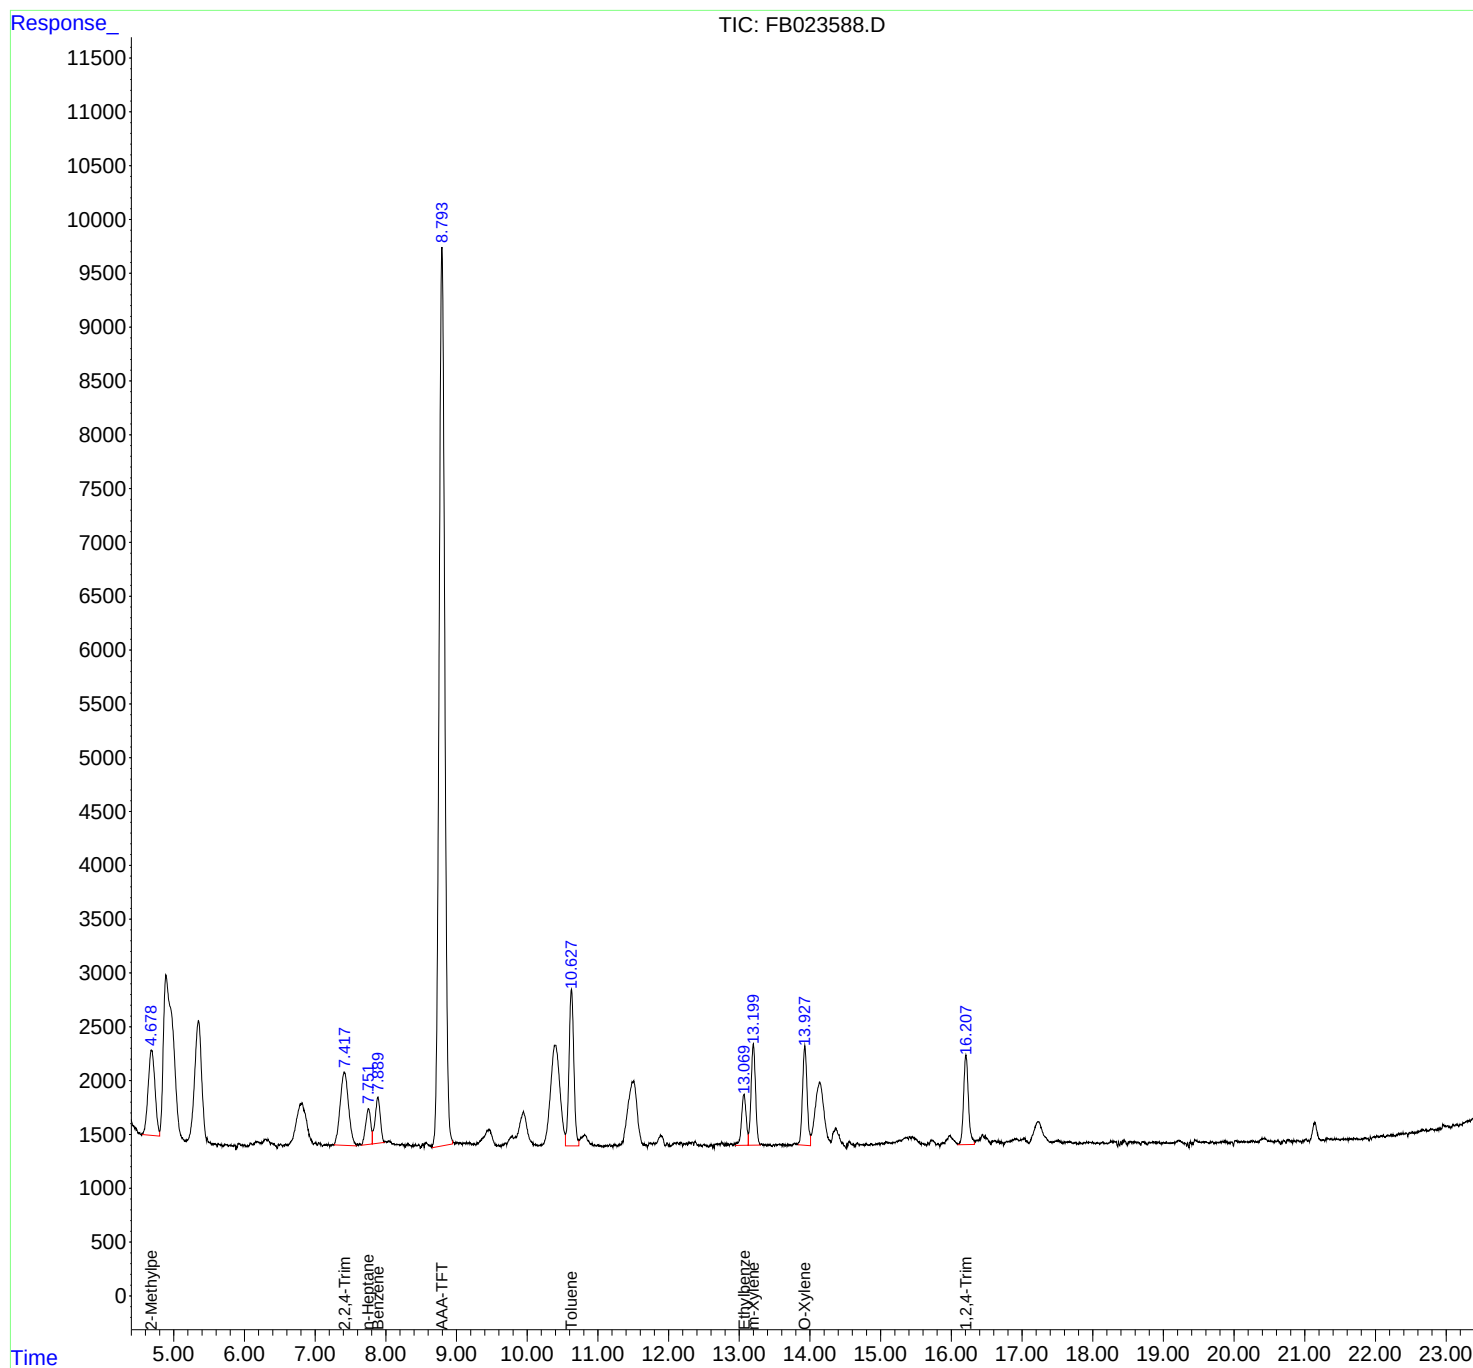


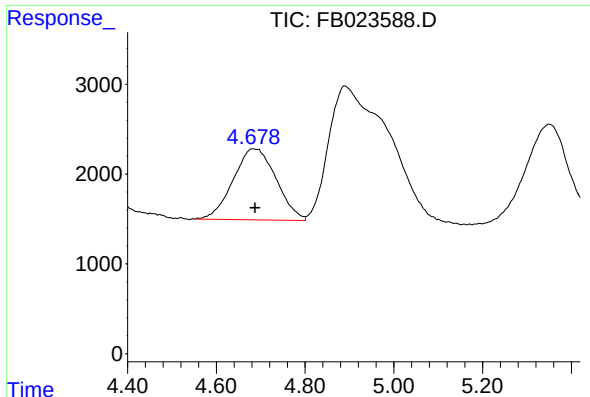

#1 2-Methylpentane


R.T.: 4.684 min
Delta R.T.: -0.003 min
Response: 53253
Conc: 1.69 ng/ml

Instrument :
FID_B
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020

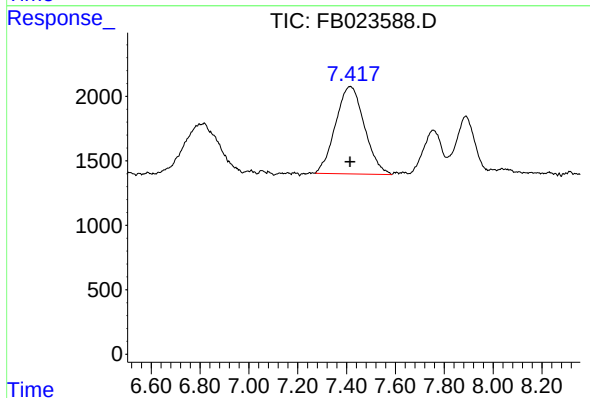


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.003 min
Response: 55567
Conc: 1.64 ng/ml

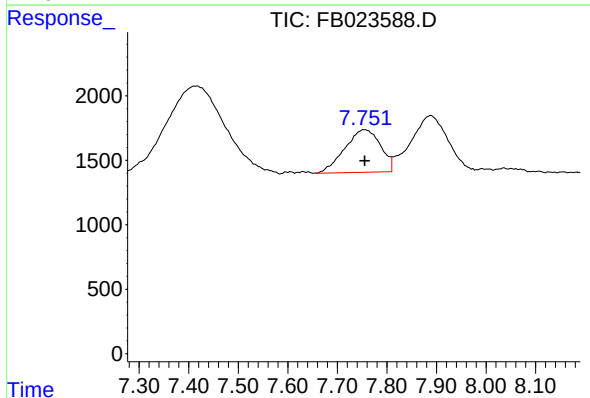


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: 0.000 min
Response: 16447
Conc: 0.49 ng/ml

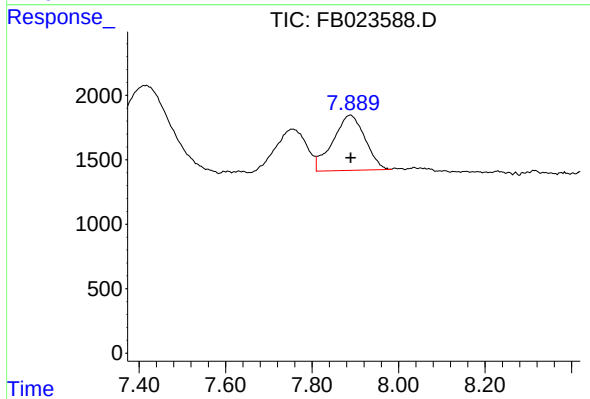

#4 Benzene


R.T.: 7.890 min
Delta R.T.: 0.000 min
Response: 22030
Conc: 0.54 ng/ml

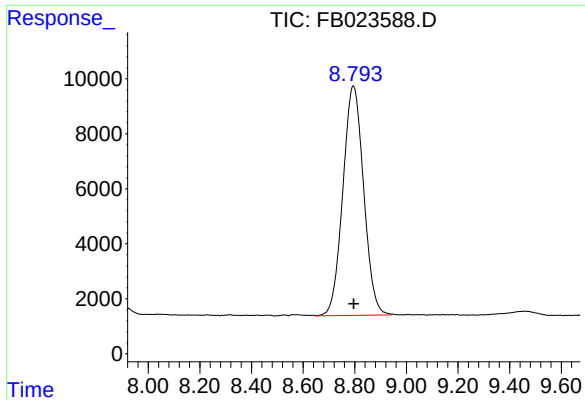

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: -0.002 min
Response: 466981
Conc: 19.66 ng/ml

Instrument :
FID_B
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020

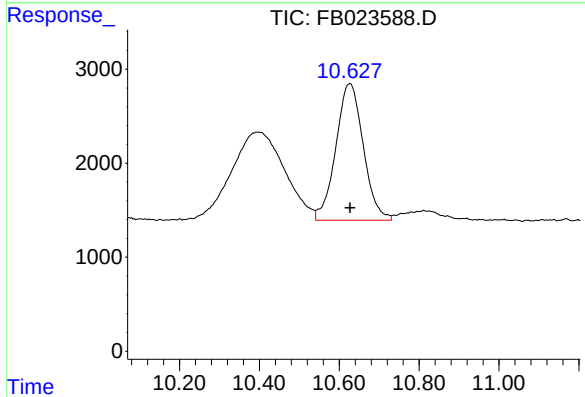


#6 Toluene

R.T.: 10.628 min
Delta R.T.: 0.000 min
Response: 69326
Conc: 1.75 ng/ml

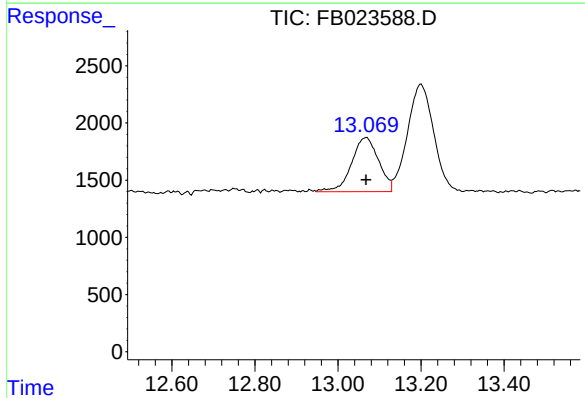


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: 0.000 min
Response: 21378
Conc: 0.57 ng/ml

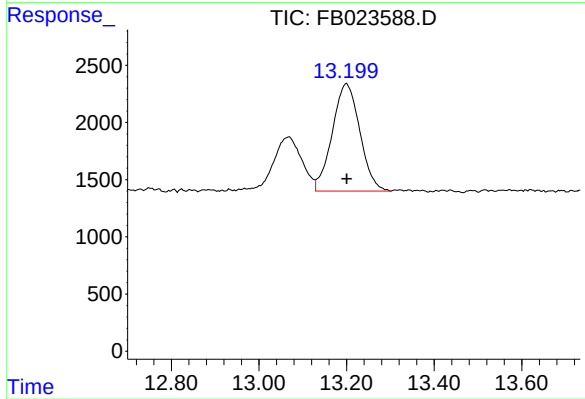

#8 m-Xylene


R.T.: 13.200 min
Delta R.T.: 0.000 min
Response: 41038
Conc: 1.15 ng/ml

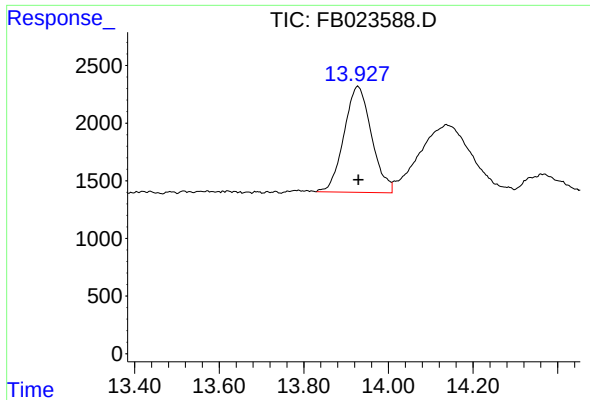

#9 O-Xylene

R.T.: 13.928 min
Delta R.T.: 0.000 min
Response: 41458
Conc: 1.20 ng/ml

Instrument :
FID_B
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020

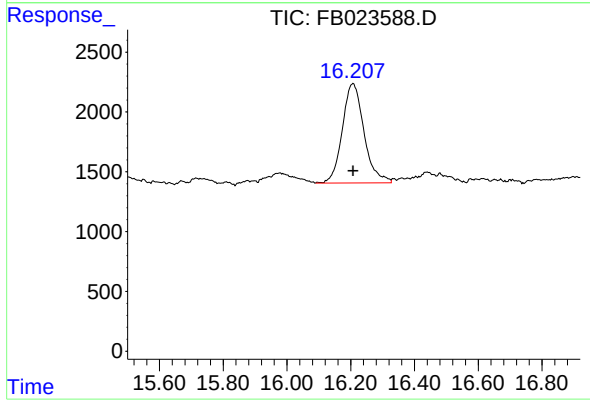

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: 0.001 min
Response: 39210
Conc: 1.34 ng/ml