

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013020\
 Data File : FB023589.D
 Signal(s) : FID2B.CH
 Acq On : 30 Jan 2020 16:01
 Operator : DD/AJ
 Sample : L1161-07
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2020

Integration File: Calibration.e
 Quant Time: Jan 31 00:35:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
 Quant Title :
 QLast Update : Thu Jan 16 11:42:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	480469	20.227 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	186050	5.888 ng/ml
2) t 2,2,4-Trimethylpentane	7.413	207718	6.118 ng/ml
3) t n-Heptane	7.755	64116	1.915 ng/ml
4) t Benzene	7.890	80693	1.976 ng/ml
6) t Toluene	10.627	245419	6.210 ng/ml
7) t Ethylbenzene	13.067	74131	1.985 ng/ml
8) t m-Xylene	13.199	145696	4.097 ng/ml
9) t O-Xylene	13.927	145148	4.201 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	123027	4.207 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013020\
Data File : FB023589.D
Signal(s) : FID2B.CH
Acq On : 30 Jan 2020 16:01
Operator : DD/AJ
Sample : L1161-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020

Integration File: Calibration.e
Quant Time: Jan 31 00:35:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
Quant Title :
QLast Update : Thu Jan 16 11:42:55 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

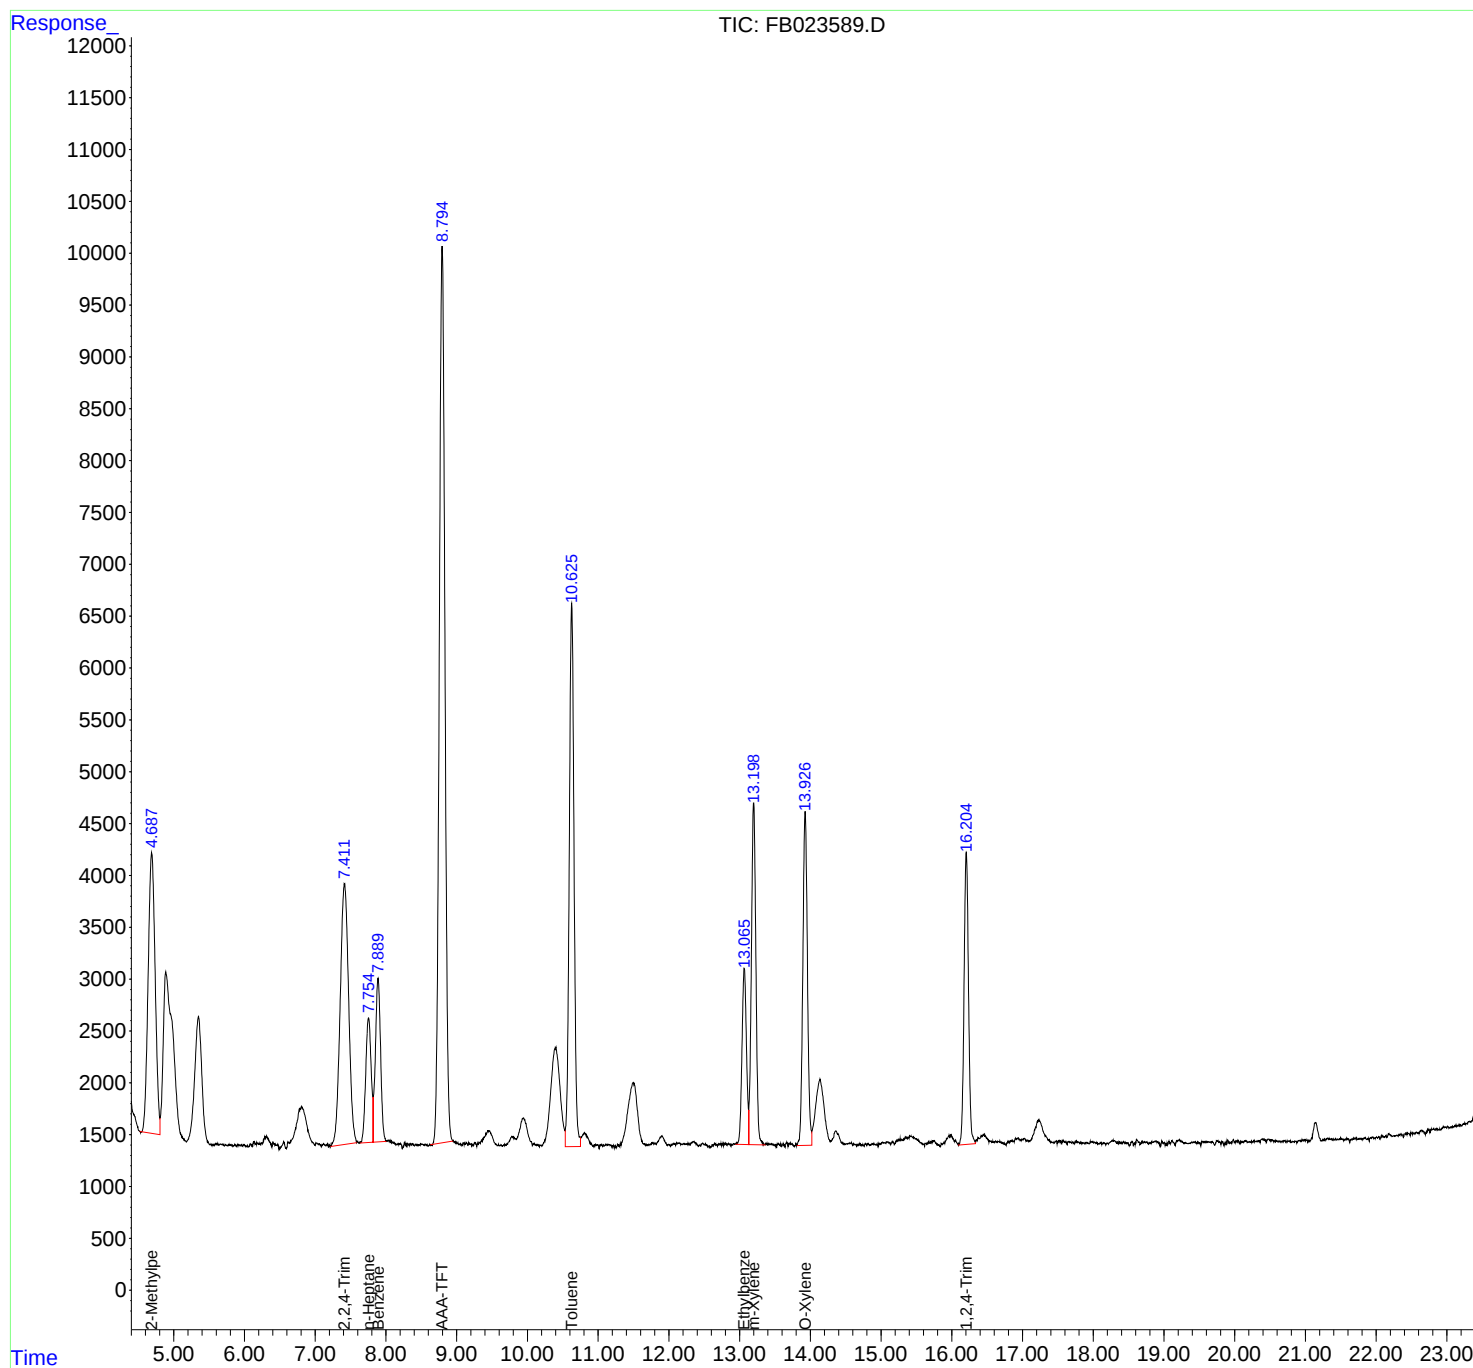


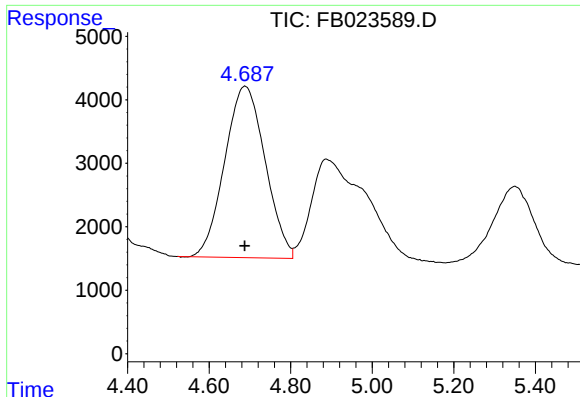

#1 2-Methylpentane


R.T.: 4.689 min
Delta R.T.: 0.002 min
Response: 186050
Conc: 5.89 ng/ml

Instrument :
FID_B
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020

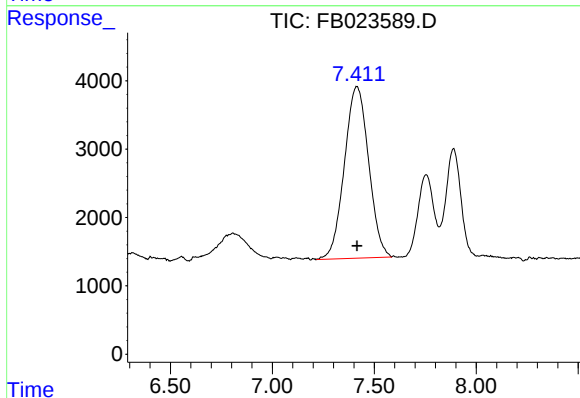


#2 2,2,4-Trimethylpentane

R.T.: 7.413 min
Delta R.T.: -0.003 min
Response: 207718
Conc: 6.12 ng/ml

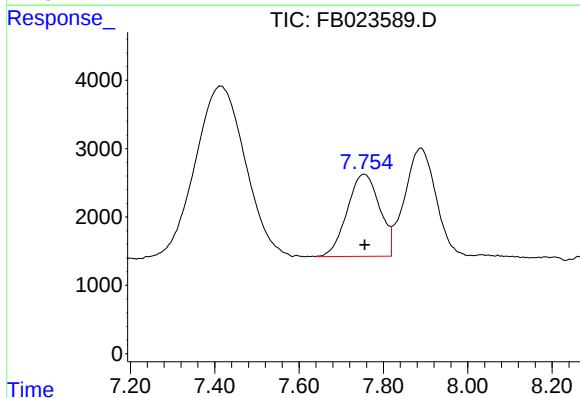


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.000 min
Response: 64116
Conc: 1.91 ng/ml

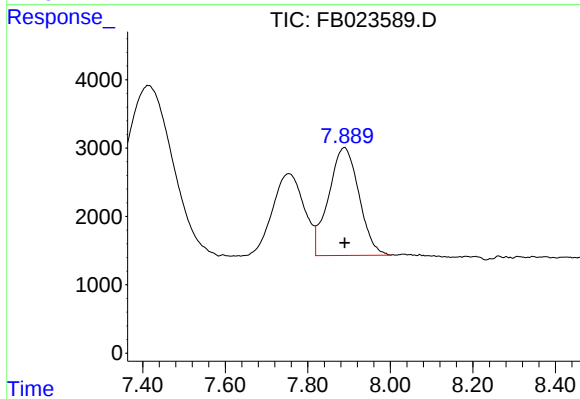

#4 Benzene


R.T.: 7.890 min
Delta R.T.: 0.000 min
Response: 80693
Conc: 1.98 ng/ml

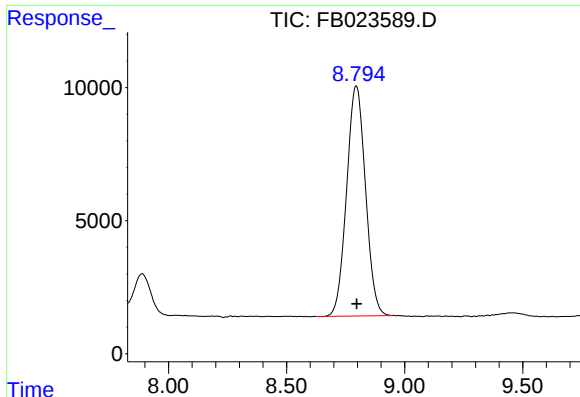

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: -0.001 min
Response: 480469
Conc: 20.23 ng/ml

Instrument :
FID_B
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020

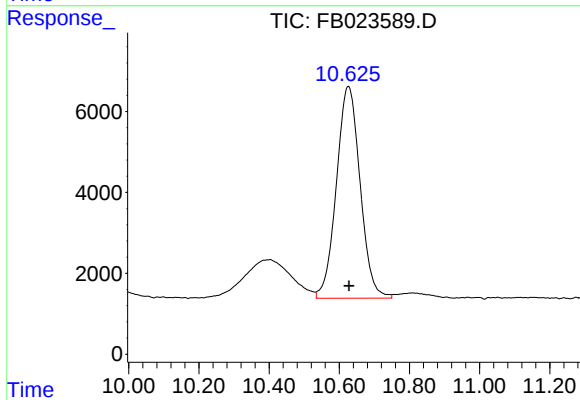


#6 Toluene

R.T.: 10.627 min
Delta R.T.: 0.000 min
Response: 245419
Conc: 6.21 ng/ml

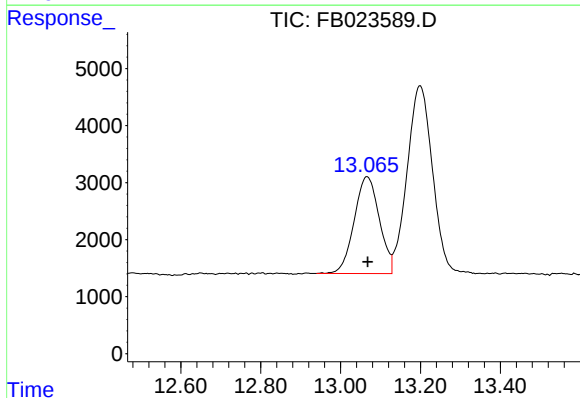


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: -0.001 min
Response: 74131
Conc: 1.98 ng/ml

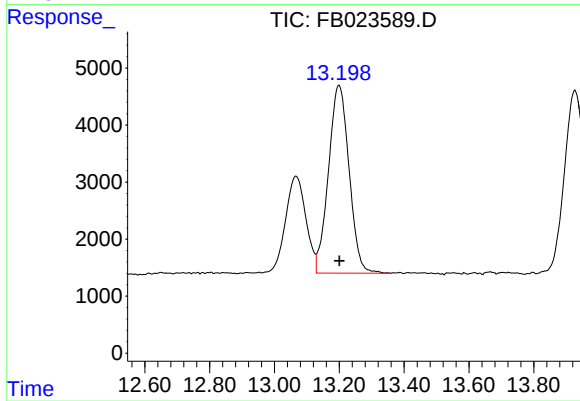

#8 m-Xylene


R.T.: 13.199 min
Delta R.T.: -0.001 min
Response: 145696
Conc: 4.10 ng/ml

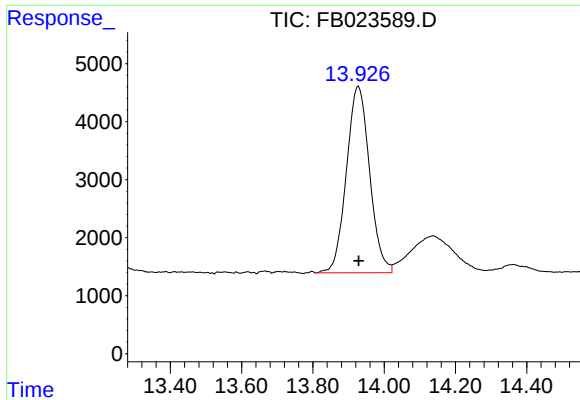

#9 O-Xylene

R.T.: 13.927 min
Delta R.T.: -0.001 min
Response: 145148
Conc: 4.20 ng/ml

Instrument :
FID_B
ClientSampleId :
LOD-MDL-WATER-01-QT1-2020

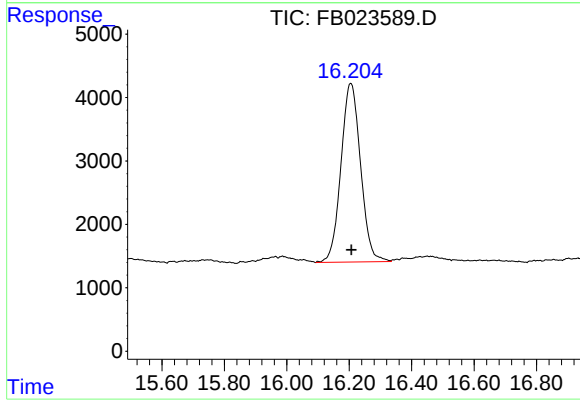

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: -0.001 min
Response: 123027
Conc: 4.21 ng/ml