

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013020\
 Data File : FB023590.D
 Signal(s) : FID2B.CH
 Acq On : 30 Jan 2020 16:32
 Operator : DD/AJ
 Sample : L1161-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 LOQ-WATER-02-QT1-2020

Integration File: Calibration.e
 Quant Time: Jan 31 00:35:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
 Quant Title :
 QLast Update : Thu Jan 16 11:42:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	484917	20.414 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	224202	7.095 ng/ml
2) t 2,2,4-Trimethylpentane	7.412	247745	7.297 ng/ml
3) t n-Heptane	7.754	78001	2.329 ng/ml
4) t Benzene	7.888	96579	2.365 ng/ml
6) t Toluene	10.626	295294	7.472 ng/ml
7) t Ethylbenzene	13.067	92855	2.486 ng/ml
8) t m-Xylene	13.200	178552	5.021 ng/ml
9) t O-Xylene	13.927	174543	5.051 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	151361	5.176 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013020\
Data File : FB023590.D
Signal(s) : FID2B.CH
Acq On : 30 Jan 2020 16:32
Operator : DD/AJ
Sample : L1161-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
LOQ-WATER-02-QT1-2020

Integration File: Calibration.e
Quant Time: Jan 31 00:35:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
Quant Title :
QLast Update : Thu Jan 16 11:42:55 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

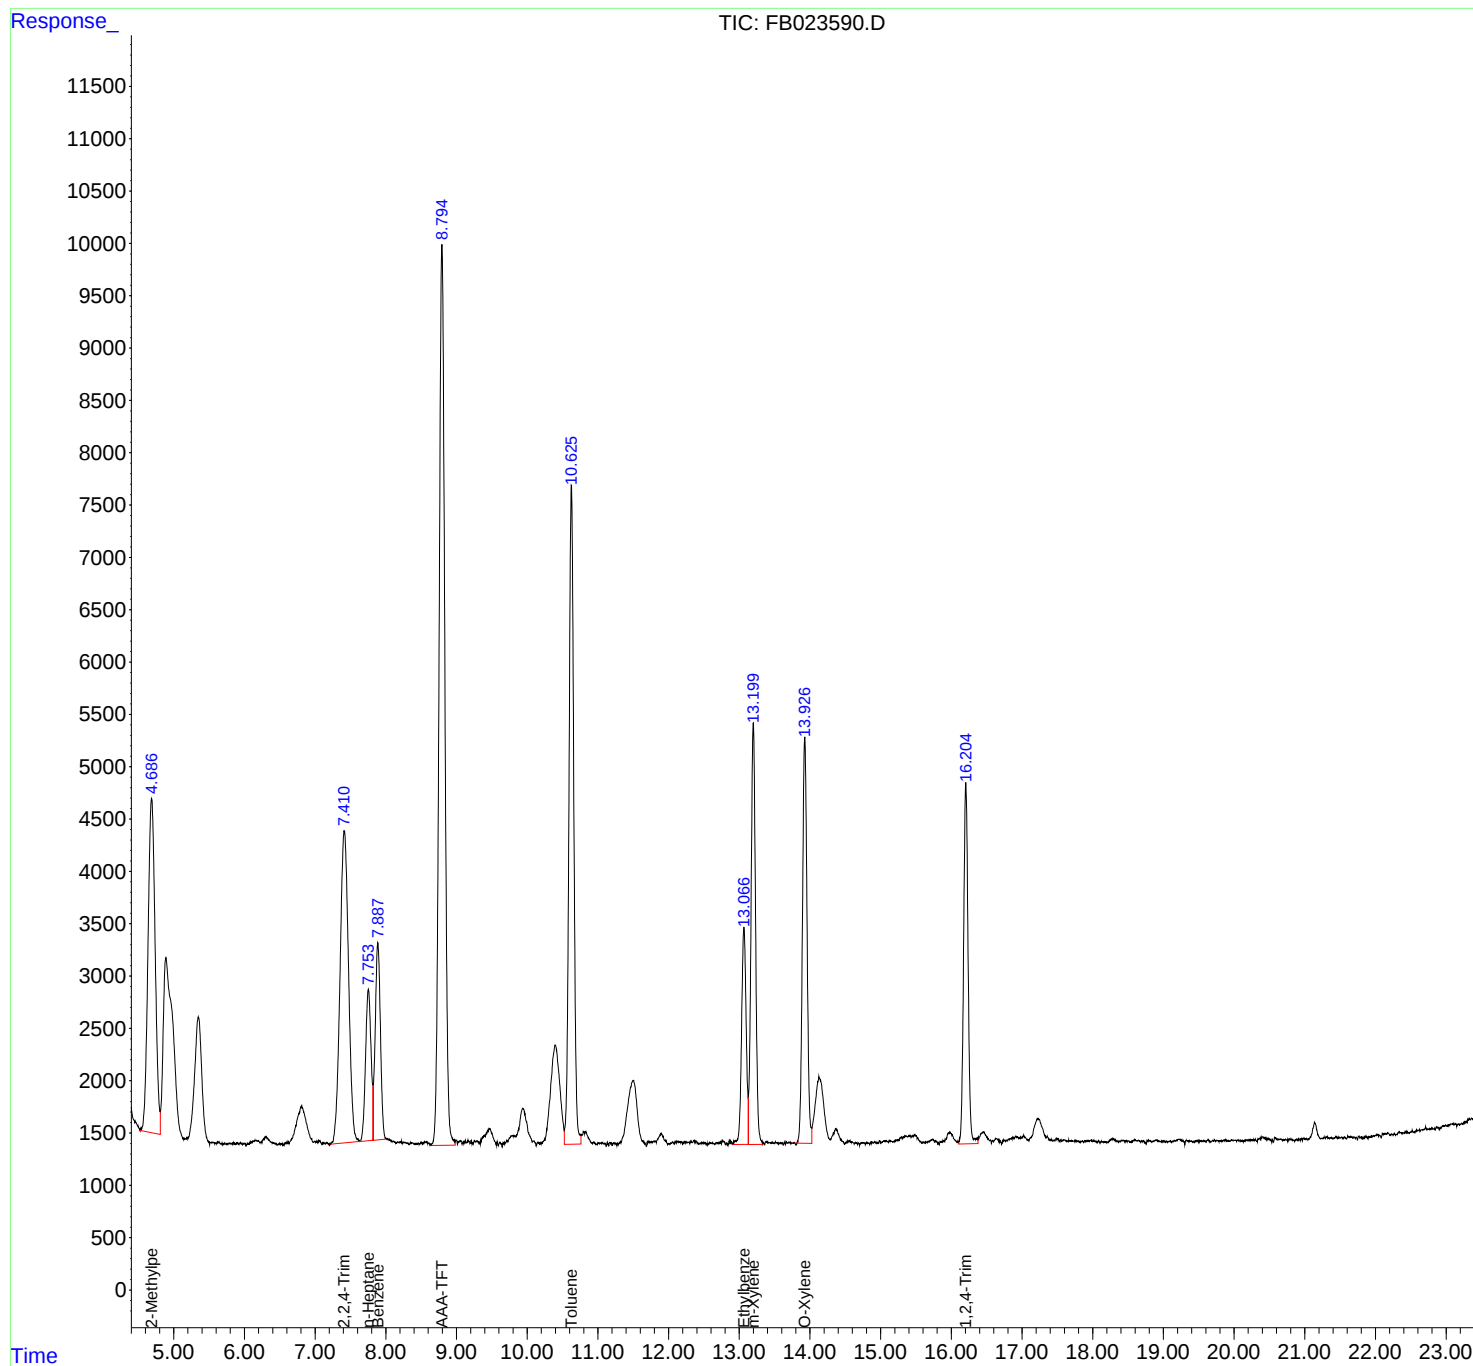


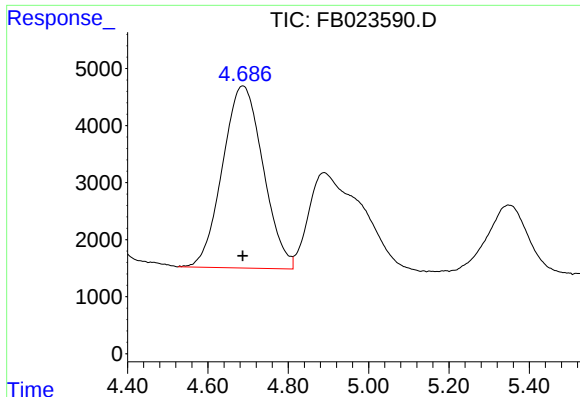

#1 2-Methylpentane


R.T.: 4.688 min
Delta R.T.: 0.000 min
Response: 224202
Conc: 7.09 ng/ml

Instrument :
FID_B
ClientSampleId :
LOQ-WATER-02-QT1-2020

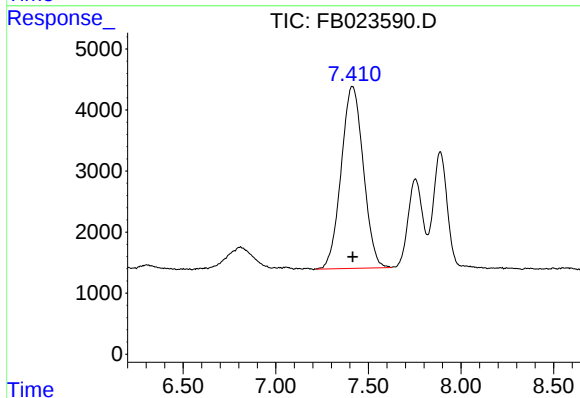


#2 2,2,4-Trimethylpentane

R.T.: 7.412 min
Delta R.T.: -0.004 min
Response: 247745
Conc: 7.30 ng/ml

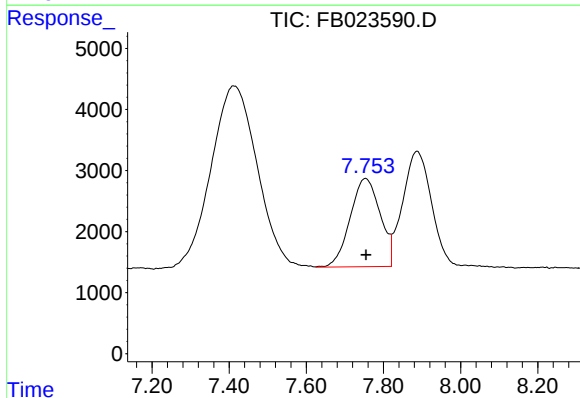


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: -0.001 min
Response: 78001
Conc: 2.33 ng/ml

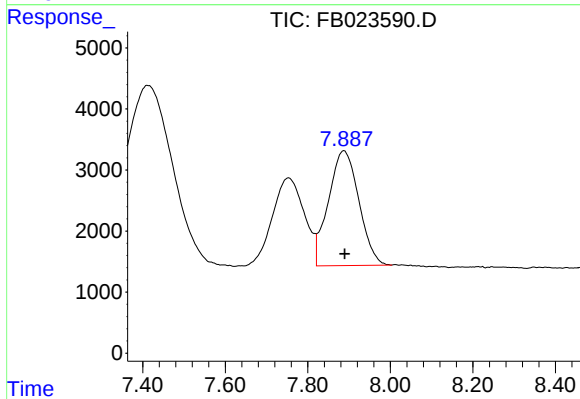

#4 Benzene


R.T.: 7.888 min
Delta R.T.: -0.001 min
Response: 96579
Conc: 2.36 ng/ml

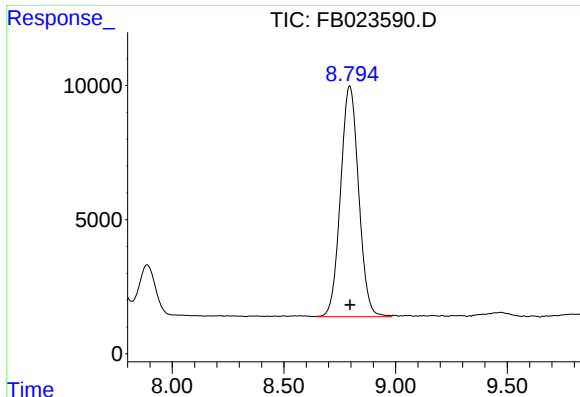

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: -0.002 min
Response: 484917
Conc: 20.41 ng/ml

Instrument :
FID_B
ClientSampleId :
LOQ-WATER-02-QT1-2020

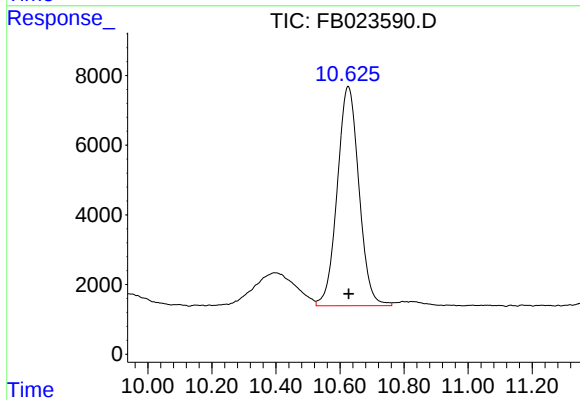


#6 Toluene

R.T.: 10.626 min
Delta R.T.: -0.001 min
Response: 295294
Conc: 7.47 ng/ml

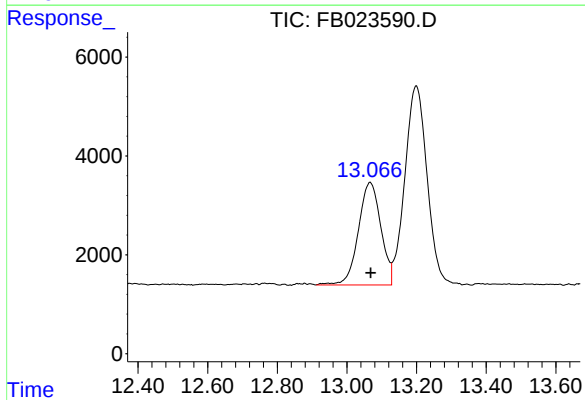


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: 0.000 min
Response: 92855
Conc: 2.49 ng/ml

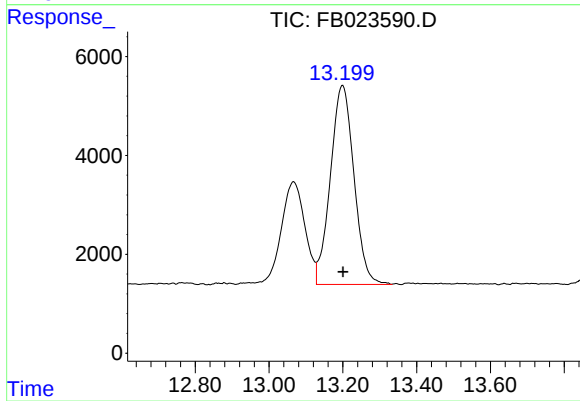

#8 m-Xylene


R.T.: 13.200 min
Delta R.T.: 0.000 min
Response: 178552
Conc: 5.02 ng/ml

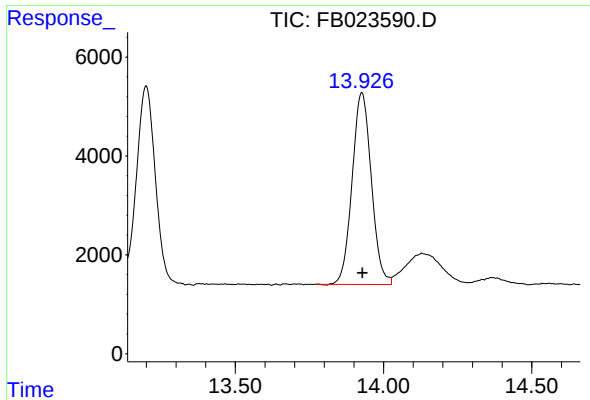

#9 O-Xylene

R.T.: 13.927 min
Delta R.T.: -0.002 min
Response: 174543
Conc: 5.05 ng/ml

Instrument :
FID_B
ClientSampleId :
LOQ-WATER-02-QT1-2020

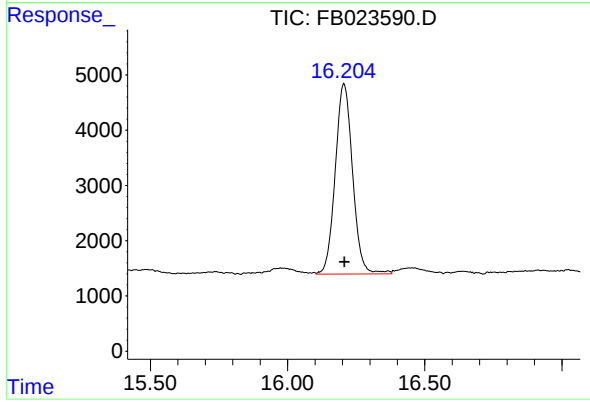

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: -0.001 min
Response: 151361
Conc: 5.18 ng/ml