

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013023\
 Data File : FB029175.D
 Signal(s) : FID2B.CH
 Acq On : 30 Jan 2023 13:38
 Operator : AJ/MA
 Sample : BSF0130S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jan 30 23:57:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011723.M
 Quant Title :
 QLast Update : Tue Jan 17 12:59:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	191349	15.659 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.711	341808	23.347 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	446452	28.138 ng/ml
3) t n-Heptane	7.750	112914	6.758 ng/ml
4) t Benzene	7.886	163236	7.678 ng/ml
6) t Toluene	10.618	480415	23.836 ng/ml
7) t Ethylbenzene	13.055	161641	8.427 ng/ml
8) t m-Xylene	13.187	325283	17.386 ng/ml
9) t O-Xylene	13.914	332961	18.503 ng/ml
10) t 1,2,4-Trimethylbenzene	16.189	363382	20.383 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013023\
Data File : FB029175.D
Signal(s) : FID2B.CH
Acq On : 30 Jan 2023 13:38
Operator : AJ/MA
Sample : BSF0130S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 30 23:57:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011723.M
Quant Title :
QLast Update : Tue Jan 17 12:59:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

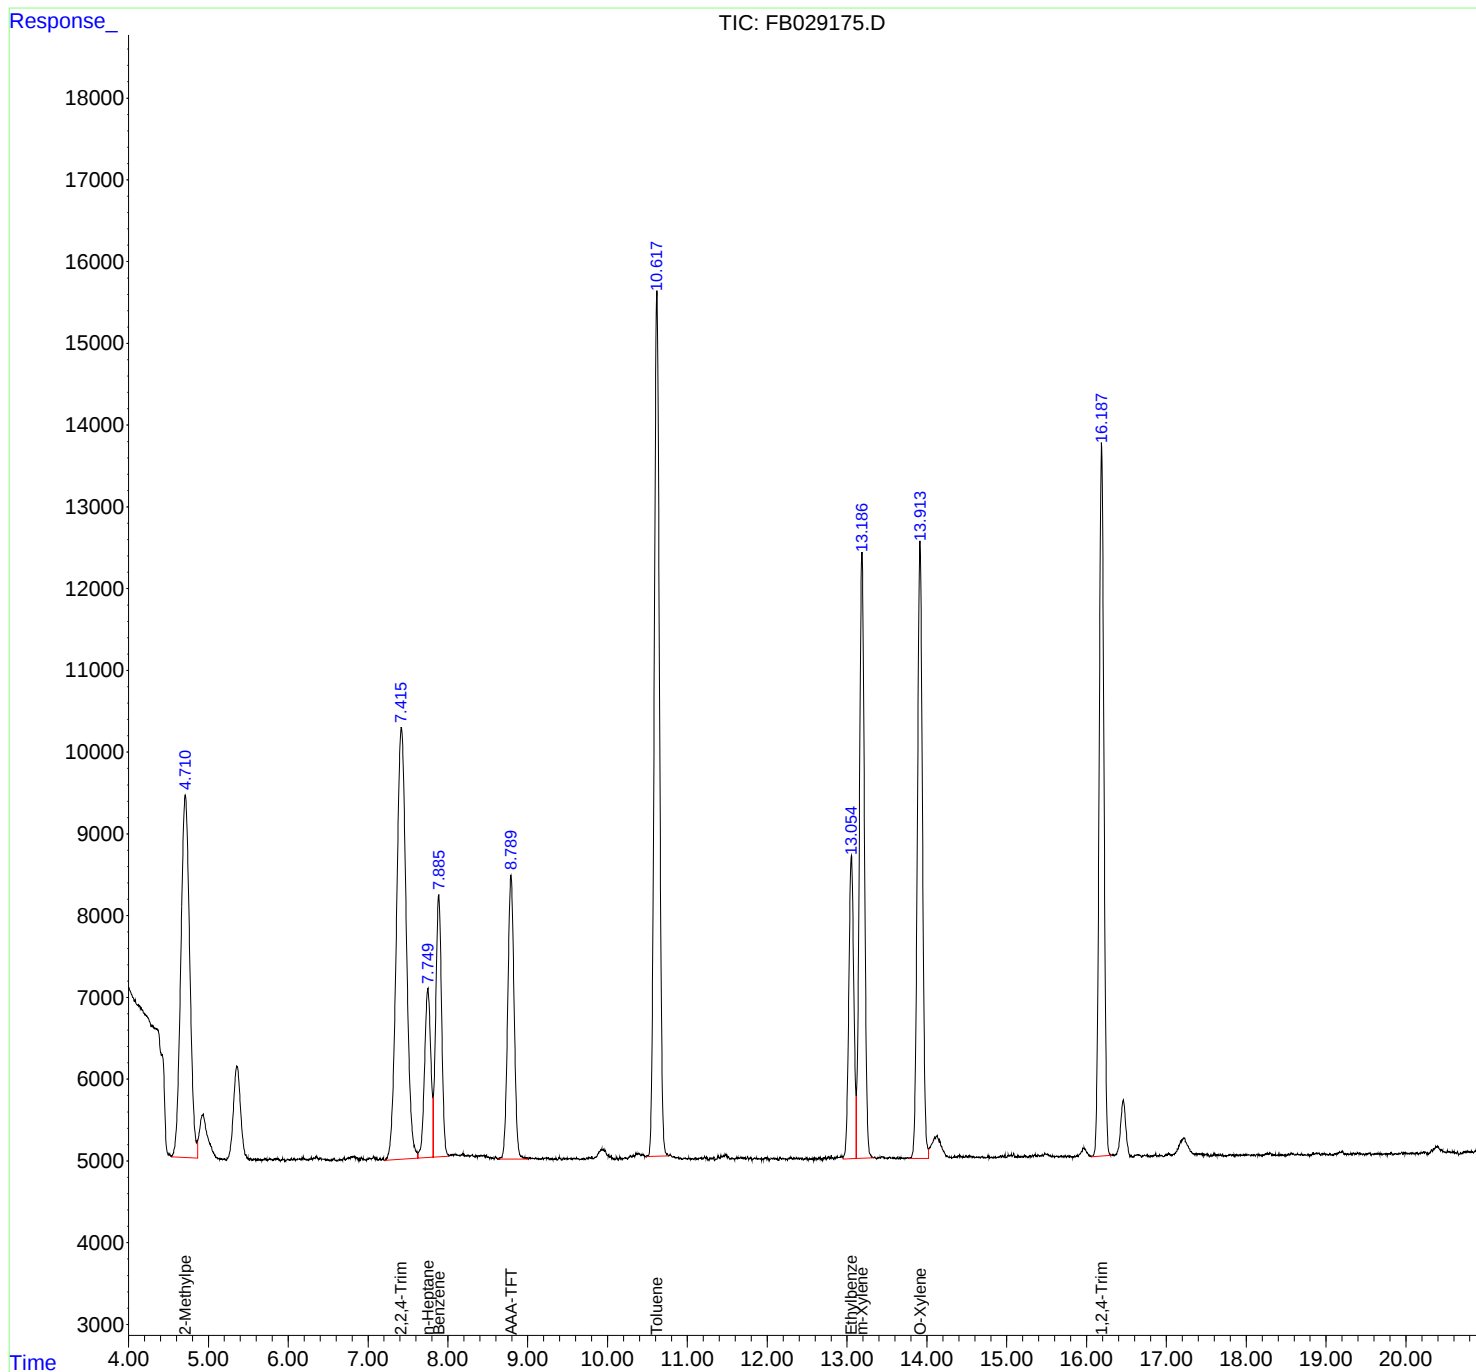


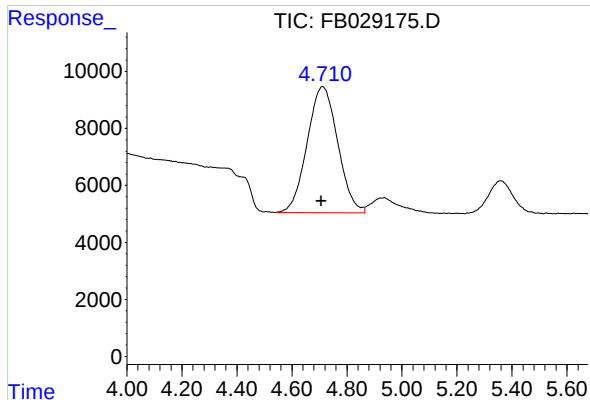

#1 2-Methylpentane


R.T.: 4.711 min
Delta R.T.: 0.004 min
Response: 341808
Conc: 23.35 ng/ml

Instrument :
FID_B
ClientSampleId :

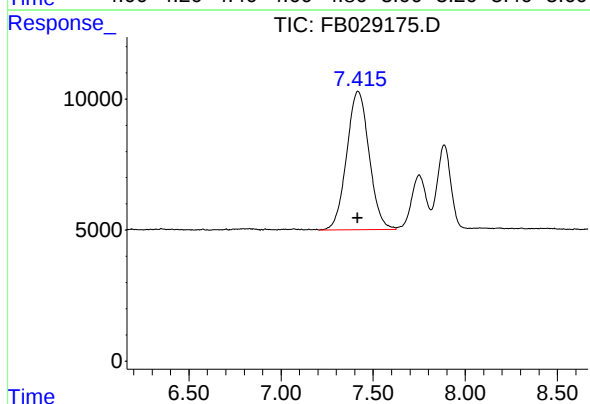


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.001 min
Response: 446452
Conc: 28.14 ng/ml

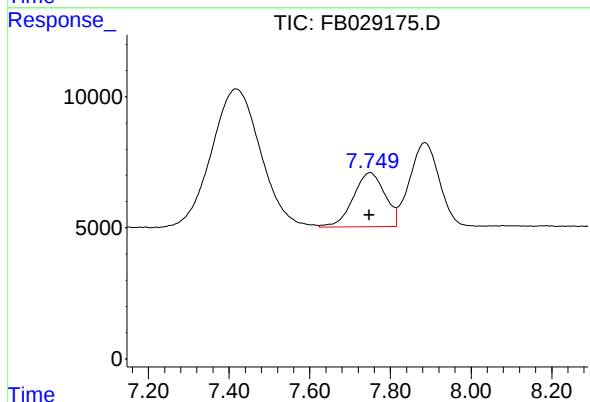


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: 0.003 min
Response: 112914
Conc: 6.76 ng/ml

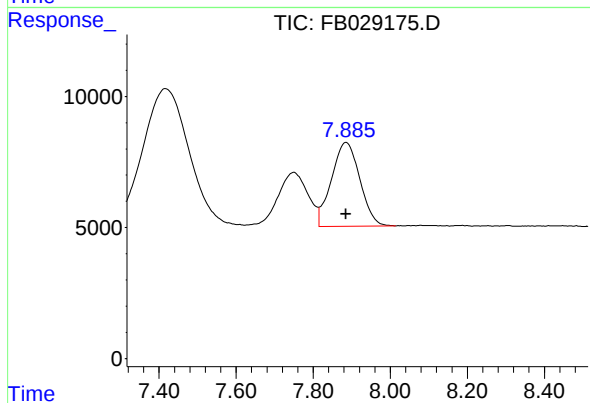

#4 Benzene


R.T.: 7.886 min
Delta R.T.: 0.001 min
Response: 163236
Conc: 7.68 ng/ml

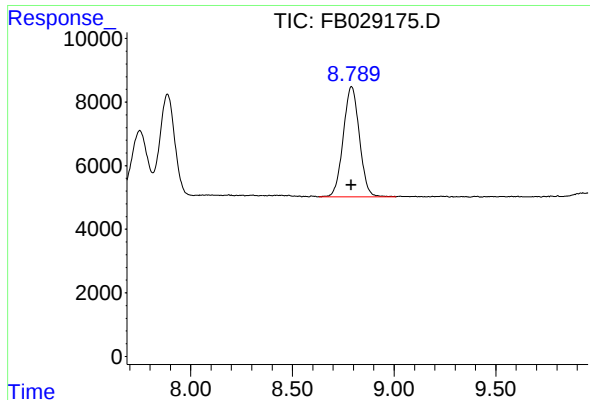

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: 0.001 min
Response: 191349
Conc: 15.66 ng/ml

Instrument :
FID_B
ClientSampleId :

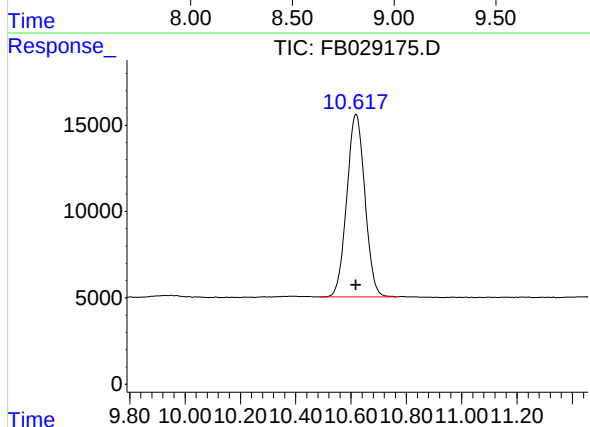


#6 Toluene

R.T.: 10.618 min
Delta R.T.: 0.000 min
Response: 480415
Conc: 23.84 ng/ml

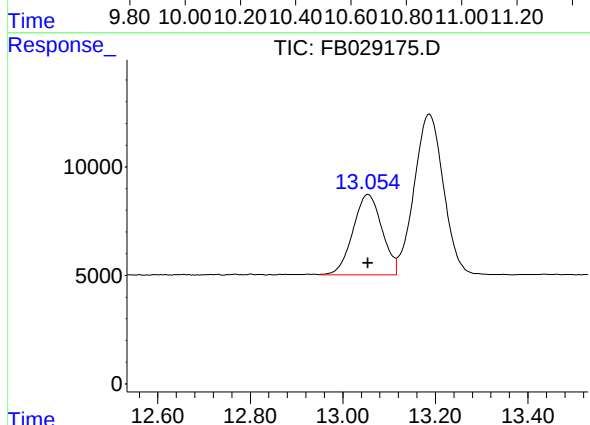


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: 0.000 min
Response: 161641
Conc: 8.43 ng/ml

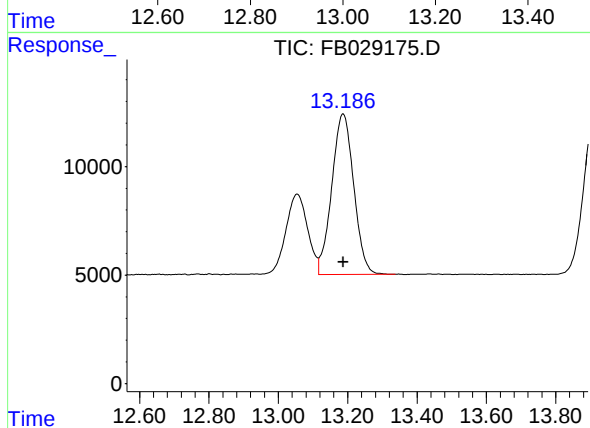

#8 m-Xylene


R.T.: 13.187 min
Delta R.T.: 0.000 min
Response: 325283
Conc: 17.39 ng/ml

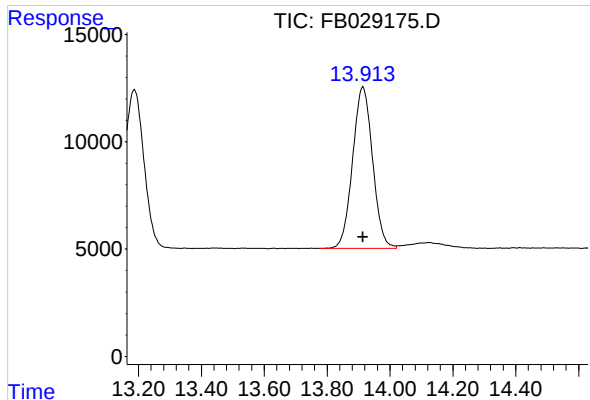

#9 O-Xylene

R.T.: 13.914 min
Delta R.T.: 0.000 min
Response: 332961
Conc: 18.50 ng/ml

Instrument :
FID_B
ClientSampleId :

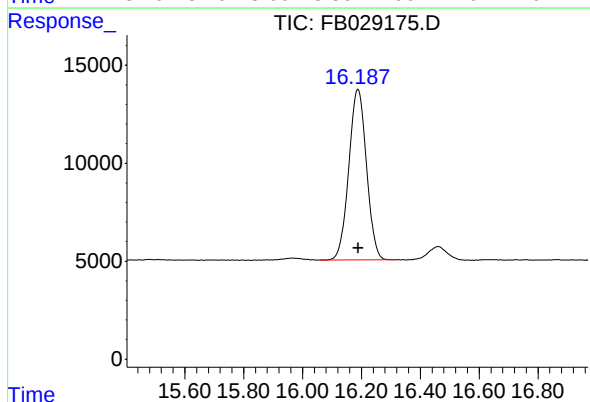

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min
Delta R.T.: -0.001 min
Response: 363382
Conc: 20.38 ng/ml