

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013023\
Data File : FB029176.D
Signal(s) : FID2B.CH
Acq On : 30 Jan 2023 14:16
Operator : AJ/MA
Sample : 01358-02
Misc : 8.09G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 30 23:57:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011723.M
Quant Title :
QLast Update : Tue Jan 17 12:59:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	160591	13.142 ng/ml
Target Compounds			
6) t Toluene	10.623	17096	0.848 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013023\
Data File : FB029176.D
Signal(s) : FID2B.CH
Acq On : 30 Jan 2023 14:16
Operator : AJ/MA
Sample : 01358-02
Misc : 8.09G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 30 23:57:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011723.M
Quant Title :
QLast Update : Tue Jan 17 12:59:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

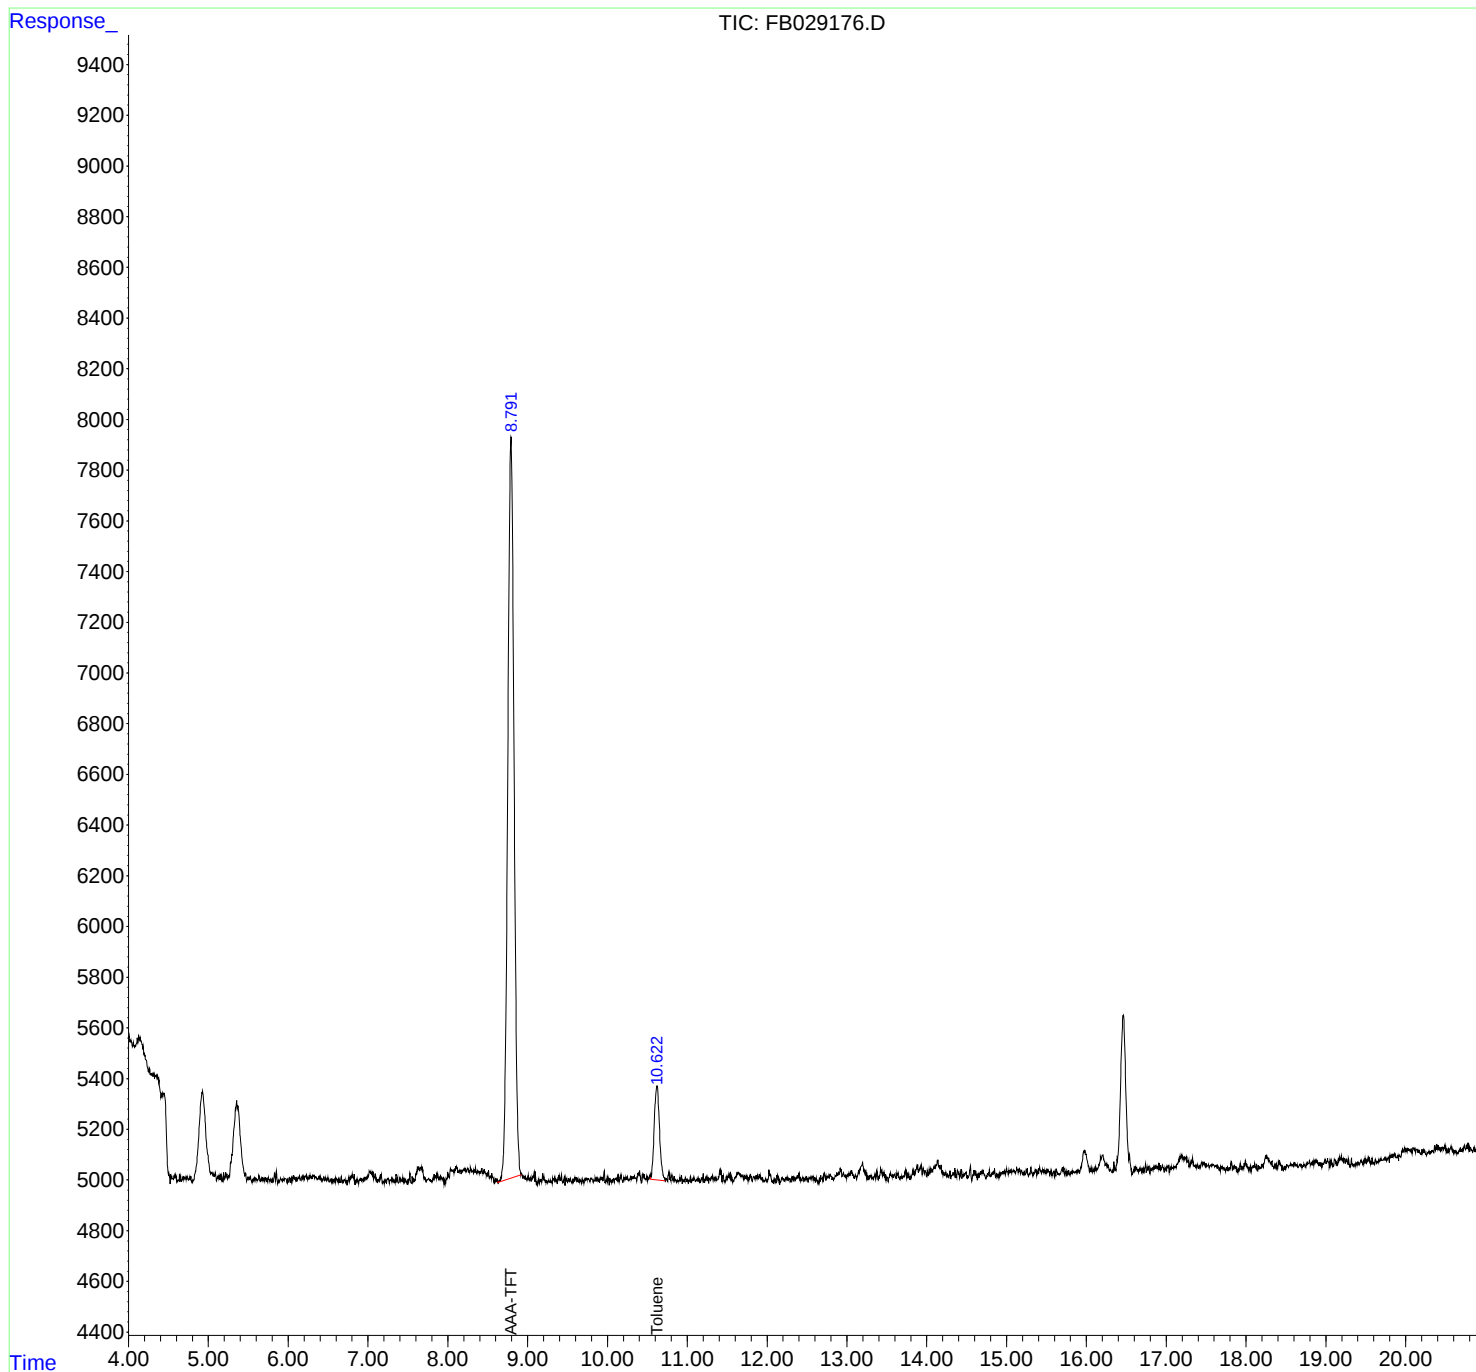

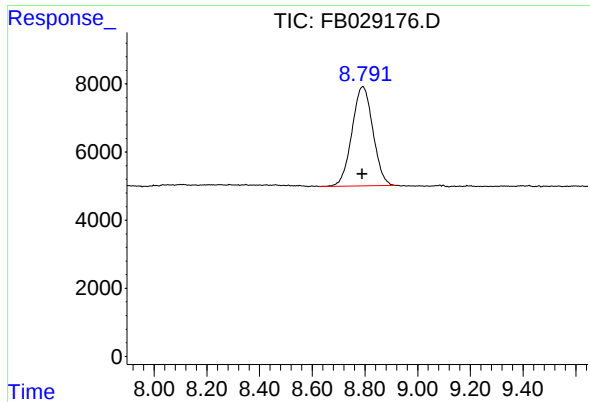


#5 AAA-TFT

R.T.: 8.793 min
Delta R.T.: 0.003 min
Response: 160591
Conc: 13.14 ng/ml

Instrument : FID_B

ClientSampleId :

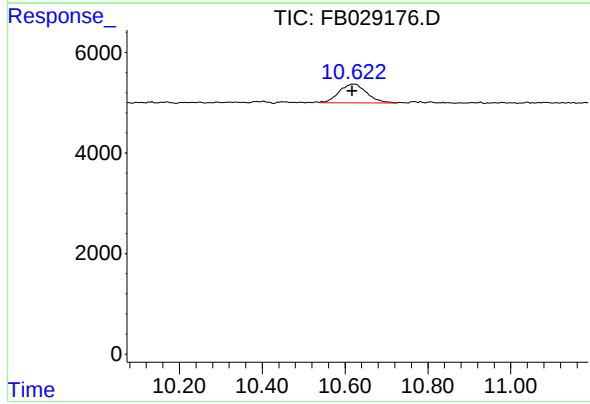

#6 Toluene

R.T.: 10.623 min
Delta R.T.: 0.005 min
Response: 17096
Conc: 0.85 ng/ml