

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013023\
Data File : FB029183.D
Signal(s) : FID2B.CH
Acq On : 30 Jan 2023 19:48
Operator : AJ/MA
Sample : 01358-08
Misc : 8.89G/5.00 ML DI WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 30 23:58:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011723.M
Quant Title :
QLast Update : Tue Jan 17 12:59:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	158842	12.999 ng/ml
Target Compounds			
6) t Toluene	10.619	48671	2.415 ng/ml
7) t Ethylbenzene	13.032	79590	4.149 ng/ml
9) t O-Xylene	13.915	115828	6.437 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013023\
Data File : FB029183.D
Signal(s) : FID2B.CH
Acq On : 30 Jan 2023 19:48
Operator : AJ/MA
Sample : 01358-08
Misc : 8.89G/5.00 ML DI WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 30 23:58:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011723.M
Quant Title :
QLast Update : Tue Jan 17 12:59:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

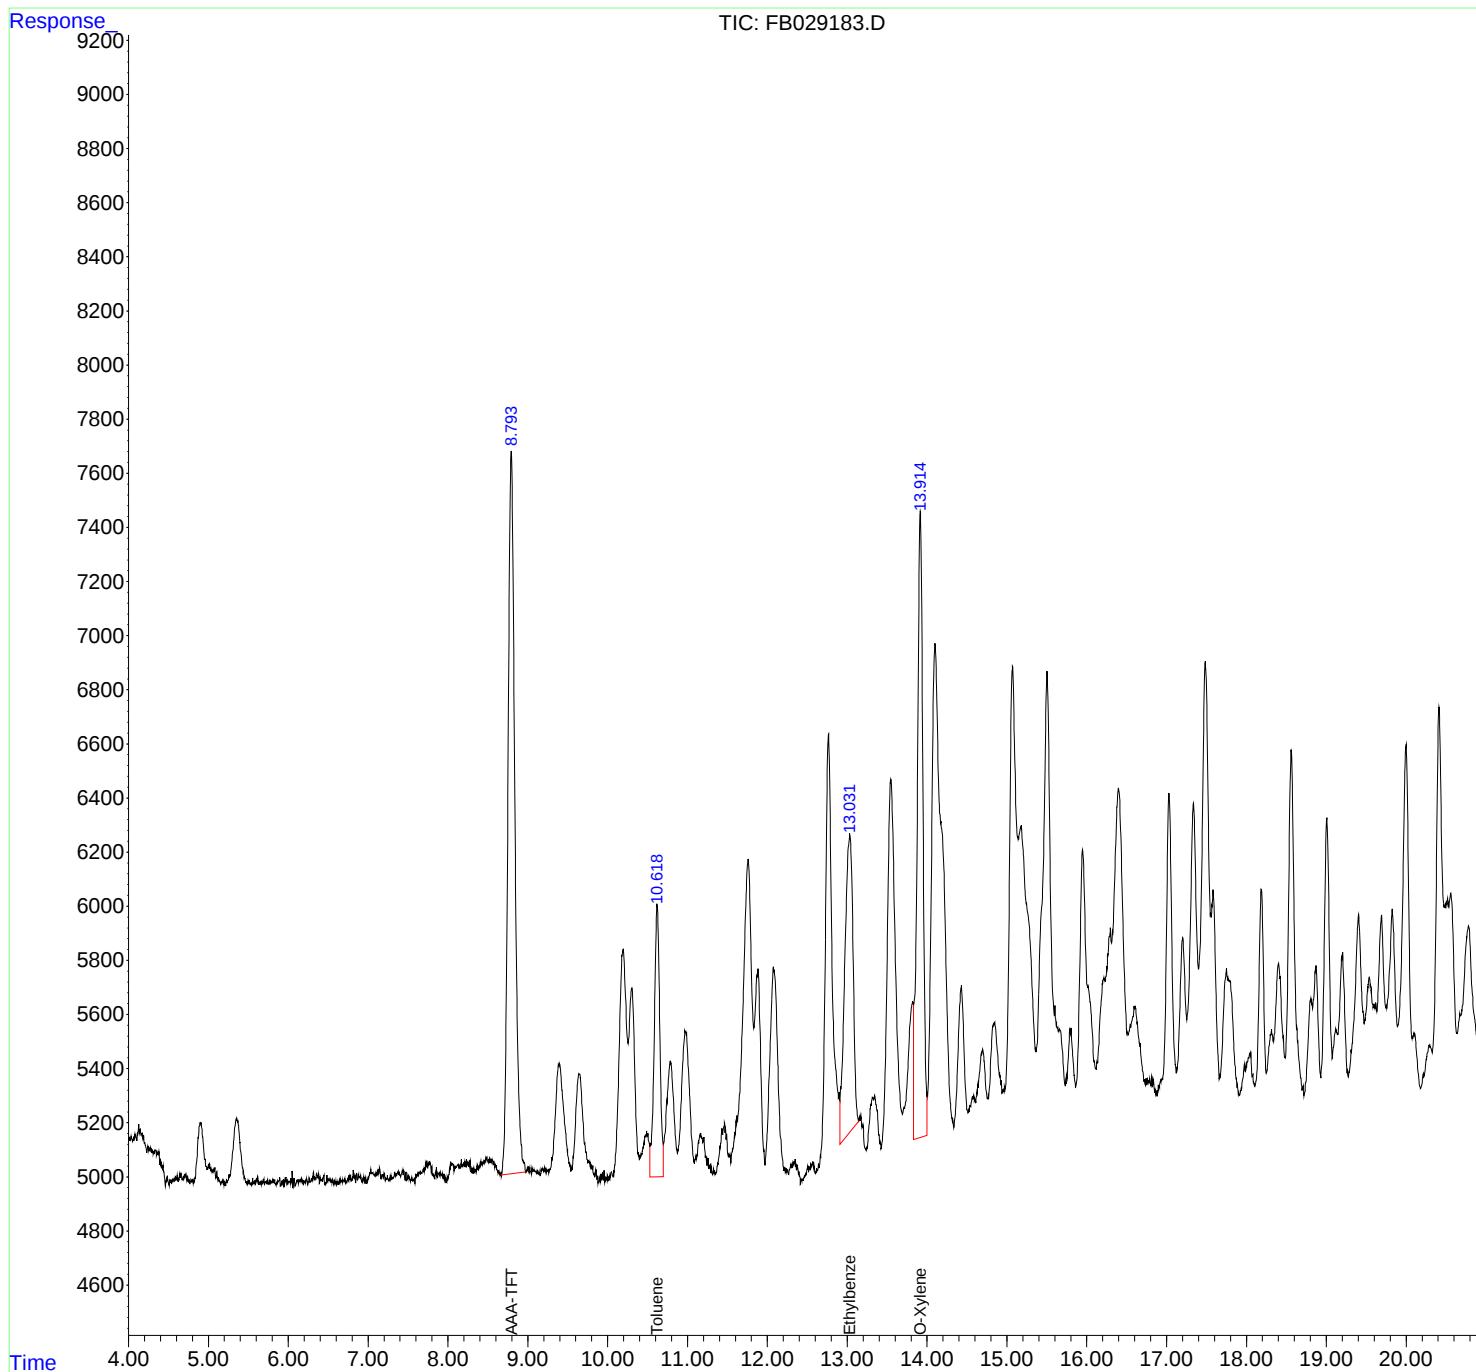


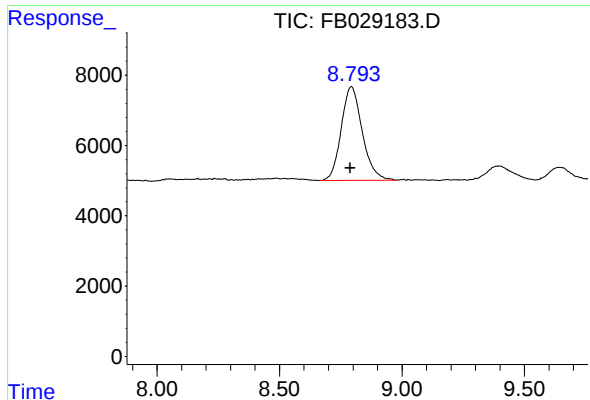

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: 0.005 min
Response: 158842
Conc: 13.00 ng/ml

Instrument :
FID_B
ClientSampleId :

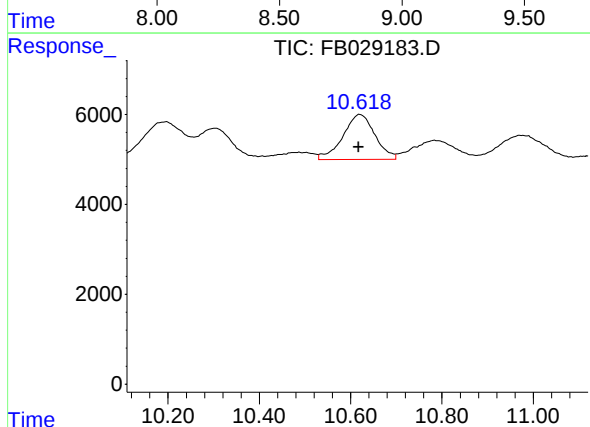


#6 Toluene

R.T.: 10.619 min
Delta R.T.: 0.002 min
Response: 48671
Conc: 2.41 ng/ml

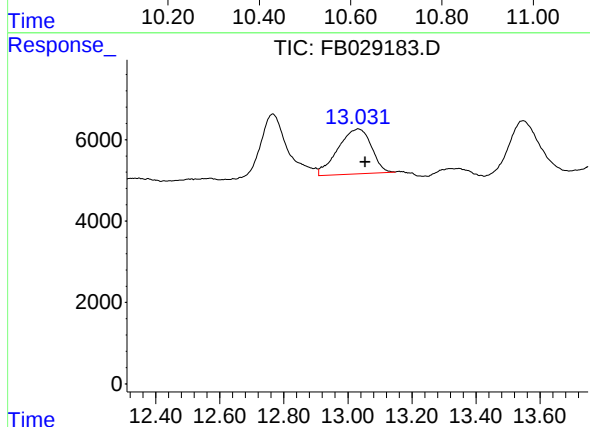

#7 Ethylbenzene

R.T.: 13.032 min
Delta R.T.: -0.022 min
Response: 79590
Conc: 4.15 ng/ml

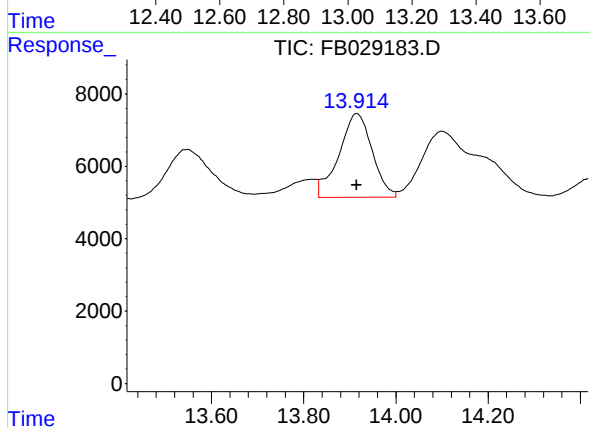

#9 O-Xylene

R.T.: 13.915 min
Delta R.T.: 0.001 min
Response: 115828
Conc: 6.44 ng/ml