

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013023\
Data File : FB029184.D
Signal(s) : FID2B.CH
Acq On : 30 Jan 2023 20:25
Operator : AJ/MA
Sample : 01358-14
Misc : 7.07G/5.00 ML DI WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 30 23:58:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011723.M
Quant Title :
QLast Update : Tue Jan 17 12:59:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	259114	21.205 ng/ml
Target Compounds			
6) t Toluene	10.621	16929	0.840 ng/ml
7) t Ethylbenzene	13.043	1594	0.083 ng/ml
8) t m-Xylene	13.182	3525	0.188 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	32238	1.808 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013023\
Data File : FB029184.D
Signal(s) : FID2B.CH
Acq On : 30 Jan 2023 20:25
Operator : AJ/MA
Sample : 01358-14
Misc : 7.07G/5.00 ML DI WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 30 23:58:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011723.M
Quant Title :
QLast Update : Tue Jan 17 12:59:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

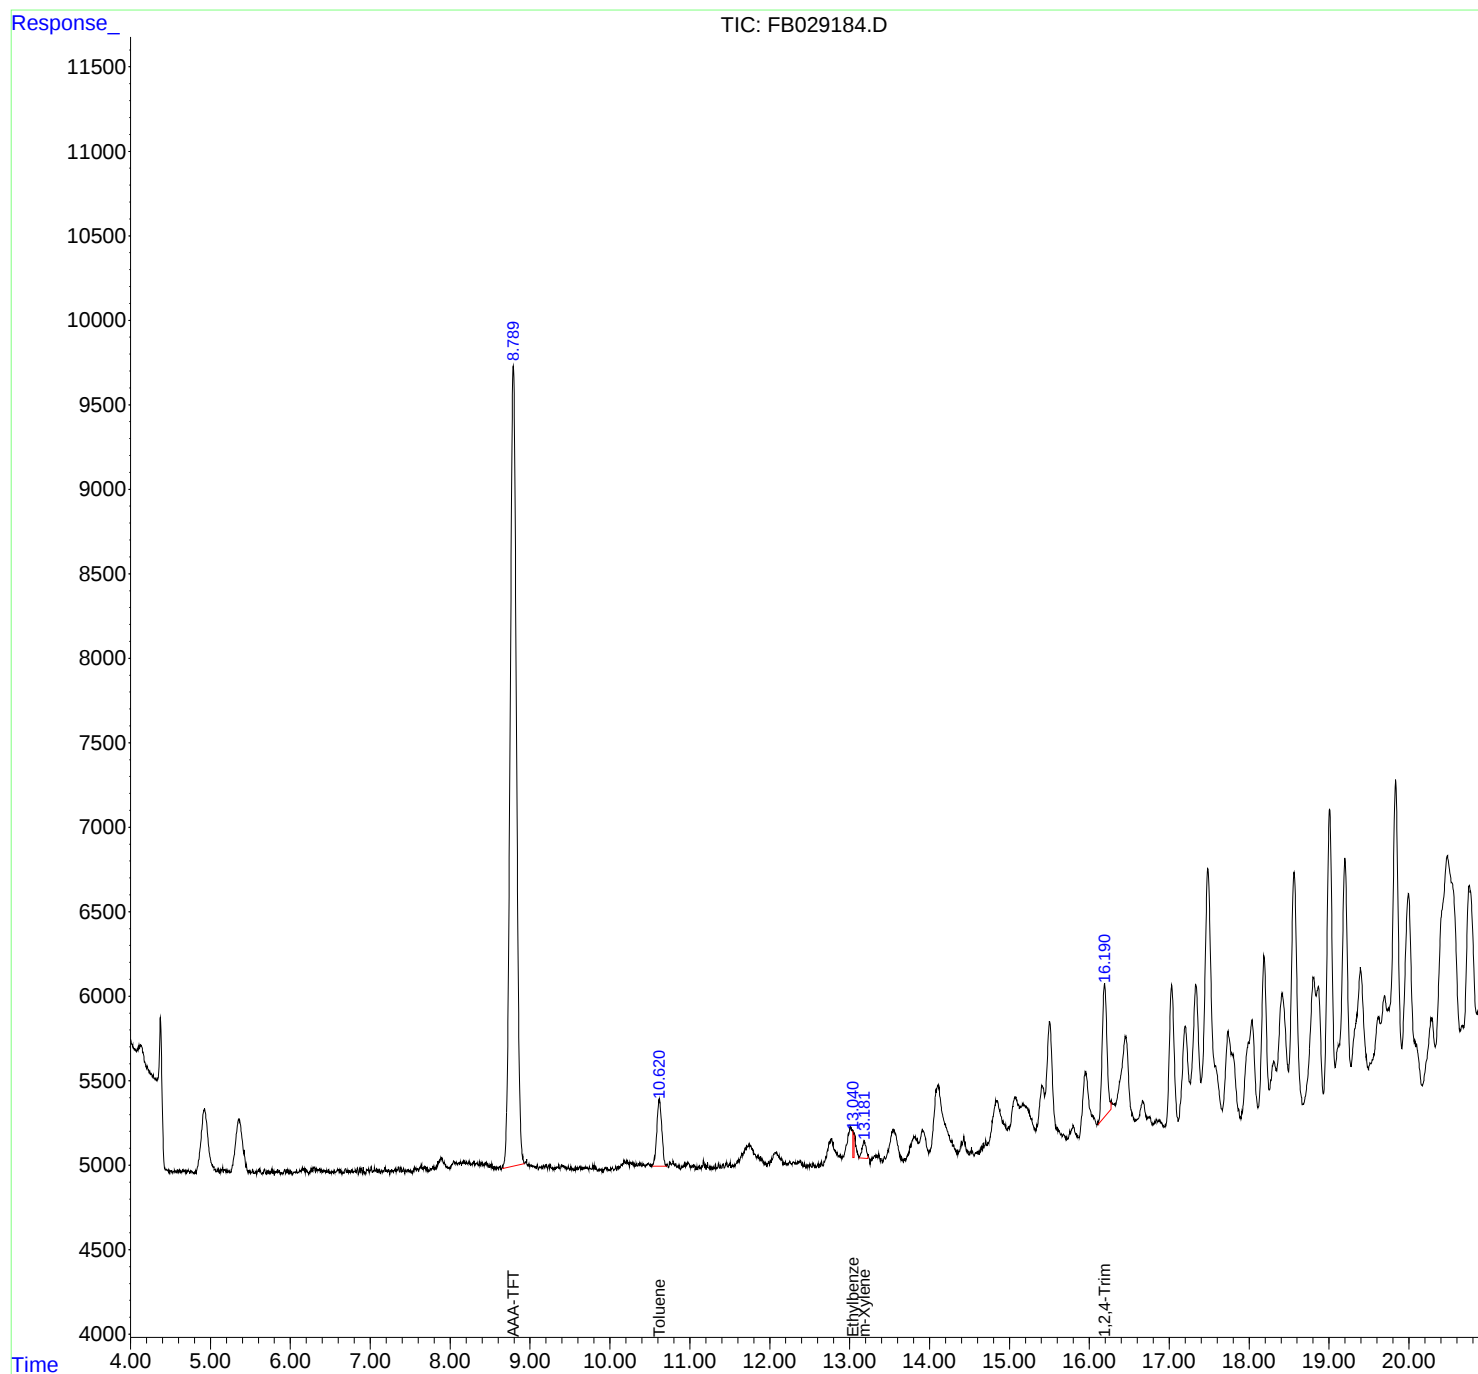


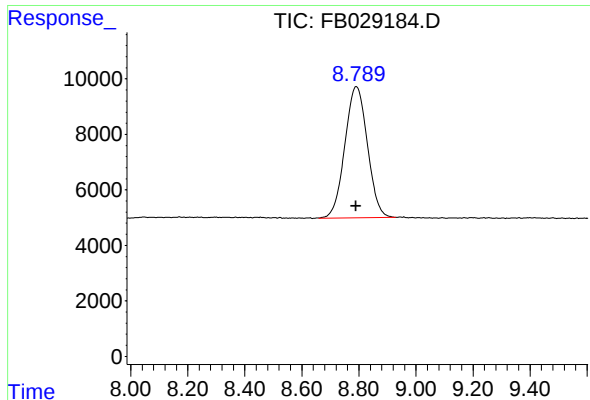

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: 0.001 min
Response: 259114
Conc: 21.21 ng/ml

Instrument :
FID_B
ClientSampleId :

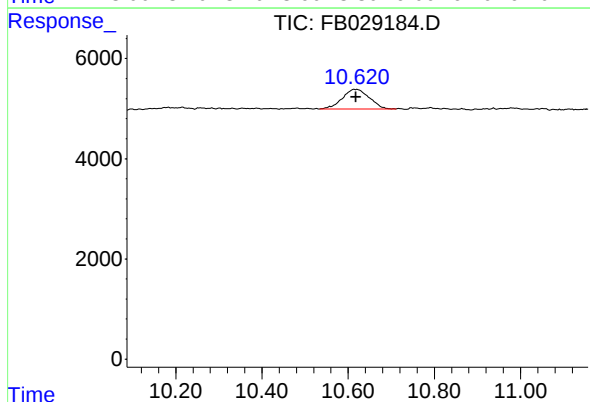


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.004 min
Response: 16929
Conc: 0.84 ng/ml

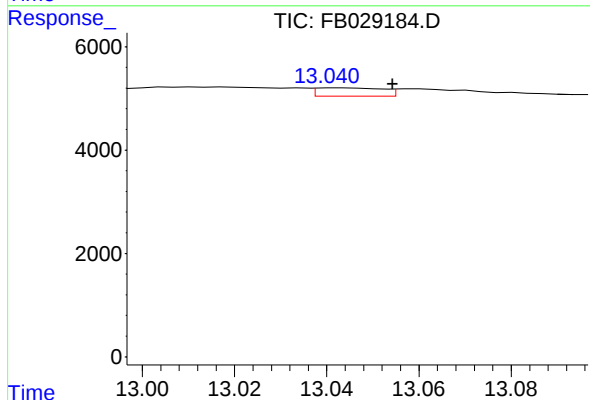


#7 Ethylbenzene

R.T.: 13.043 min
Delta R.T.: -0.012 min
Response: 1594
Conc: 0.08 ng/ml

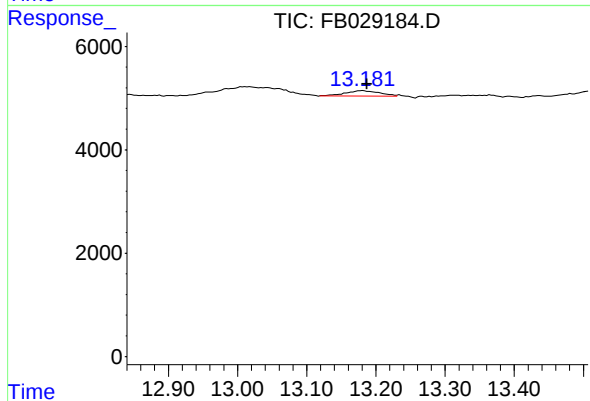

#8 m-Xylene

R.T.: 13.182 min
Delta R.T.: -0.005 min
Response: 3525
Conc: 0.19 ng/ml

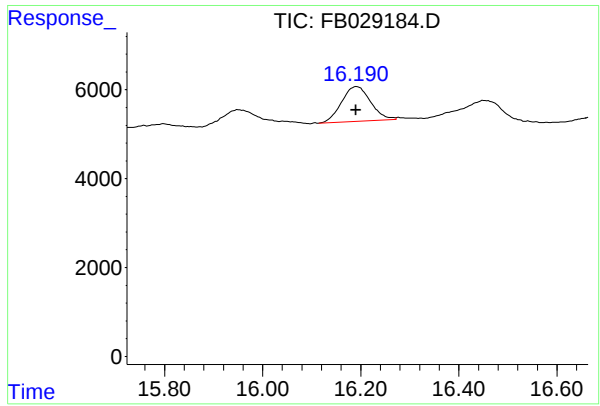

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: 0.002 min
Response: 32238
Conc: 1.81 ng/ml

Instrument :
FID_B
ClientSampleId :