

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013023\
 Data File : FB029185.D
 Signal(s) : FID2B.CH
 Acq On : 30 Jan 2023 21:02
 Operator : AJ/MA
 Sample : 01358-08 50X
 Misc : 6.34G/5.00 ML MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jan 30 23:58:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011723.M
 Quant Title :
 QLast Update : Tue Jan 17 12:59:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.790	303481	24.836 ng/ml
Target Compounds				
6) t	Toluene	10.619	21613	1.072 ng/ml
7) t	Ethylbenzene	13.045	4047	0.211 ng/ml
8) t	m-Xylene	13.186	11751	0.628 ng/ml
9) t	O-Xylene	13.917	10159	0.565 ng/ml
10) t	1,2,4-Trimethylbenzene	16.188	7292	0.409 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013023\
Data File : FB029185.D
Signal(s) : FID2B.CH
Acq On : 30 Jan 2023 21:02
Operator : AJ/MA
Sample : 01358-08 50X
Misc : 6.34G/5.00 ML MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 30 23:58:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011723.M
Quant Title :
QLast Update : Tue Jan 17 12:59:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

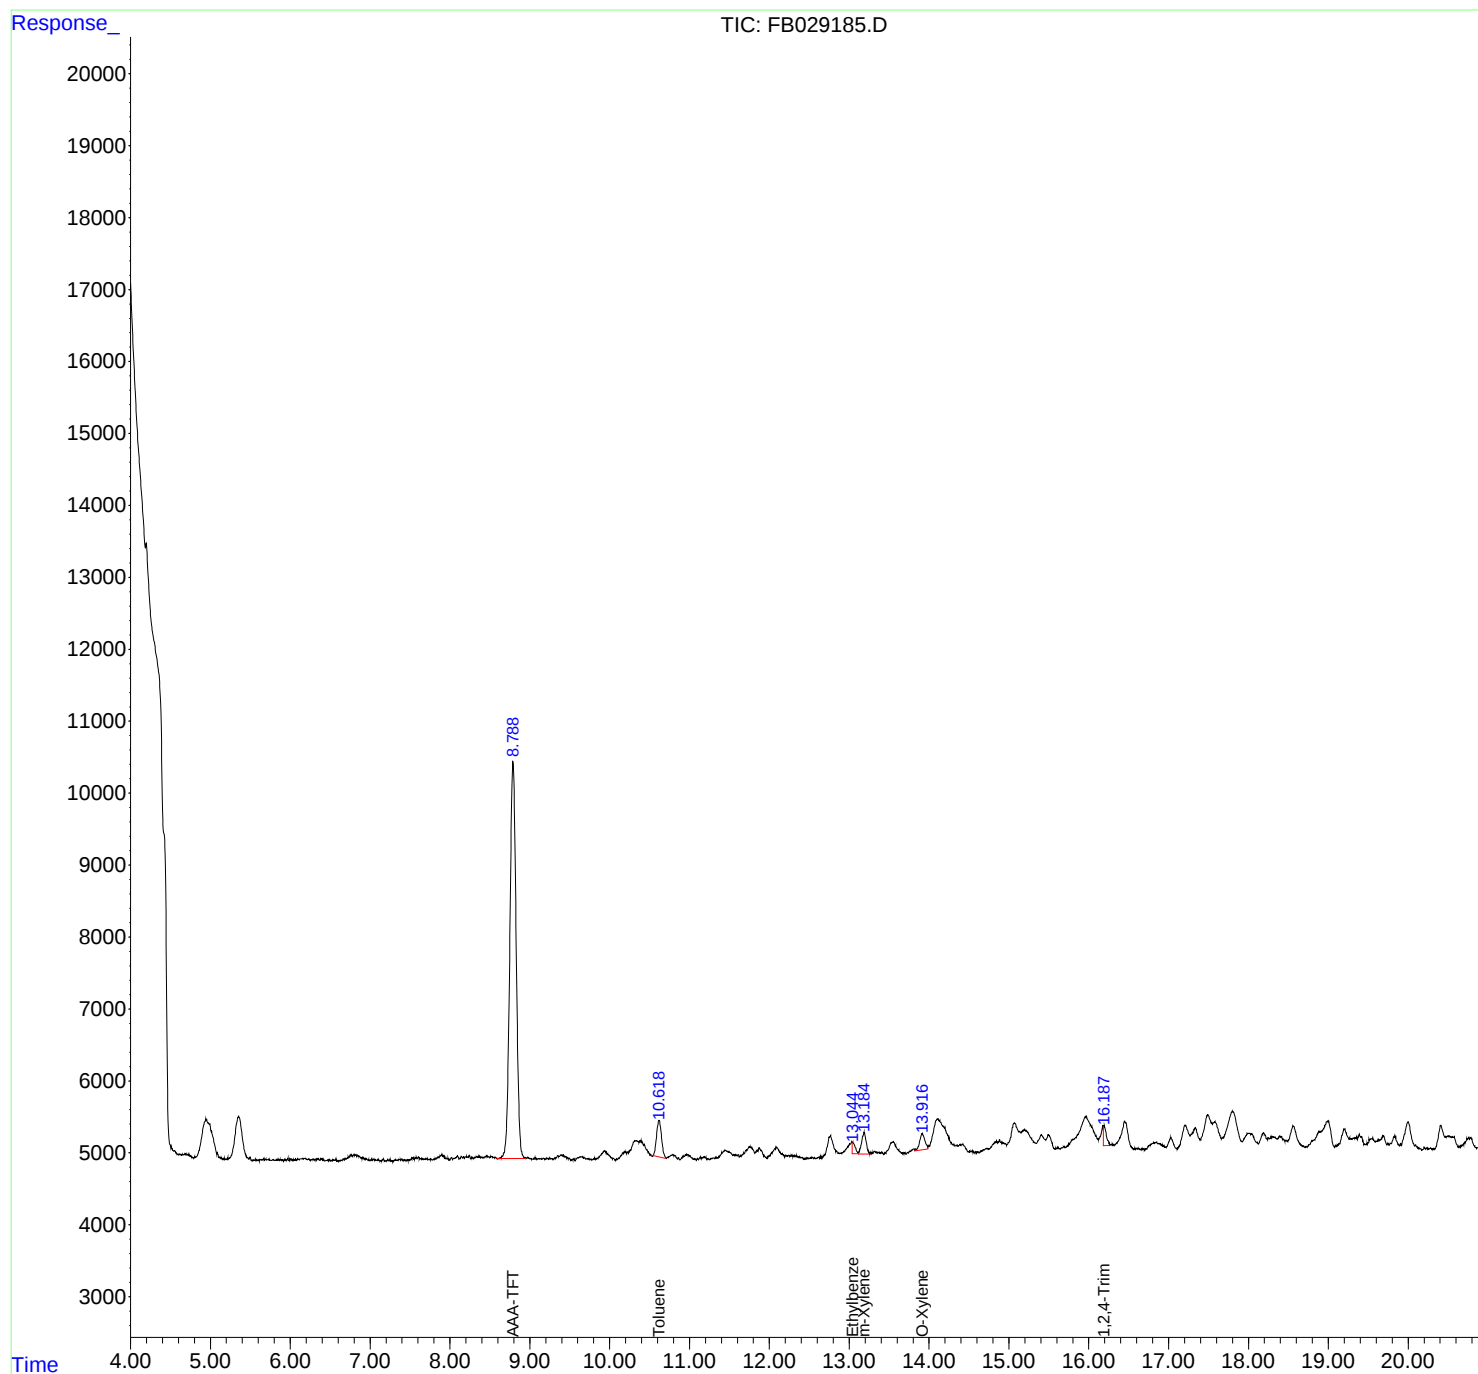


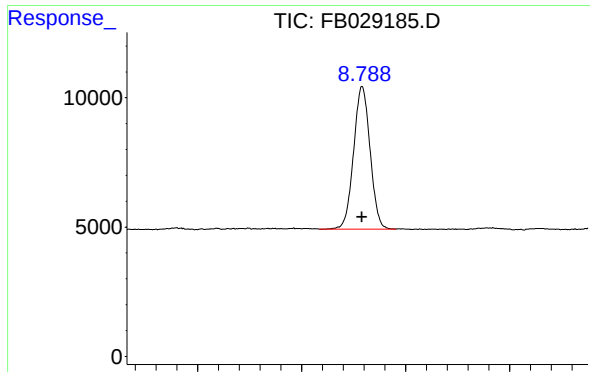

#5 AAA-TFT


R.T.: 8.790 min
Delta R.T.: 0.000 min
Response: 303481
Conc: 24.84 ng/ml

Instrument :
FID_B
ClientSampleId :

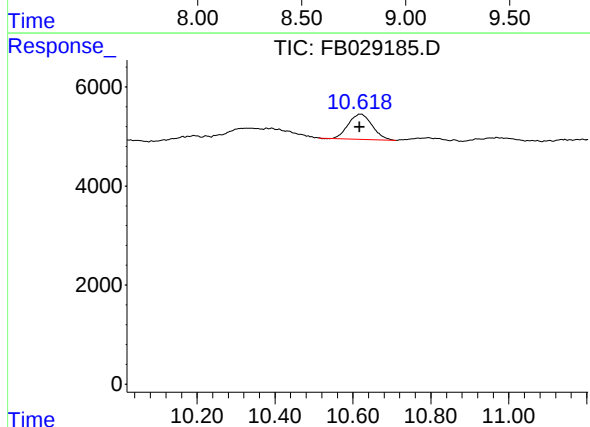


#6 Toluene

R.T.: 10.619 min
Delta R.T.: 0.002 min
Response: 21613
Conc: 1.07 ng/ml

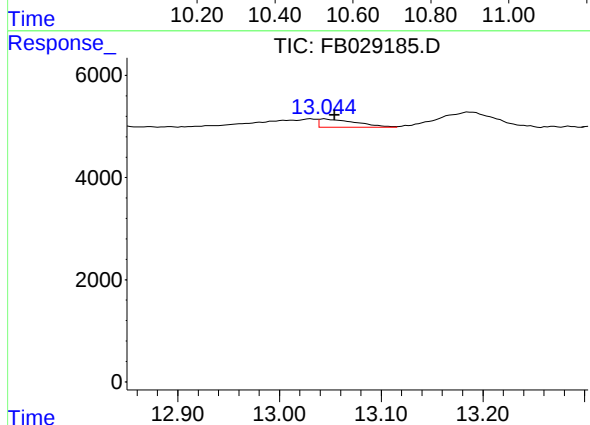


#7 Ethylbenzene

R.T.: 13.045 min
Delta R.T.: -0.009 min
Response: 4047
Conc: 0.21 ng/ml

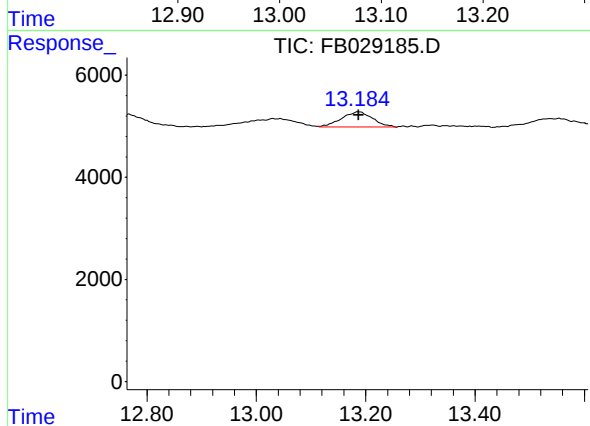

#8 m-Xylene


R.T.: 13.186 min
Delta R.T.: -0.001 min
Response: 11751
Conc: 0.63 ng/ml

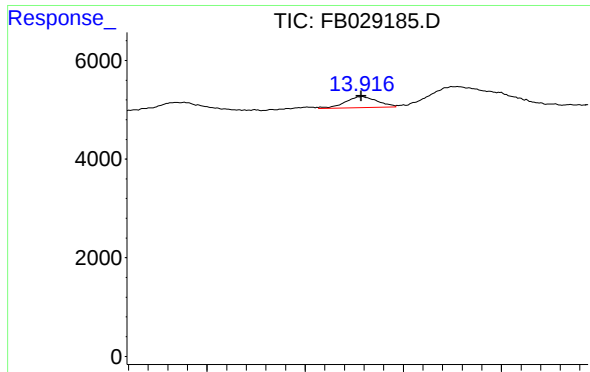

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: 0.003 min
Response: 10159
Conc: 0.56 ng/ml

Instrument :
FID_B
ClientSampleId :

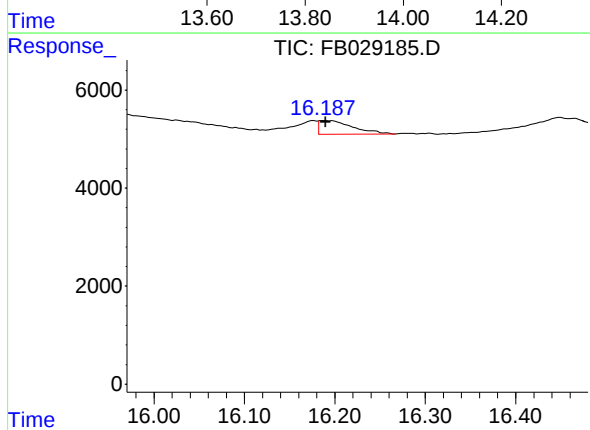

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: -0.002 min
Response: 7292
Conc: 0.41 ng/ml