

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013023\
 Data File : FB029181.D
 Signal(s) : FID2B.CH
 Acq On : 30 Jan 2023 17:21
 Operator : AJ/MA
 Sample : BSF0130S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0130S2

Integration File: Calibration.e
 Quant Time: Jan 30 23:58:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011723.M
 Quant Title :
 QLast Update : Tue Jan 17 12:59:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	322254	26.372 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.708	366435	25.029 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	440608	27.770 ng/ml
3) t n-Heptane	7.749	132913	7.954 ng/ml
4) t Benzene	7.886	191346	9.000 ng/ml
6) t Toluene	10.619	563165	27.941 ng/ml
7) t Ethylbenzene	13.055	176622	9.208 ng/ml
8) t m-Xylene	13.188	350158	18.715 ng/ml
9) t O-Xylene	13.915	343871	19.109 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	339800	19.060 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013023\
Data File : FB029181.D
Signal(s) : FID2B.CH
Acq On : 30 Jan 2023 17:21
Operator : AJ/MA
Sample : BSF0130S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0130S2

Integration File: Calibration.e
Quant Time: Jan 30 23:58:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011723.M
Quant Title :
QLast Update : Tue Jan 17 12:59:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

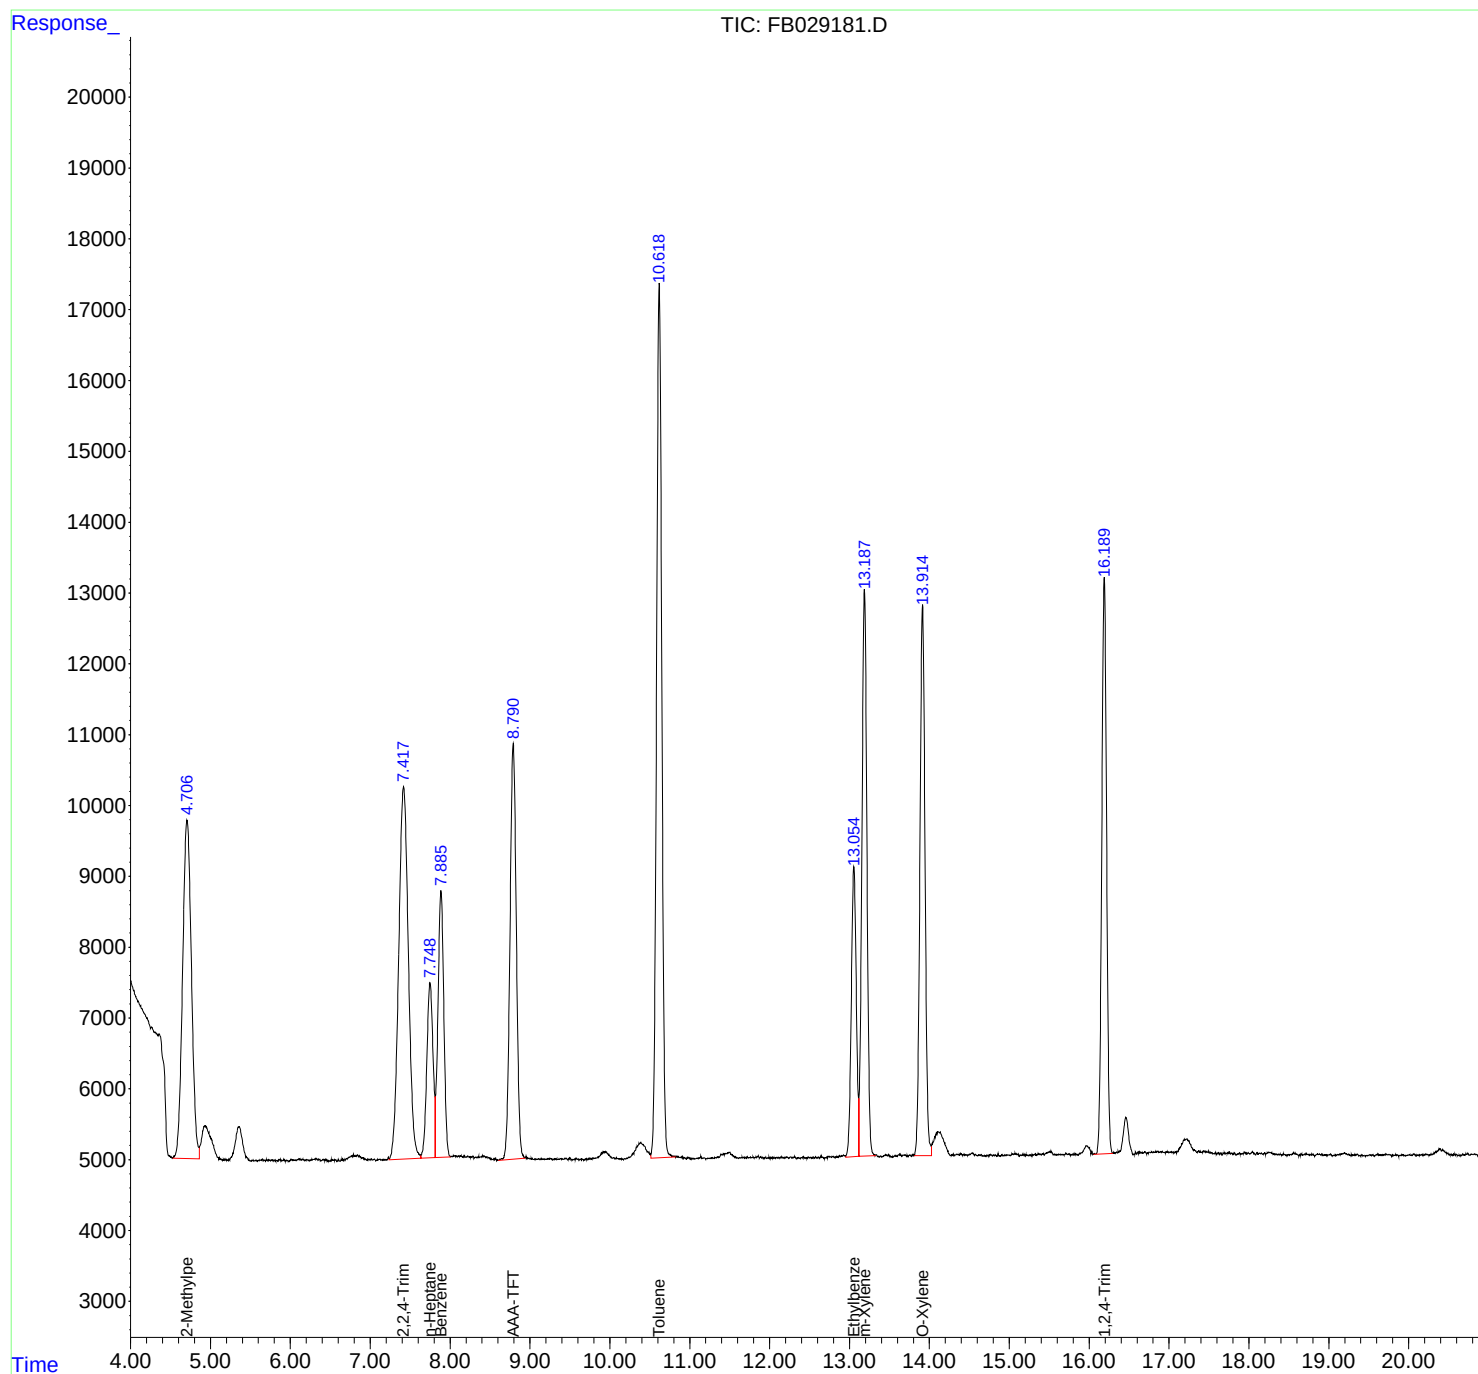


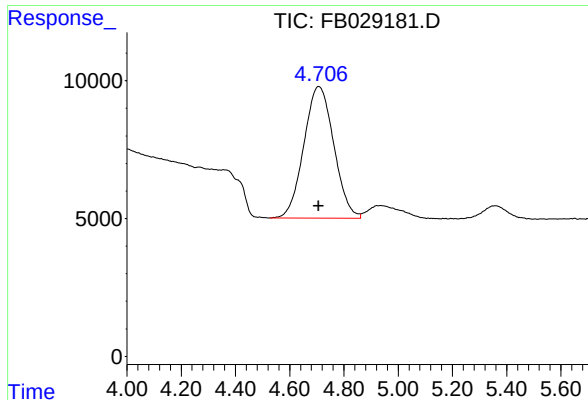

#1 2-Methylpentane


R.T.: 4.708 min
Delta R.T.: 0.001 min
Response: 366435
Conc: 25.03 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0130S2

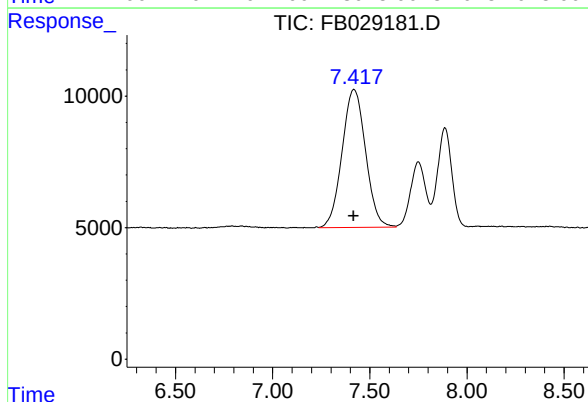


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 440608
Conc: 27.77 ng/ml

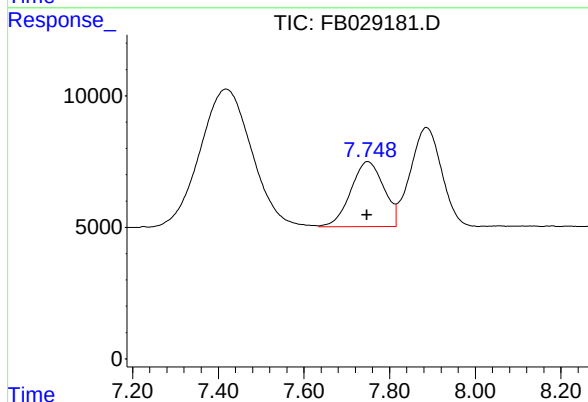


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: 0.002 min
Response: 132913
Conc: 7.95 ng/ml

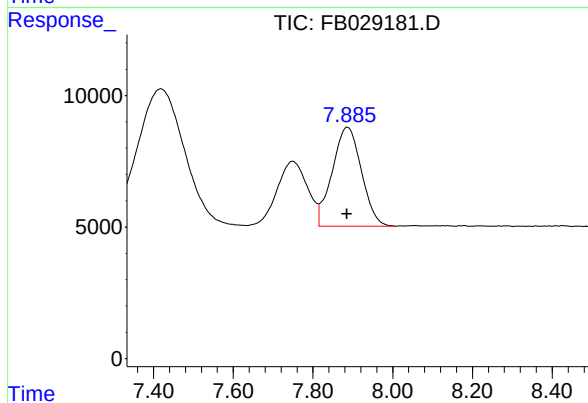

#4 Benzene


R.T.: 7.886 min
Delta R.T.: 0.002 min
Response: 191346
Conc: 9.00 ng/ml

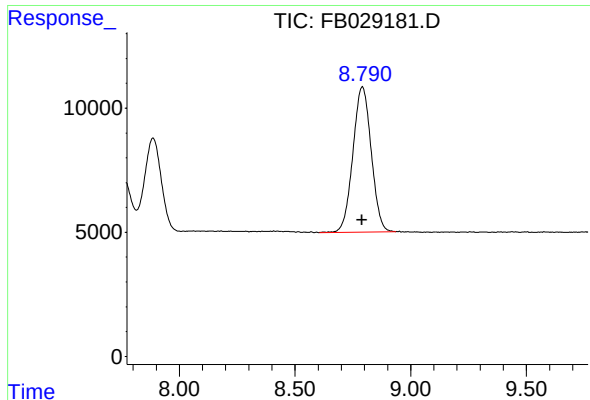

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: 0.002 min
Response: 322254
Conc: 26.37 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0130S2

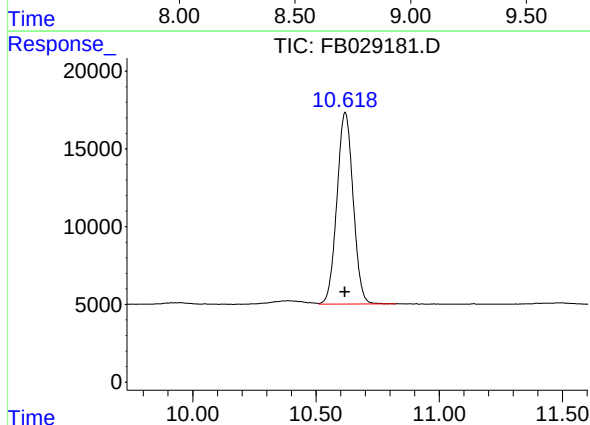


#6 Toluene

R.T.: 10.619 min
Delta R.T.: 0.001 min
Response: 563165
Conc: 27.94 ng/ml

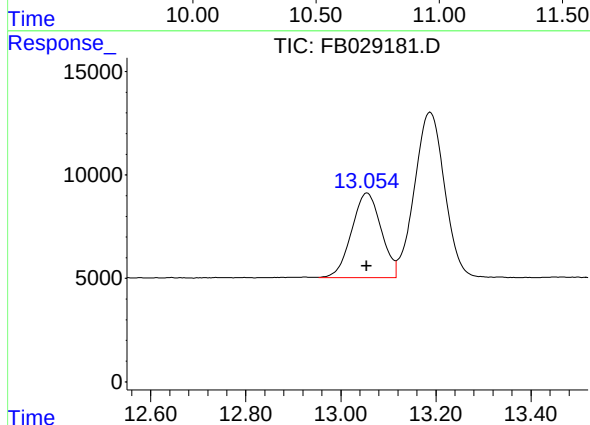


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: 0.000 min
Response: 176622
Conc: 9.21 ng/ml

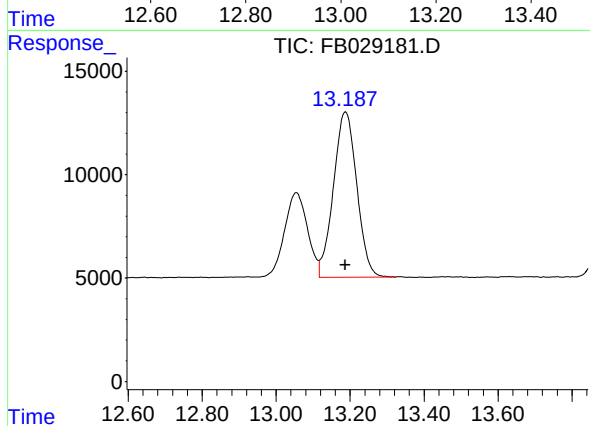

#8 m-Xylene


R.T.: 13.188 min
Delta R.T.: 0.000 min
Response: 350158
Conc: 18.72 ng/ml

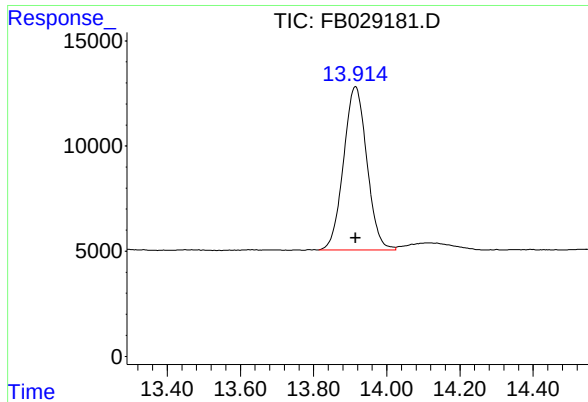

#9 O-Xylene

R.T.: 13.915 min
Delta R.T.: 0.000 min
Response: 343871
Conc: 19.11 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0130S2

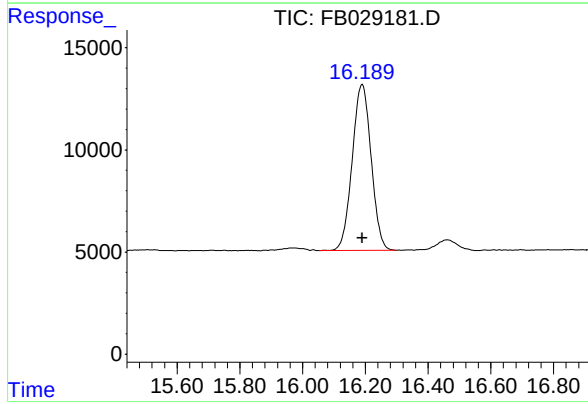

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: 0.000 min
Response: 339800
Conc: 19.06 ng/ml