

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013023\
 Data File : FB029187.D
 Signal(s) : FID2B.CH
 Acq On : 30 Jan 2023 22:16
 Operator : AJ/MA
 Sample : BSF0130S3
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0130S3

Integration File: Calibration.e
 Quant Time: Jan 30 23:58:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011723.M
 Quant Title :
 QLast Update : Tue Jan 17 12:59:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	268332	21.959 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.705	383597	26.201 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	454884	28.670 ng/ml
3) t n-Heptane	7.750	140996	8.438 ng/ml
4) t Benzene	7.886	200461	9.429 ng/ml
6) t Toluene	10.619	586169	29.082 ng/ml
7) t Ethylbenzene	13.055	183675	9.576 ng/ml
8) t m-Xylene	13.188	362082	19.353 ng/ml
9) t O-Xylene	13.915	358479	19.921 ng/ml
10) t 1,2,4-Trimethylbenzene	16.189	346843	19.455 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013023\
Data File : FB029187.D
Signal(s) : FID2B.CH
Acq On : 30 Jan 2023 22:16
Operator : AJ/MA
Sample : BSF0130S3
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0130S3

Integration File: Calibration.e
Quant Time: Jan 30 23:58:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011723.M
Quant Title :
QLast Update : Tue Jan 17 12:59:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

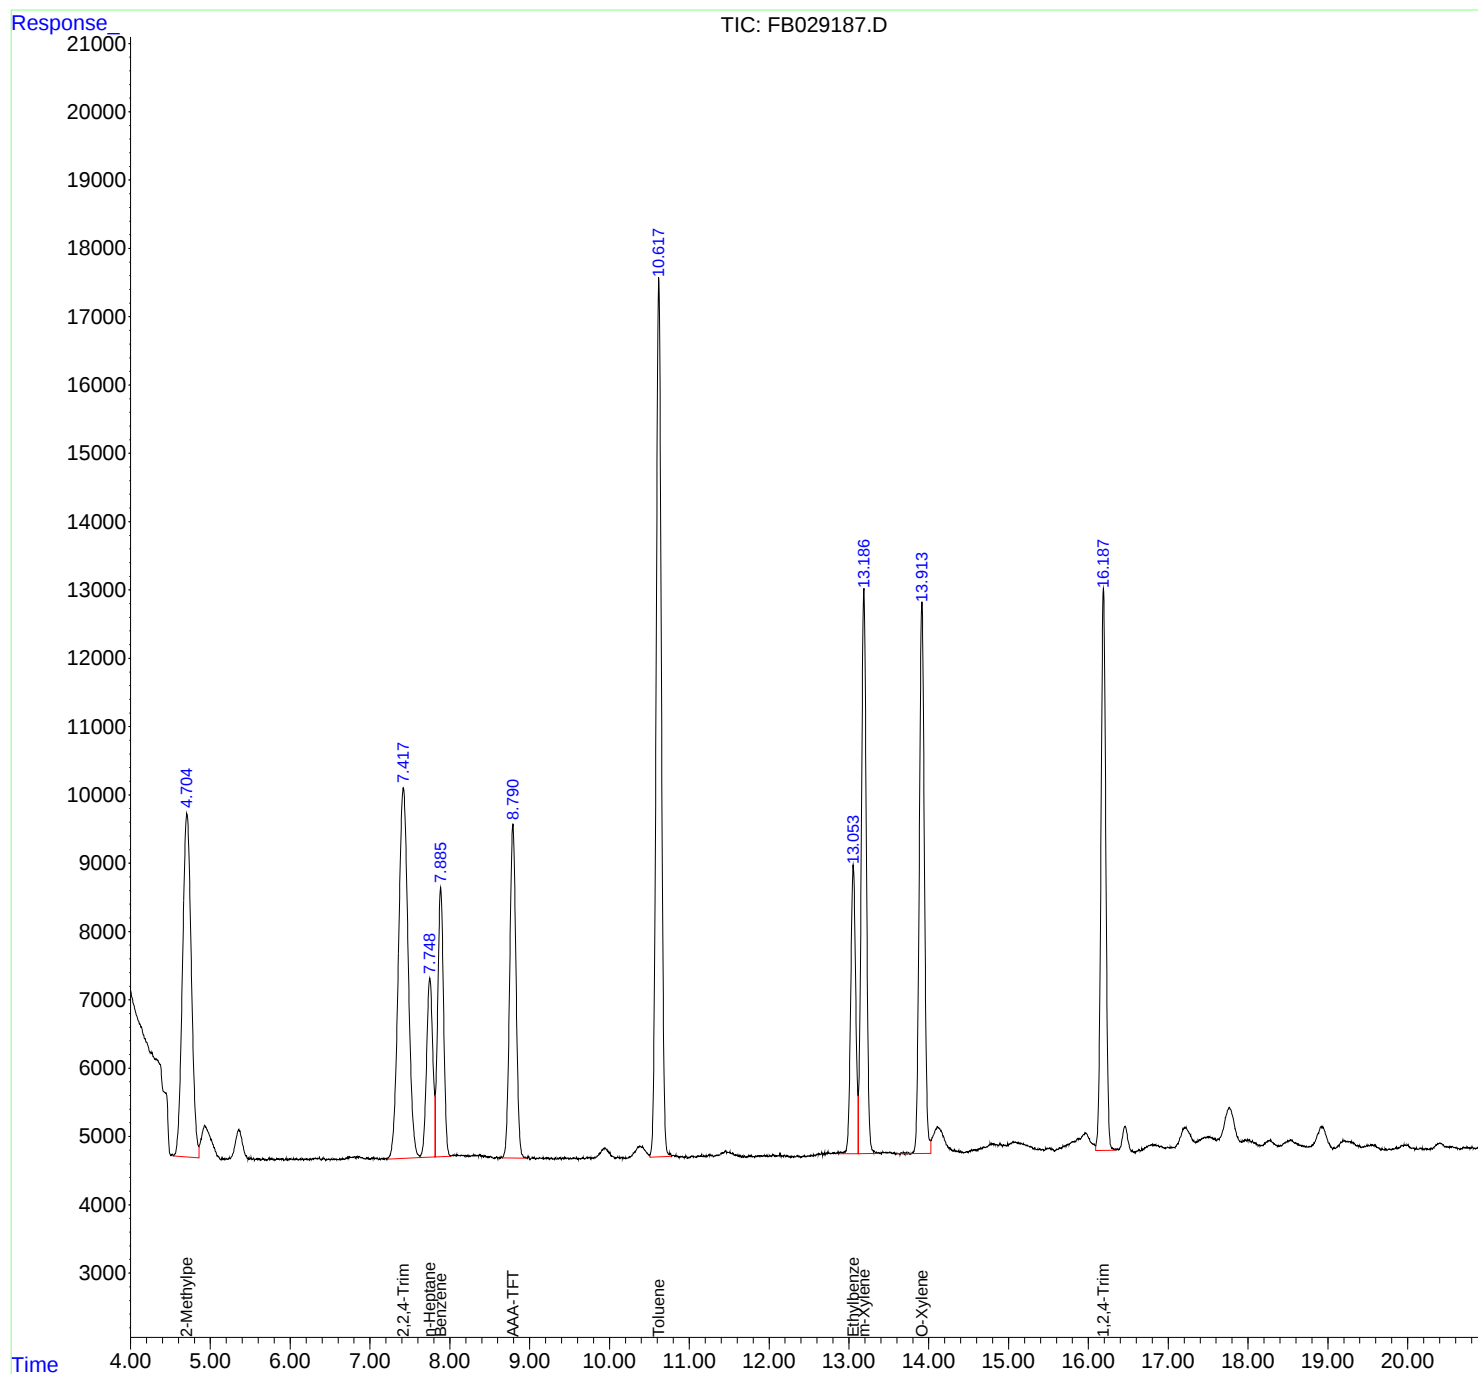


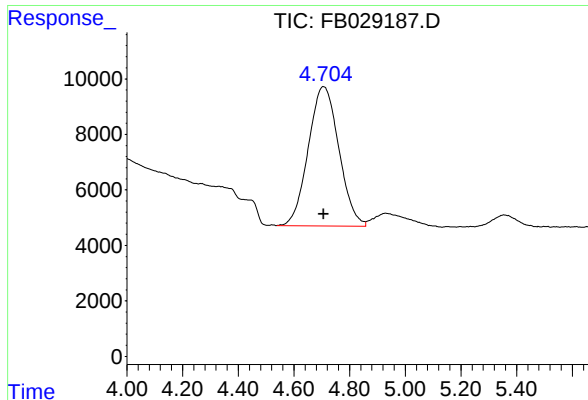

#1 2-Methylpentane


R.T.: 4.705 min
Delta R.T.: -0.002 min
Response: 383597
Conc: 26.20 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0130S3

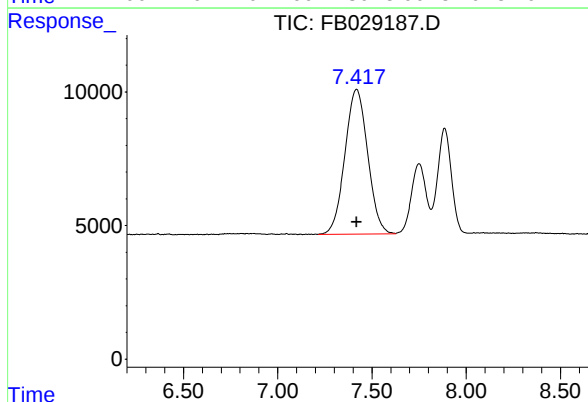


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 454884
Conc: 28.67 ng/ml

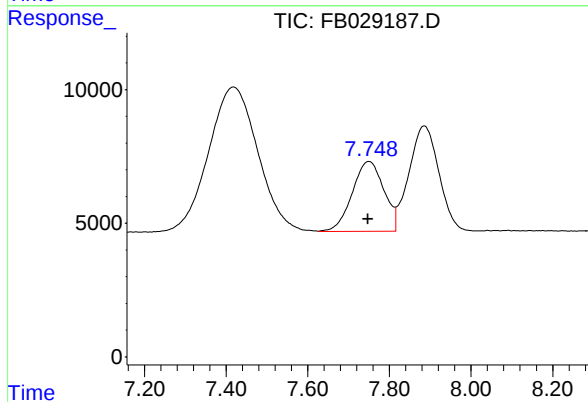


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: 0.002 min
Response: 140996
Conc: 8.44 ng/ml

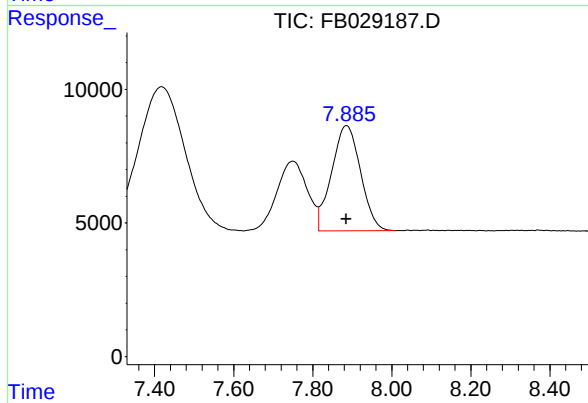

#4 Benzene


R.T.: 7.886 min
Delta R.T.: 0.001 min
Response: 200461
Conc: 9.43 ng/ml

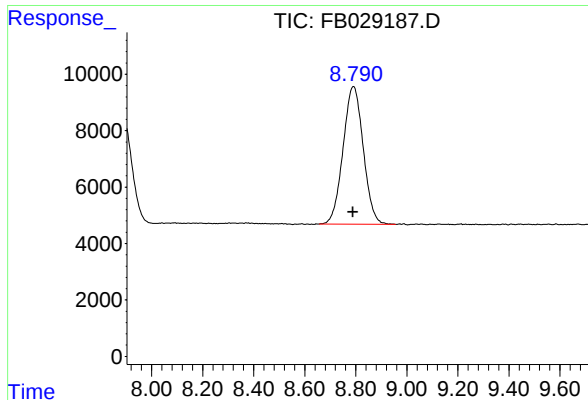

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: 0.002 min
Response: 268332
Conc: 21.96 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0130S3

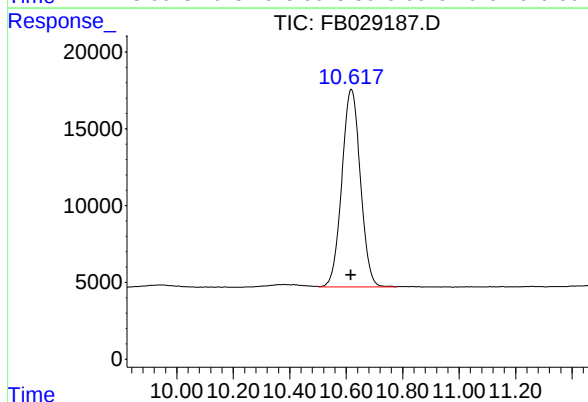


#6 Toluene

R.T.: 10.619 min
Delta R.T.: 0.000 min
Response: 586169
Conc: 29.08 ng/ml

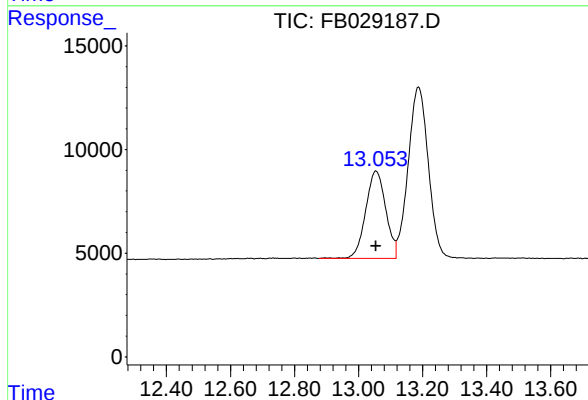


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: 0.000 min
Response: 183675
Conc: 9.58 ng/ml

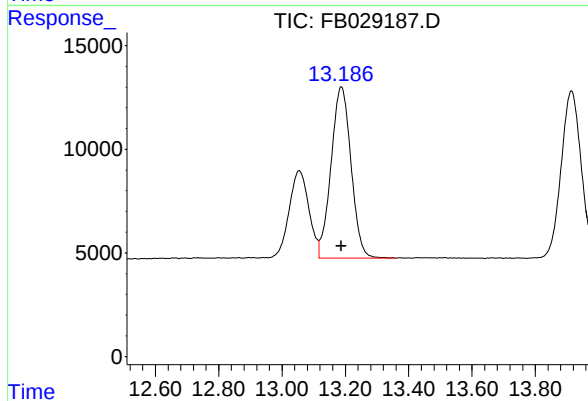

#8 m-Xylene


R.T.: 13.188 min
Delta R.T.: 0.000 min
Response: 362082
Conc: 19.35 ng/ml

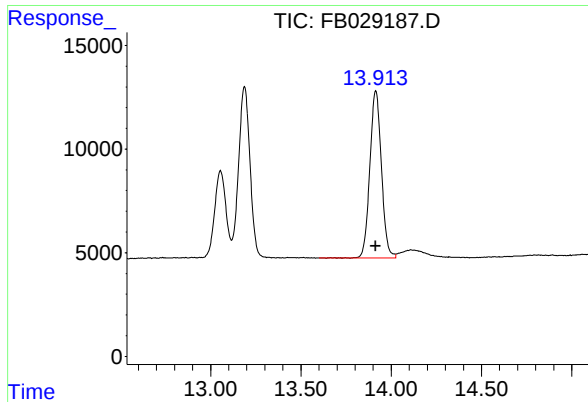

#9 O-Xylene

R.T.: 13.915 min
Delta R.T.: 0.000 min
Response: 358479
Conc: 19.92 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0130S3

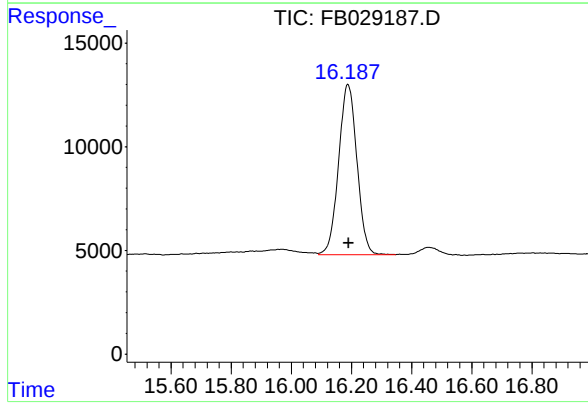

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min
Delta R.T.: -0.001 min
Response: 346843
Conc: 19.46 ng/ml