

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013025\
 Data File : FB031382.D
 Signal(s) : FID2B.CH
 Acq On : 30 Jan 2025 9:47
 Operator : YP/AJ
 Sample : VBF0130S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jan 31 00:54:56 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011525.M
 Quant Title :
 QLast Update : Wed Jan 15 12:01:08 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.786	503550	21.111 ng/ml
Target Compounds			
6) t Toluene	10.614	3383	0.087 ng/ml
8) t m-Xylene	13.185	392	0.010 ng/ml
9) t O-Xylene	13.924	6926	0.194 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	7244	0.256 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013025\
Data File : FB031382.D
Signal(s) : FID2B.CH
Acq On : 30 Jan 2025 9:47
Operator : YP/AJ
Sample : VBF0130S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 31 00:54:56 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011525.M
Quant Title :
QLast Update : Wed Jan 15 12:01:08 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

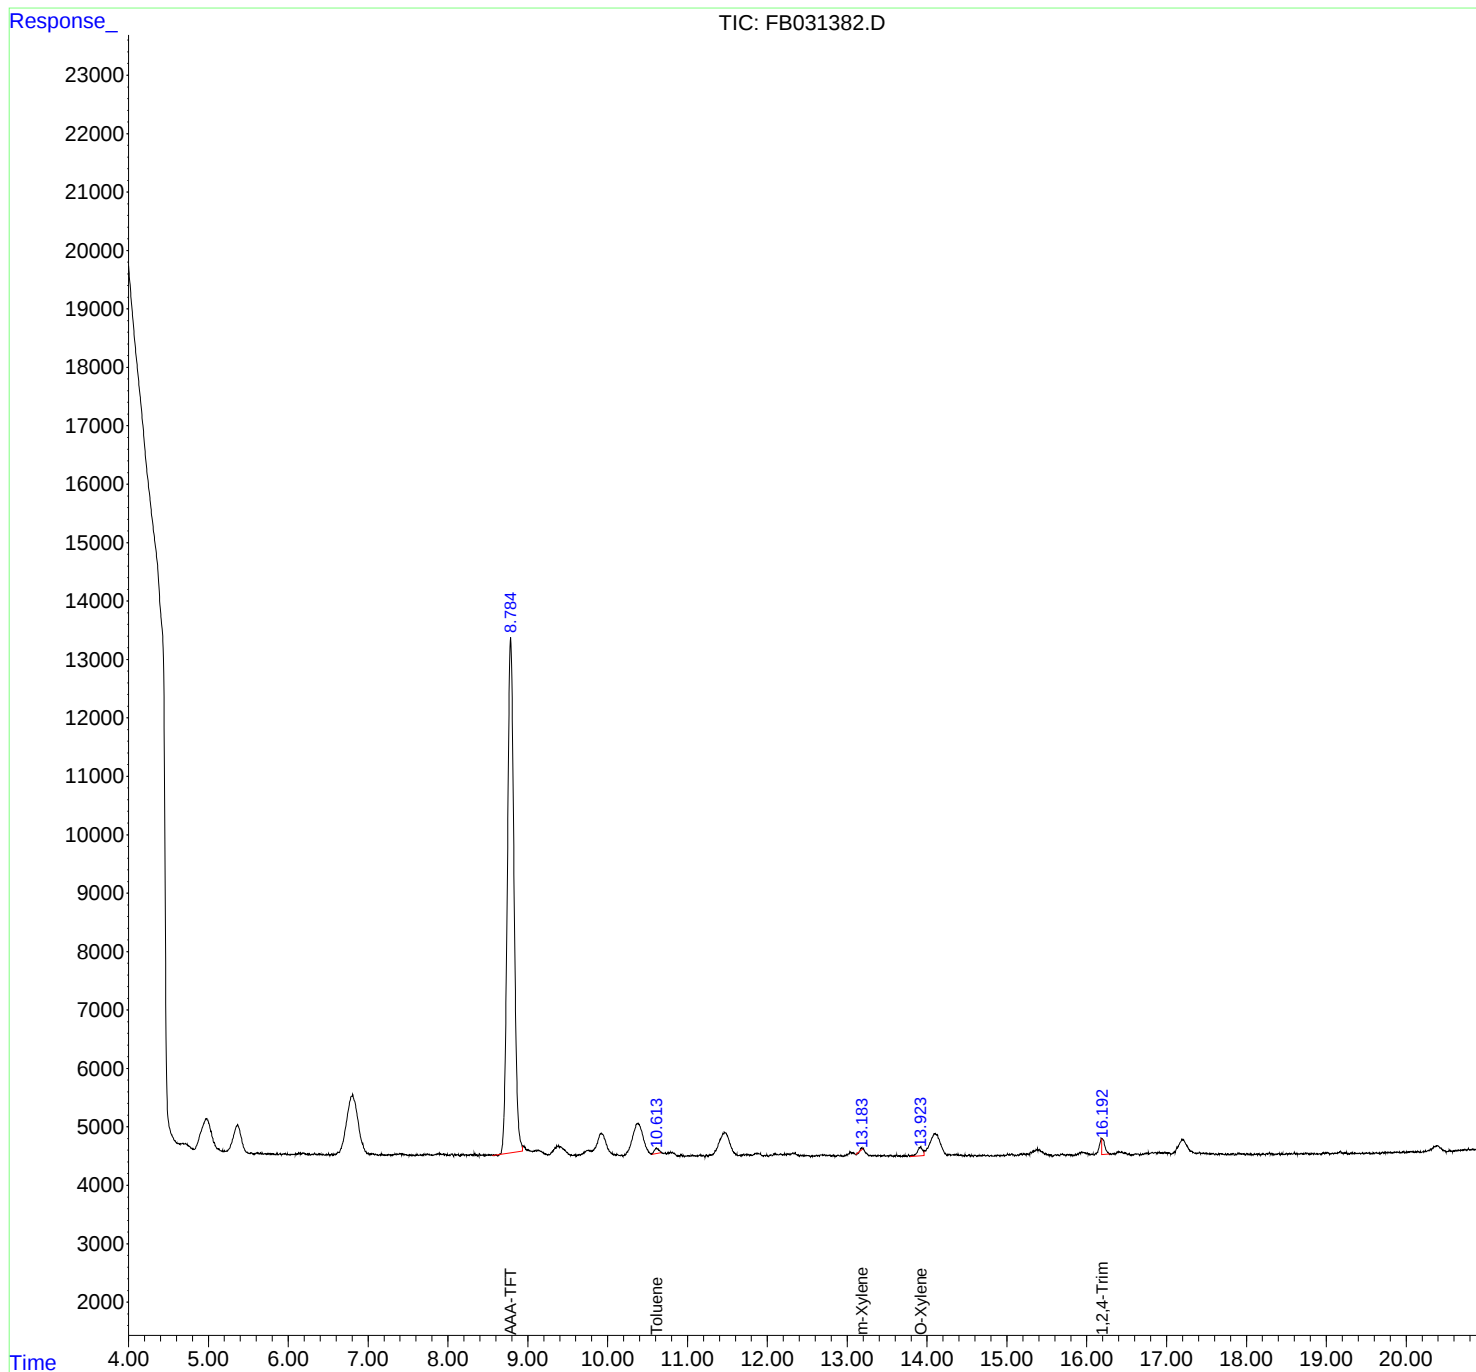


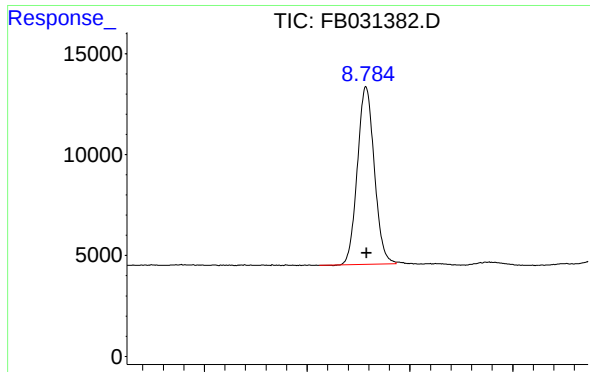

#5 AAA-TFT


R.T.: 8.786 min
Delta R.T.: -0.004 min
Response: 503550
Conc: 21.11 ng/ml

Instrument :
FID_B
ClientSampleId :

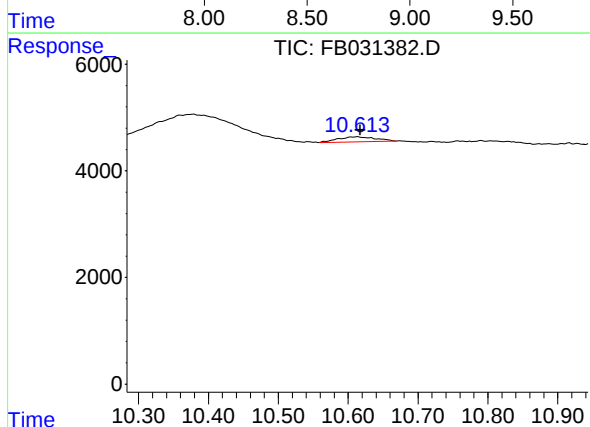


#6 Toluene

R.T.: 10.614 min
Delta R.T.: -0.003 min
Response: 3383
Conc: 0.09 ng/ml

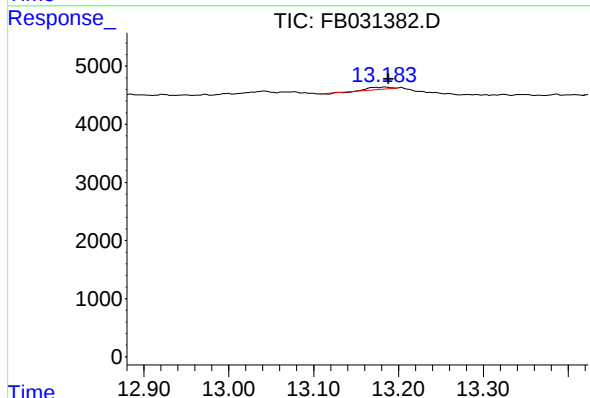


#8 m-Xylene

R.T.: 13.185 min
Delta R.T.: -0.003 min
Response: 392
Conc: 0.01 ng/ml

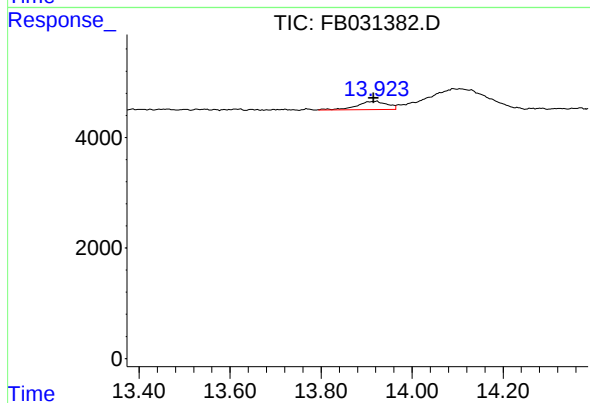

#9 O-Xylene

R.T.: 13.924 min
Delta R.T.: 0.008 min
Response: 6926
Conc: 0.19 ng/ml

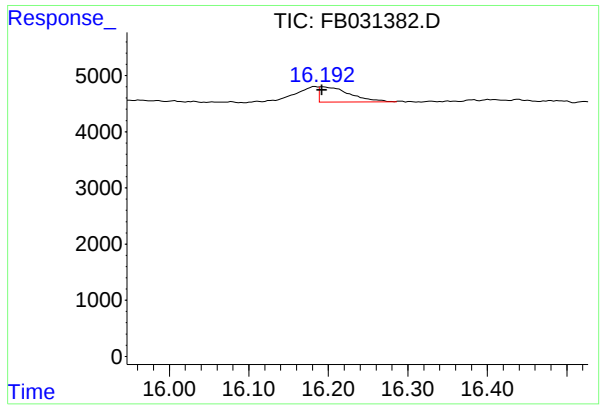

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min

Delta R.T.: 0.002 min

Response: 7244

Conc: 0.26 ng/ml

Instrument :

FID_B

ClientSampleId :