

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE012925\
Data File : FE052138.D
Signal(s) : FID1B.ch
Acq On : 30 Jan 2025 02:58
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 30 06:58:32 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE012325.M
Quant Title :
QLast Update : Fri Jan 24 03:06:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) N-DOTRIACONTANE	19.123	24653	0.236 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE012925\
Data File : FE052138.D
Signal(s) : FID1B.ch
Acq On : 30 Jan 2025 02:58
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 30 06:58:32 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE012325.M
Quant Title :
QLast Update : Fri Jan 24 03:06:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

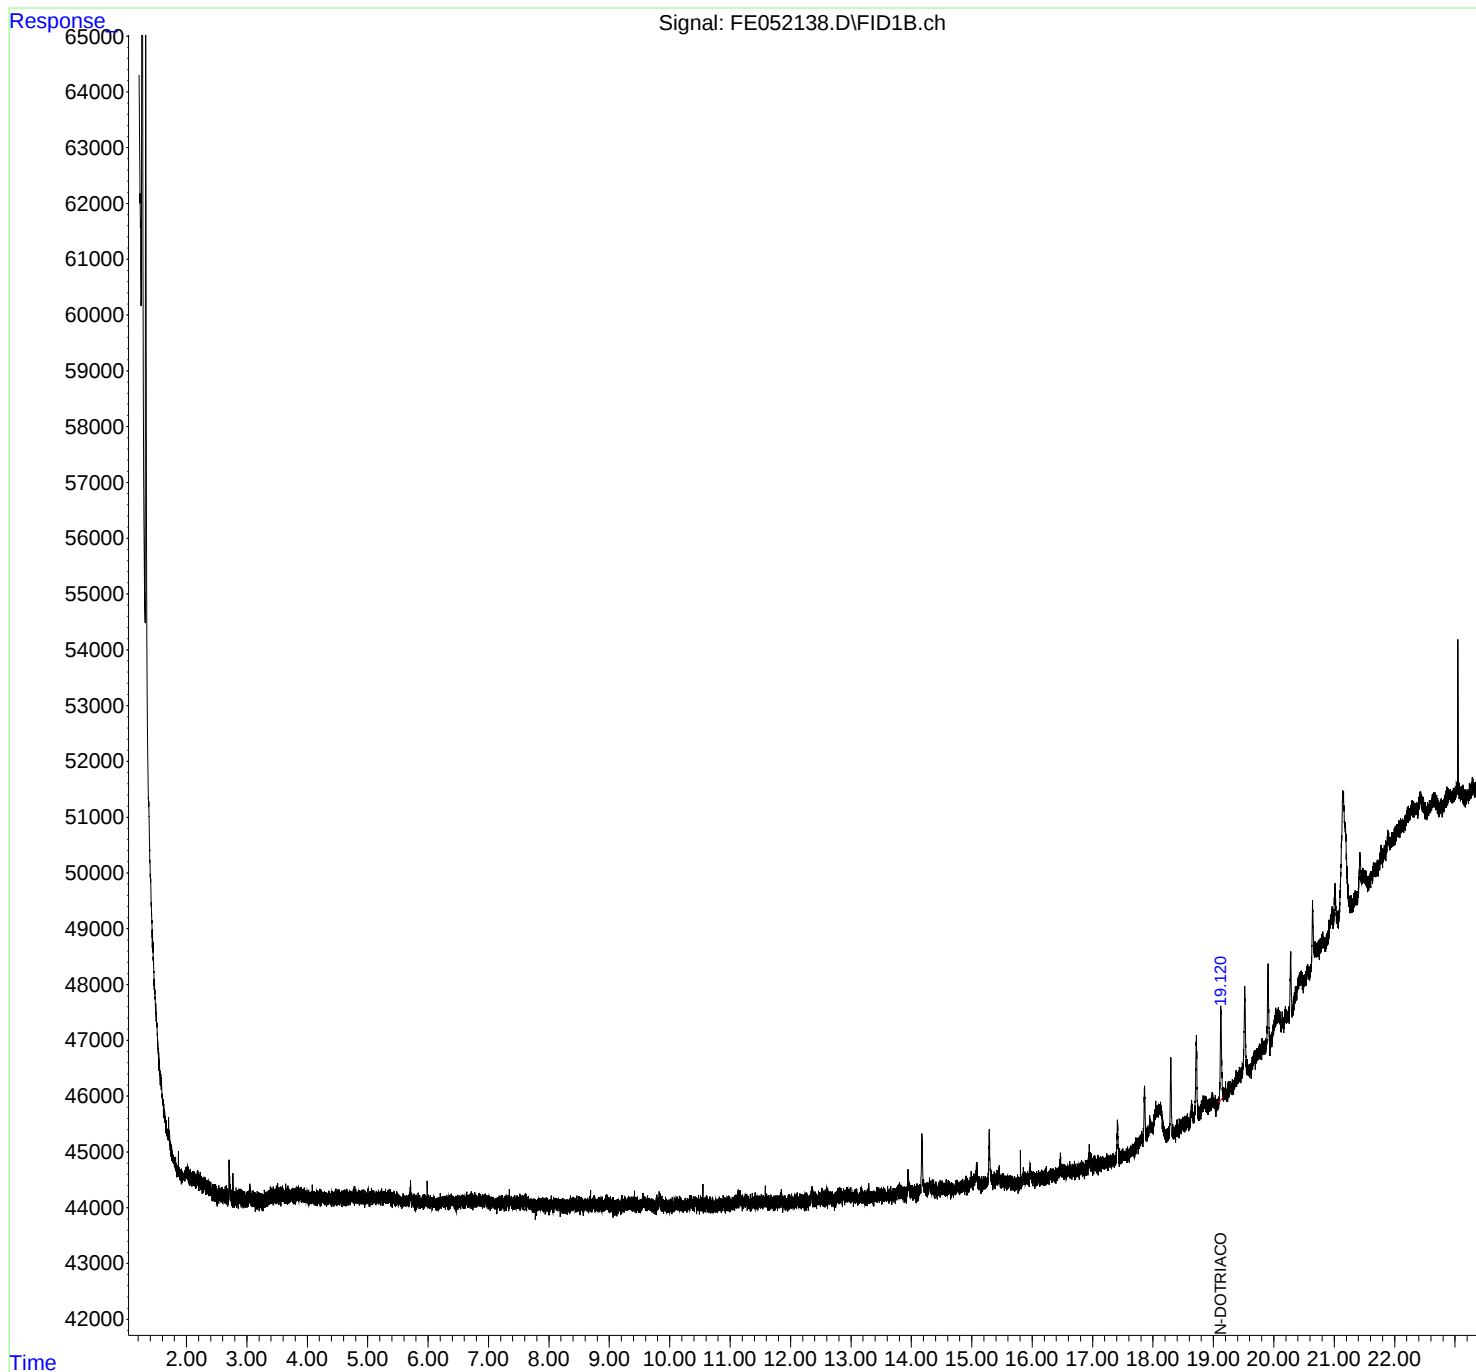


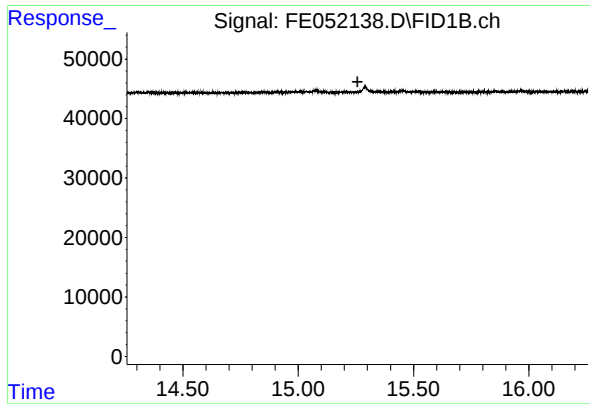

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 15.257 min
Response: 0
Conc: N.D.

Instrument :
FID_B
ClientSampleId :

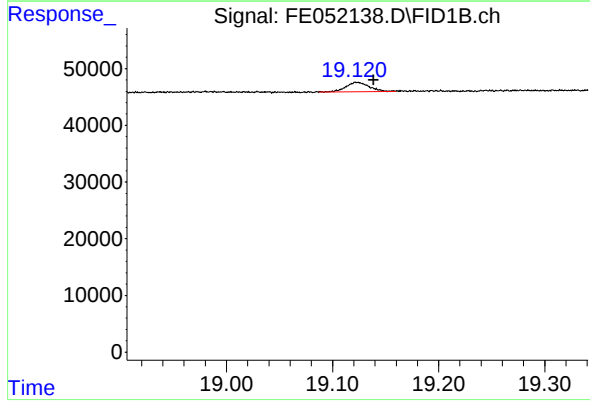

#14 N-DOTRIACONTANE

R.T.: 19.123 min
Delta R.T.: -0.016 min
Response: 24653
Conc: 0.24 ug/ml