

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013025\
 Data File : FB031391.D
 Signal(s) : FID2B.CH
 Acq On : 30 Jan 2025 14:14
 Operator : YP/AJ
 Sample : BSF0130S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0130S2

Integration File: Calibration.e
 Quant Time: Jan 31 00:55:52 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011525.M
 Quant Title :
 QLast Update : Wed Jan 15 12:01:08 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	474668	19.900 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.719	930725	28.080 ng/ml
2) t 2,2,4-Trimethylpentane	7.422	1133361	30.136 ng/ml
3) t n-Heptane	7.752	357132	9.893 ng/ml
4) t Benzene	7.890	439708	10.324 ng/ml
6) t Toluene	10.619	1228104	31.452 ng/ml
7) t Ethylbenzene	13.056	349723	10.099 ng/ml
8) t m-Xylene	13.189	752971	20.144 ng/ml
9) t O-Xylene	13.917	709971	19.935 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	556158	19.638 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013025\
Data File : FB031391.D
Signal(s) : FID2B.CH
Acq On : 30 Jan 2025 14:14
Operator : YP/AJ
Sample : BSF0130S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0130S2

Integration File: Calibration.e
Quant Time: Jan 31 00:55:52 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011525.M
Quant Title :
QLast Update : Wed Jan 15 12:01:08 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

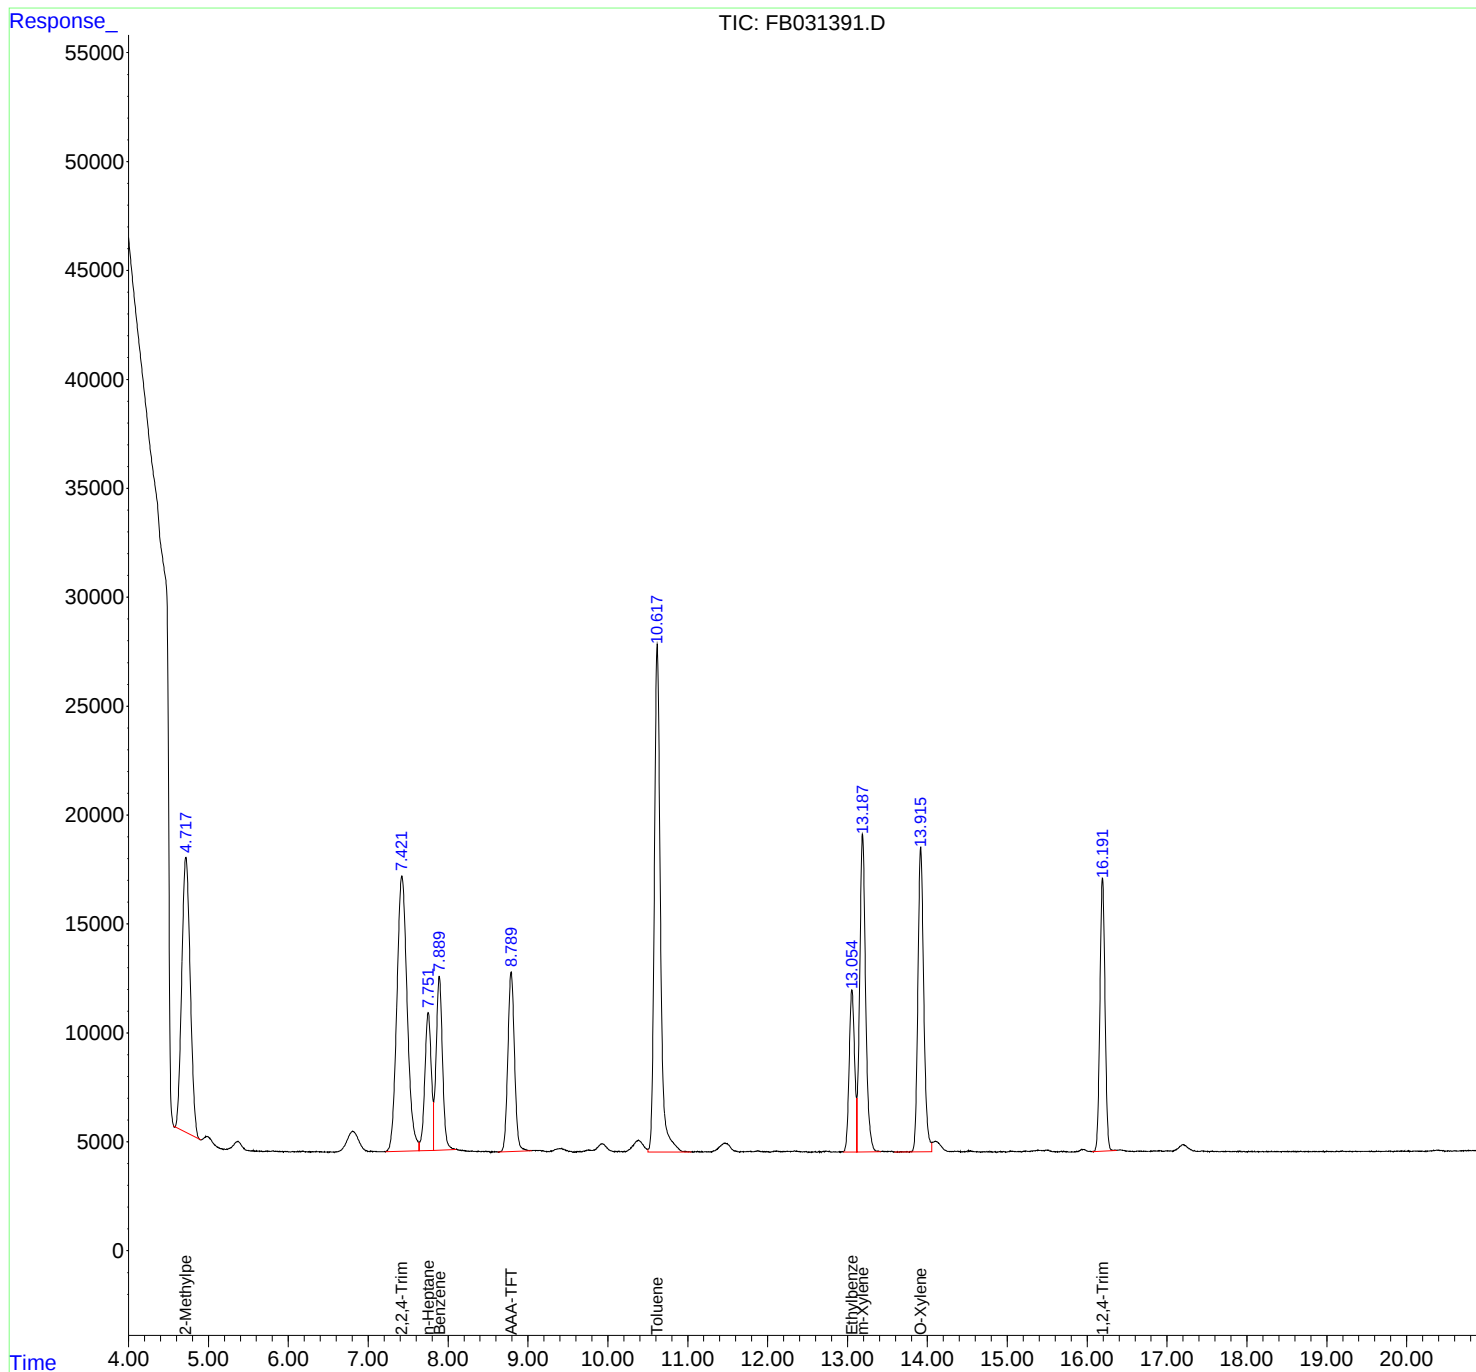


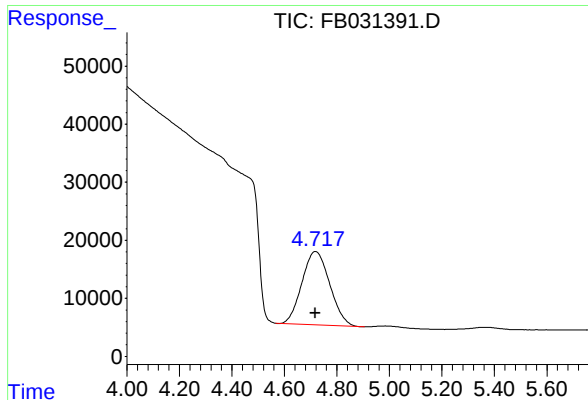

#1 2-Methylpentane


R.T.: 4.719 min
Delta R.T.: 0.000 min
Response: 930725
Conc: 28.08 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0130S2

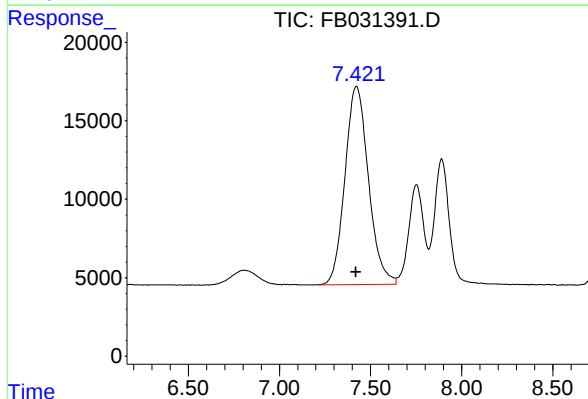


#2 2,2,4-Trimethylpentane

R.T.: 7.422 min
Delta R.T.: 0.002 min
Response: 1133361
Conc: 30.14 ng/ml

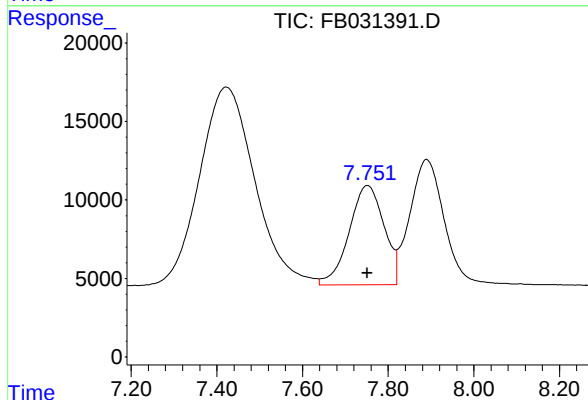


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.001 min
Response: 357132
Conc: 9.89 ng/ml

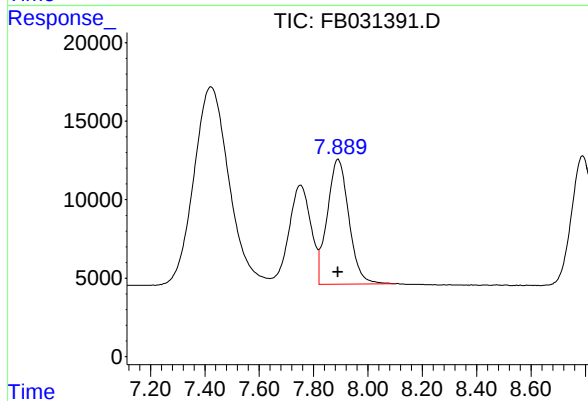

#4 Benzene


R.T.: 7.890 min
Delta R.T.: 0.000 min
Response: 439708
Conc: 10.32 ng/ml

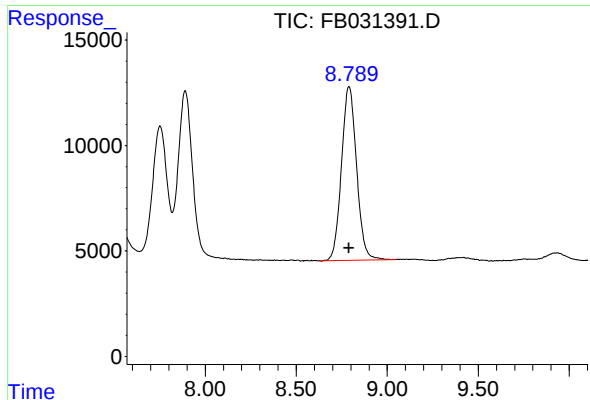

#5 AAA-TFT


R.T.: 8.790 min
Delta R.T.: 0.000 min
Response: 474668
Conc: 19.90 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0130S2

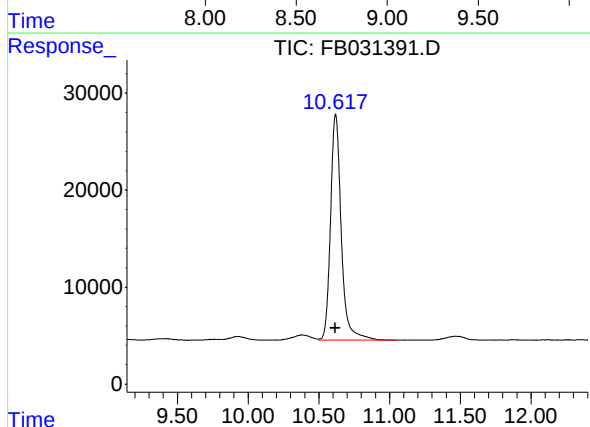


#6 Toluene

R.T.: 10.619 min
Delta R.T.: 0.001 min
Response: 1228104
Conc: 31.45 ng/ml

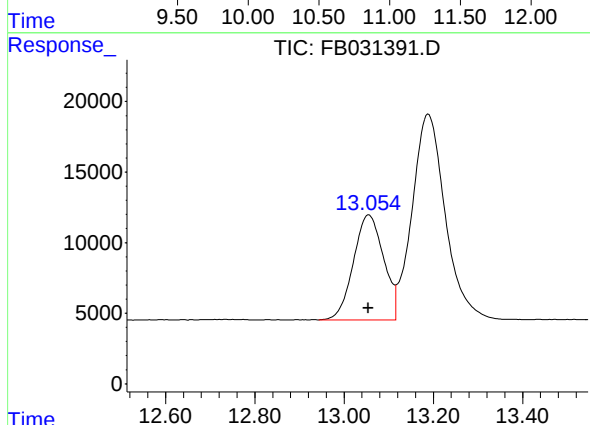


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: 0.001 min
Response: 349723
Conc: 10.10 ng/ml

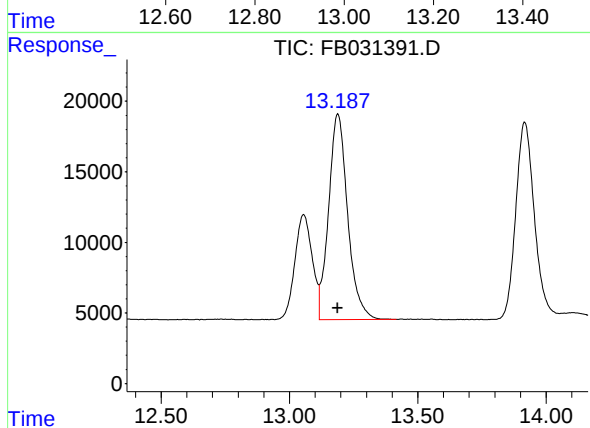

#8 m-Xylene


R.T.: 13.189 min
Delta R.T.: 0.000 min
Response: 752971
Conc: 20.14 ng/ml

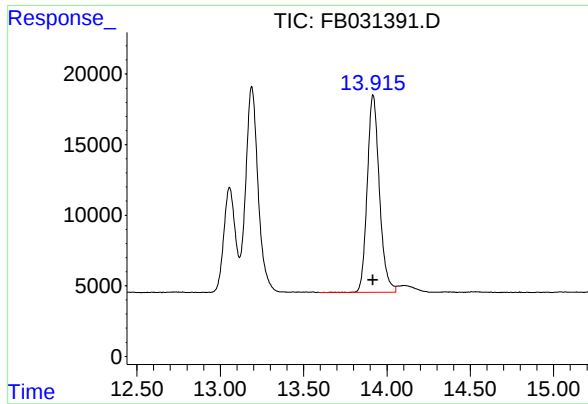

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: 0.001 min
Response: 709971
Conc: 19.94 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0130S2

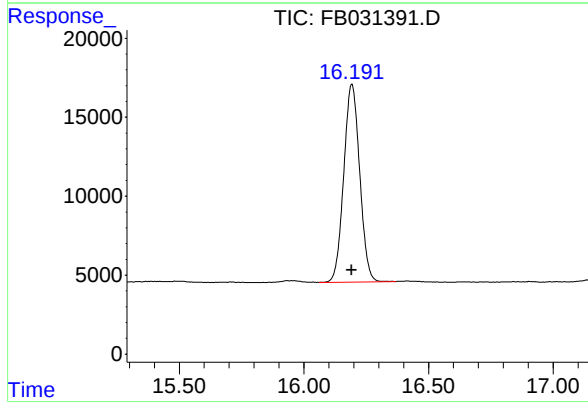

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.000 min
Response: 556158
Conc: 19.64 ng/ml