

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013025\
 Data File : FB031410.D
 Signal(s) : FID2B.CH
 Acq On : 30 Jan 2025 23:59
 Operator : YP/AJ
 Sample : BSF0130S3
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0130S3

Integration File: Calibration.e
 Quant Time: Jan 31 00:57:40 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011525.M
 Quant Title :
 QLast Update : Wed Jan 15 12:01:08 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	474372	19.888 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.719	1018766	30.736 ng/ml
2) t 2,2,4-Trimethylpentane	7.423	1231639	32.750 ng/ml
3) t n-Heptane	7.752	394364	10.924 ng/ml
4) t Benzene	7.891	491645	11.544 ng/ml
6) t Toluene	10.620	1319716	33.799 ng/ml
7) t Ethylbenzene	13.056	373835	10.796 ng/ml
8) t m-Xylene	13.190	803264	21.490 ng/ml
9) t O-Xylene	13.918	761261	21.376 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	581733	20.541 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013025\
Data File : FB031410.D
Signal(s) : FID2B.CH
Acq On : 30 Jan 2025 23:59
Operator : YP/AJ
Sample : BSF0130S3
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0130S3

Integration File: Calibration.e
Quant Time: Jan 31 00:57:40 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011525.M
Quant Title :
QLast Update : Wed Jan 15 12:01:08 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

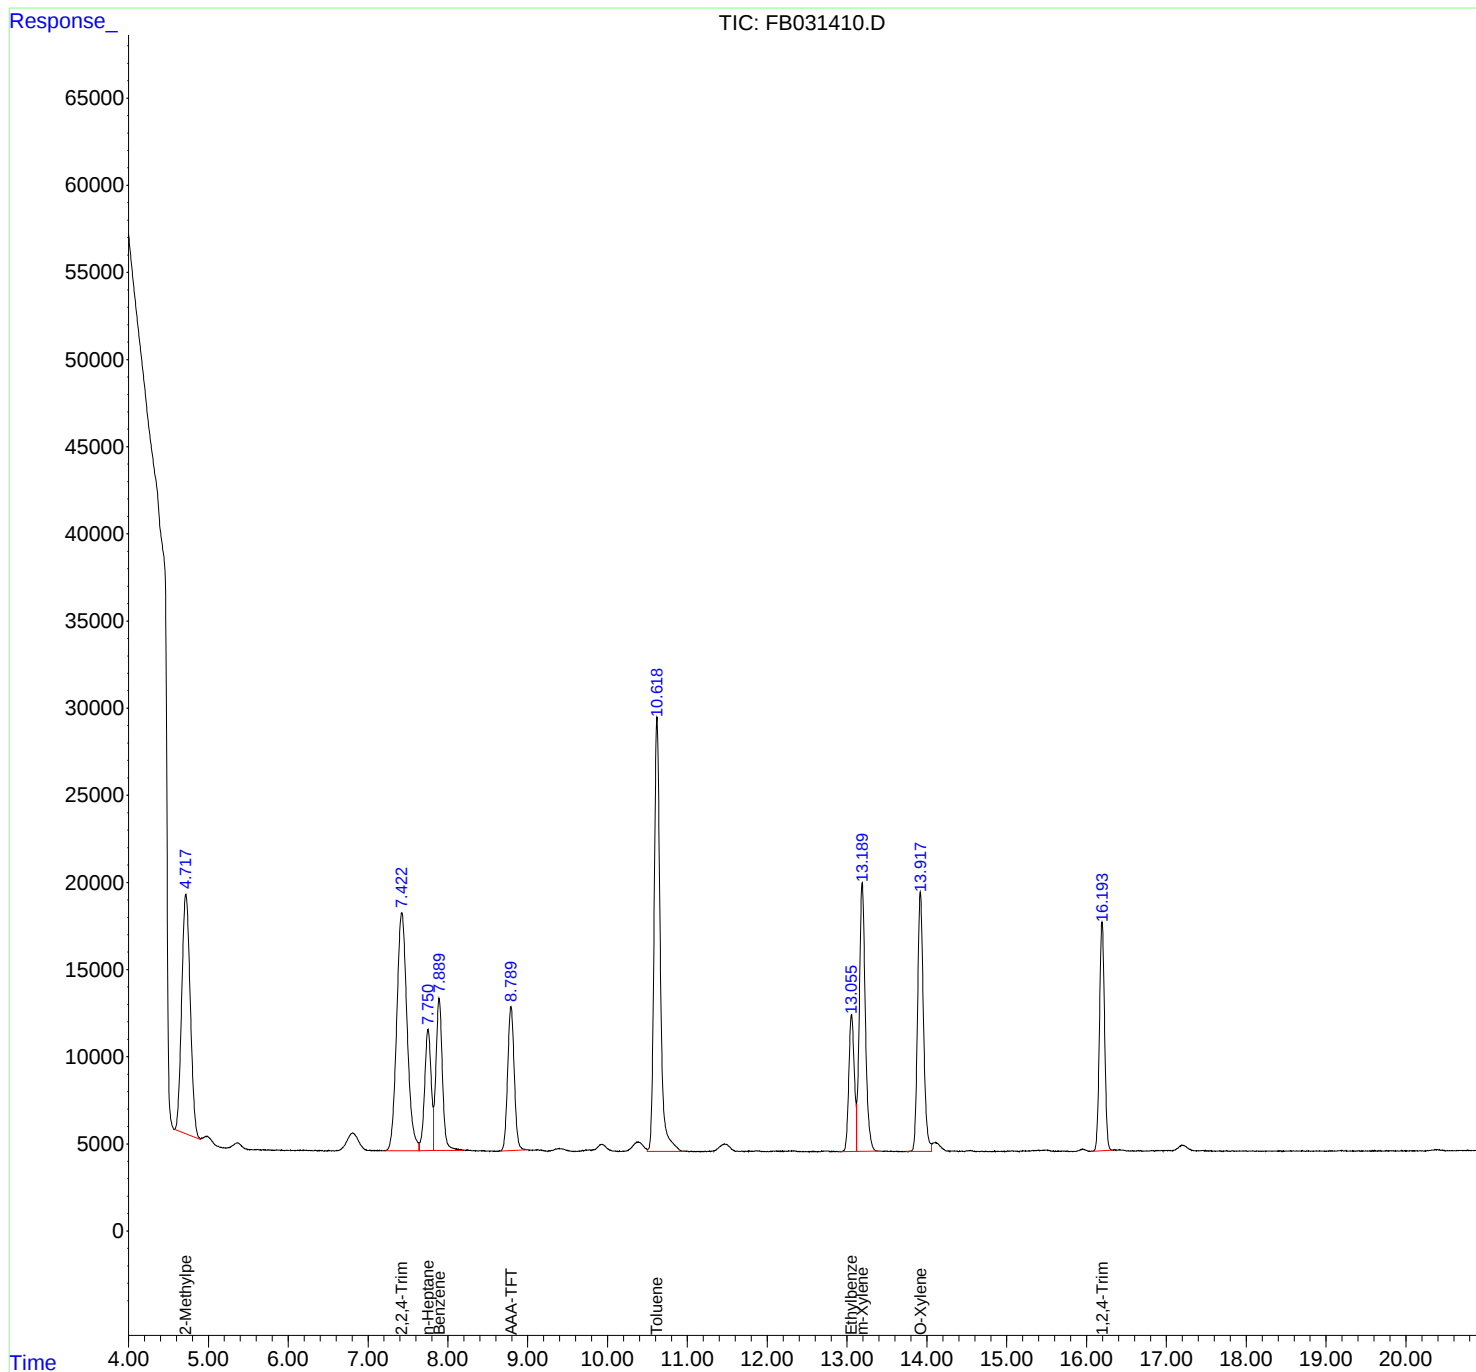


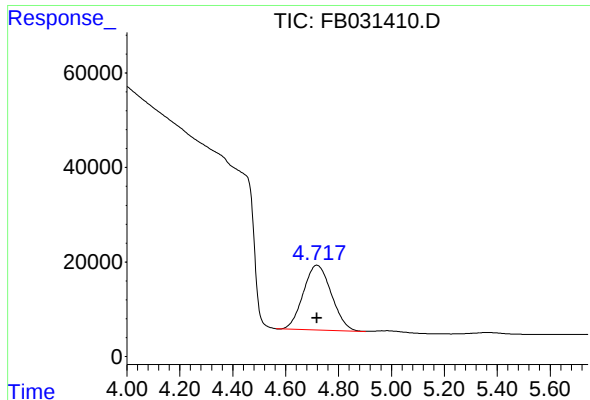

#1 2-Methylpentane


R.T.: 4.719 min
Delta R.T.: 0.000 min
Response: 1018766
Conc: 30.74 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0130S3

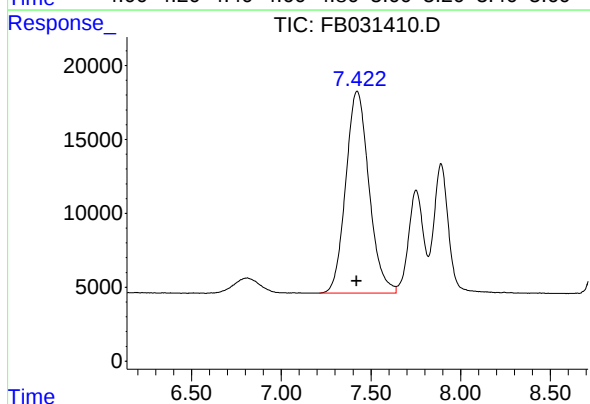


#2 2,2,4-Trimethylpentane

R.T.: 7.423 min
Delta R.T.: 0.004 min
Response: 1231639
Conc: 32.75 ng/ml

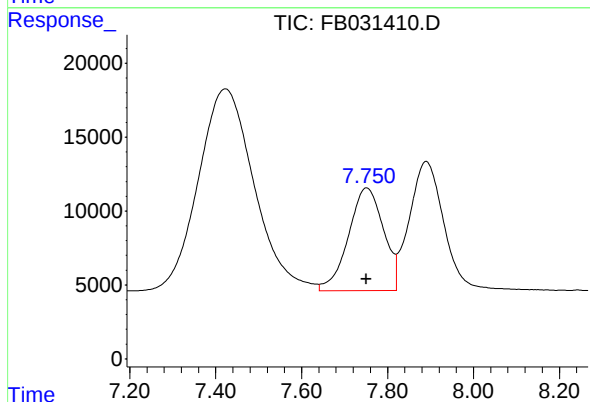


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.000 min
Response: 394364
Conc: 10.92 ng/ml

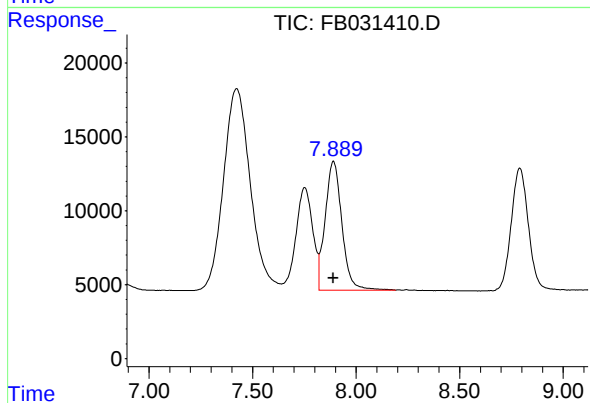

#4 Benzene


R.T.: 7.891 min
Delta R.T.: 0.000 min
Response: 491645
Conc: 11.54 ng/ml

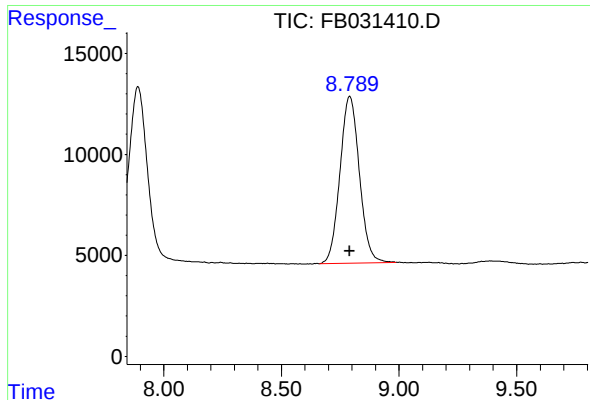

#5 AAA-TFT


R.T.: 8.790 min
Delta R.T.: 0.000 min
Response: 474372
Conc: 19.89 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0130S3

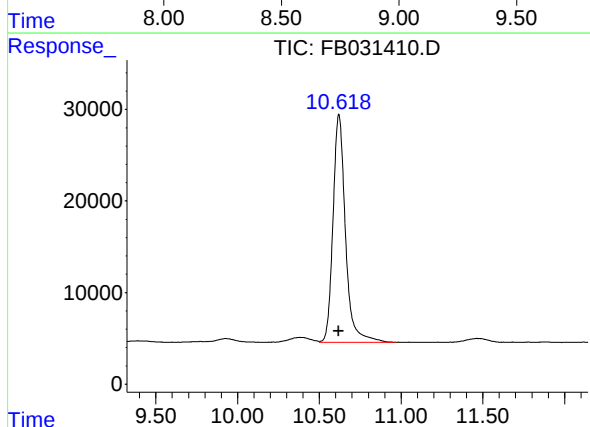


#6 Toluene

R.T.: 10.620 min
Delta R.T.: 0.002 min
Response: 1319716
Conc: 33.80 ng/ml

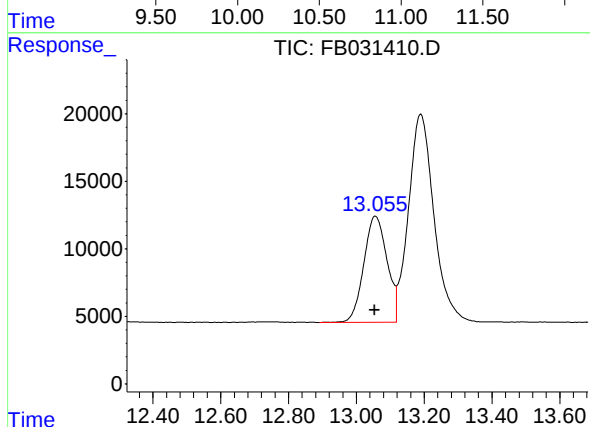


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: 0.002 min
Response: 373835
Conc: 10.80 ng/ml

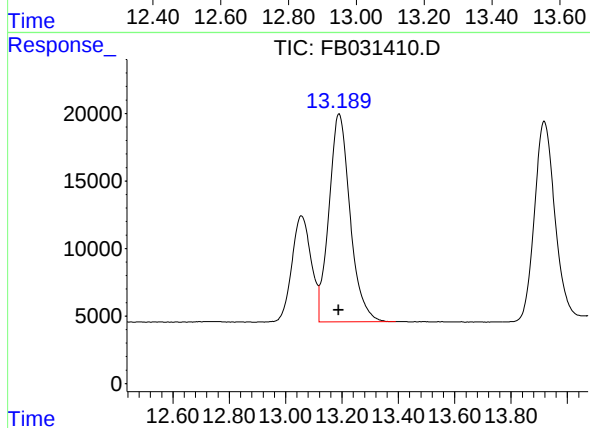

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: 0.002 min
Response: 803264
Conc: 21.49 ng/ml

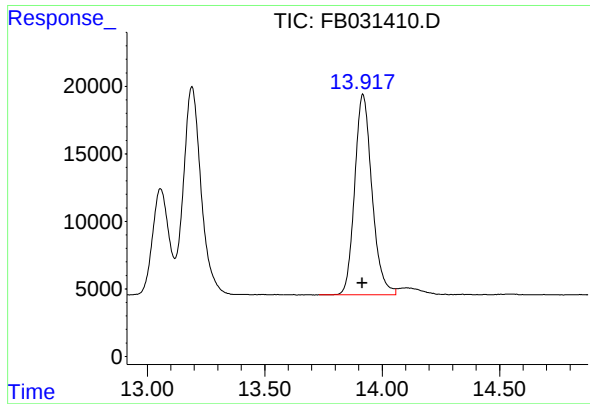

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.002 min
Response: 761261
Conc: 21.38 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0130S3

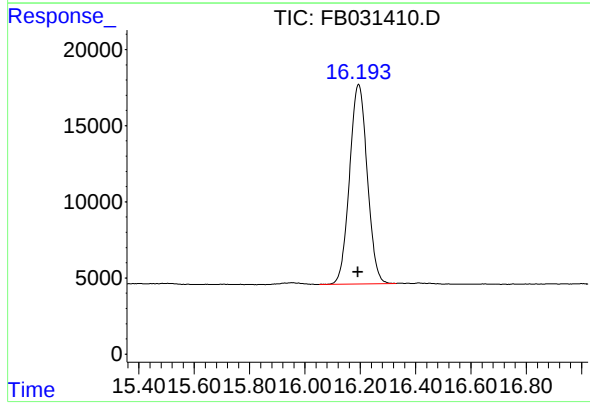

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: 0.002 min
Response: 581733
Conc: 20.54 ng/ml