

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013120\
 Data File : FB023594.D
 Signal(s) : FID2B.CH
 Acq On : 31 Jan 2020 9:41
 Operator : DD/AJ
 Sample : BSF0131S1
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jan 31 22:36:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
 Quant Title :
 QLast Update : Thu Jan 16 11:42:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	479322	20.179 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	904063	28.609 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	1040248	30.637 ng/ml
3) t n-Heptane	7.754	334920	10.001 ng/ml
4) t Benzene	7.888	411676	10.081 ng/ml
6) t Toluene	10.626	1192728	30.182 ng/ml
7) t Ethylbenzene	13.066	367794	9.848 ng/ml
8) t m-Xylene	13.199	705090	19.828 ng/ml
9) t O-Xylene	13.926	686225	19.860 ng/ml
10) t 1,2,4-Trimethylbenzene	16.204	597015	20.417 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013120\
Data File : FB023594.D
Signal(s) : FID2B.CH
Acq On : 31 Jan 2020 9:41
Operator : DD/AJ
Sample : BSF0131S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jan 31 22:36:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
Quant Title :
QLast Update : Thu Jan 16 11:42:55 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

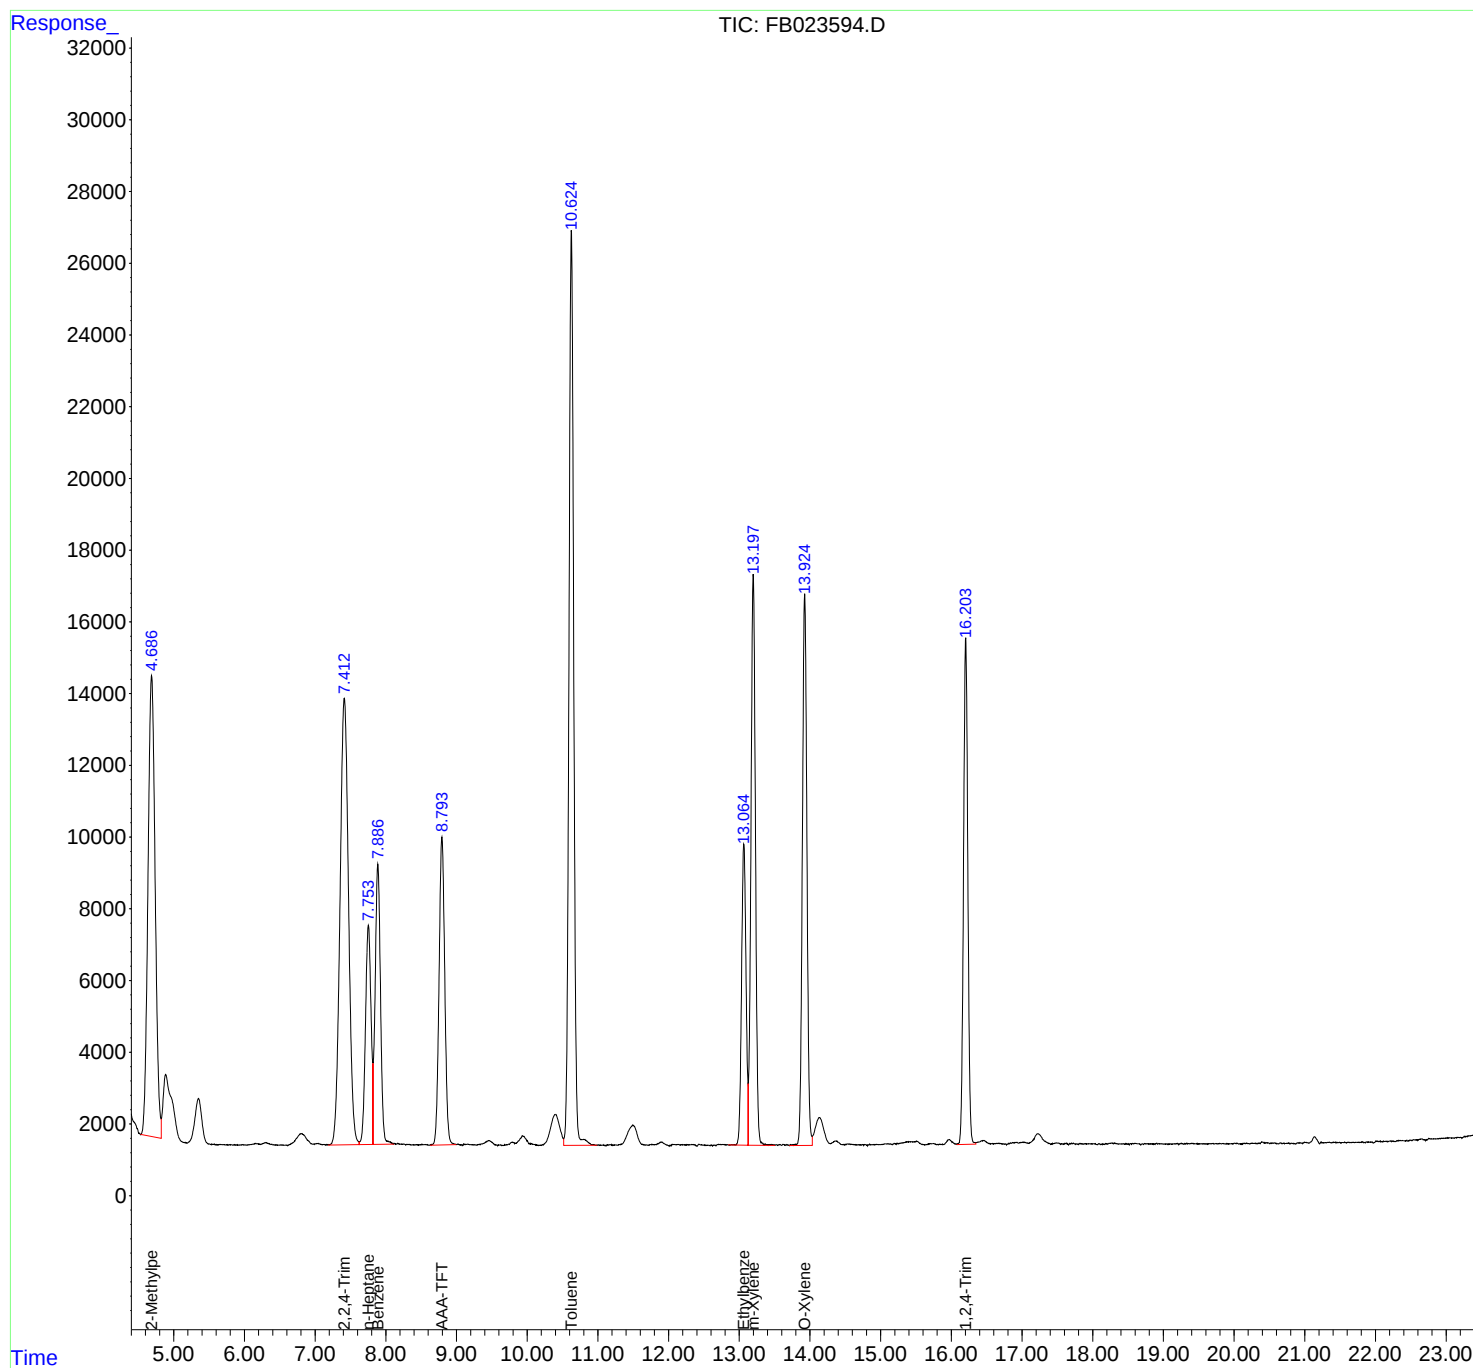

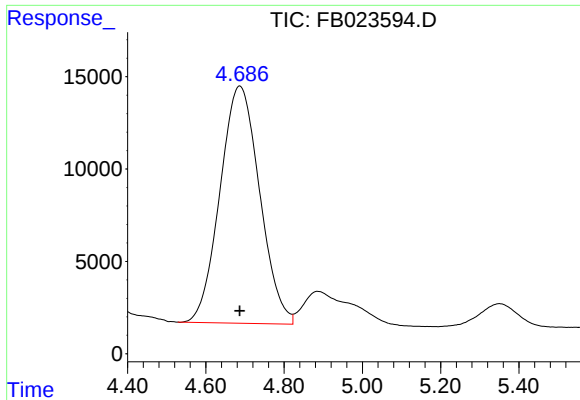


#1 2-Methylpentane

R.T.: 4.687 min
Delta R.T.: 0.000 min
Response: 904063
Conc: 28.61 ng/ml

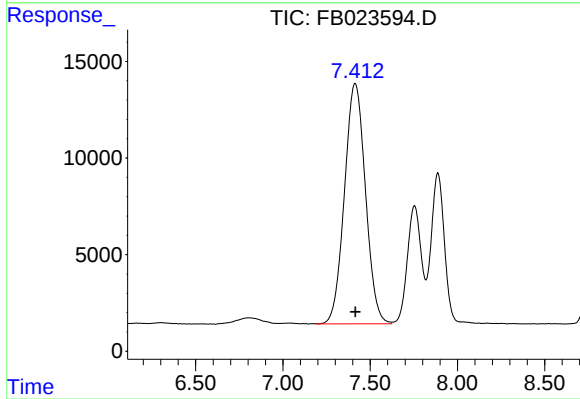


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: -0.001 min
Response: 1040248
Conc: 30.64 ng/ml

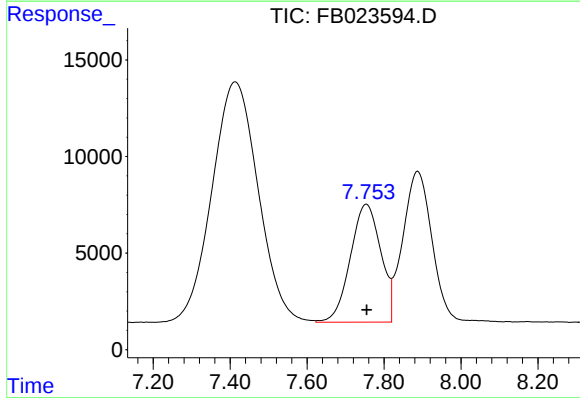


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: -0.001 min
Response: 334920
Conc: 10.00 ng/ml

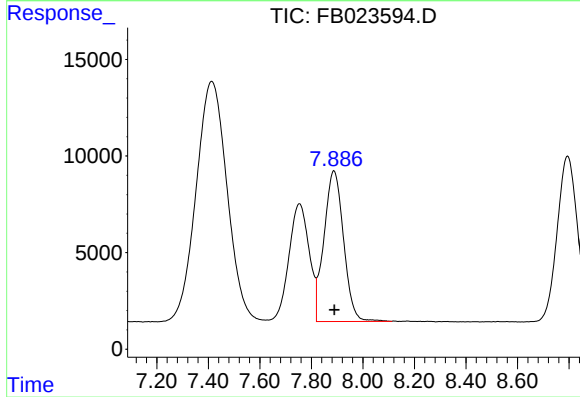


#4 Benzene

R.T.: 7.888 min
Delta R.T.: -0.002 min
Response: 411676
Conc: 10.08 ng/ml

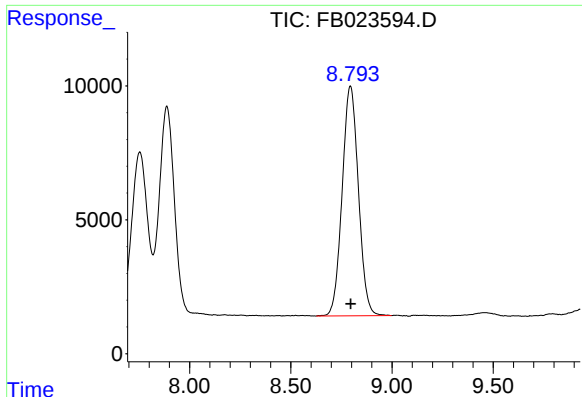


#5 AAA-TFT

R.T.: 8.795 min
Delta R.T.: -0.002 min
Response: 479322
Conc: 20.18 ng/ml

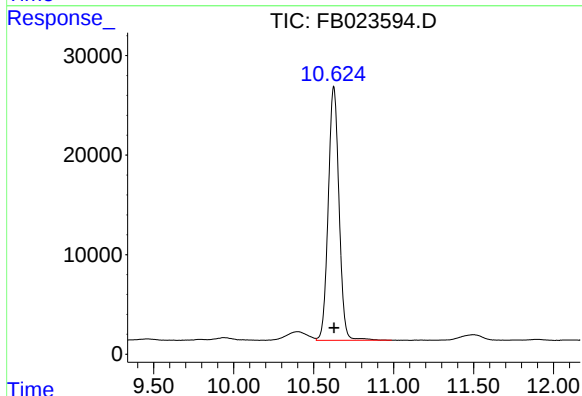


#6 Toluene

R.T.: 10.626 min
Delta R.T.: -0.002 min
Response: 1192728
Conc: 30.18 ng/ml

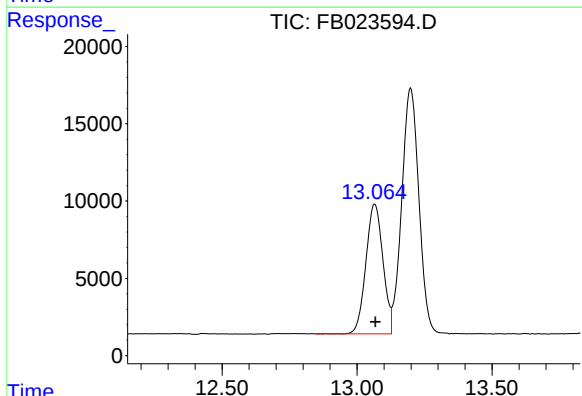


#7 Ethylbenzene

R.T.: 13.066 min
Delta R.T.: -0.003 min
Response: 367794
Conc: 9.85 ng/ml

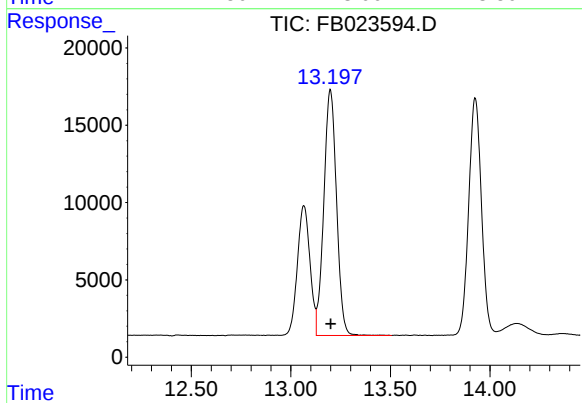


#8 m-Xylene

R.T.: 13.199 min
Delta R.T.: -0.002 min
Response: 705090
Conc: 19.83 ng/ml

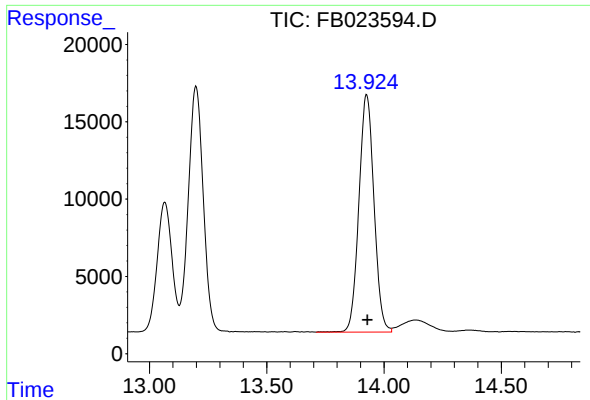

#9 O-Xylene

R.T.: 13.926 min
Delta R.T.: -0.003 min
Response: 686225
Conc: 19.86 ng/ml

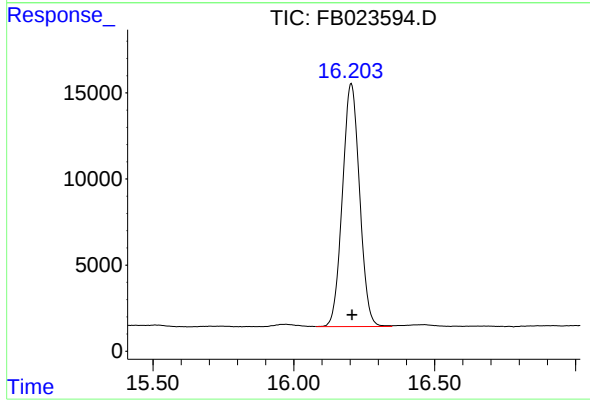

#10 1,2,4-Trimethylbenzene

R.T.: 16.204 min
Delta R.T.: -0.003 min
Response: 597015
Conc: 20.42 ng/ml