

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013123\
 Data File : FB029190.D
 Signal(s) : FID2B.CH
 Acq On : 31 Jan 2023 10:03
 Operator : AJ/MA
 Sample : 10 GRO STD
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jan 31 11:15:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB013123.M
 Quant Title :
 QLast Update : Tue Jan 31 11:15:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.788	130421	11.049 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.707	177481	15.770 ng/ml
2) t	2,2,4-Trimethylpentane	7.414	209770	15.184 ng/ml
3) t	n-Heptane	7.748	62107	5.143 ng/ml
4) t	Benzene	7.883	89561	5.216 ng/ml
6) t	Toluene	10.617	268168	16.021 ng/ml
7) t	Ethylbenzene	13.053	86811	5.245 ng/ml
8) t	m-Xylene	13.186	171632	10.401 ng/ml
9) t	O-Xylene	13.912	171086	10.411 ng/ml
10) t	1,2,4-Trimethylbenzene	16.187	175039	9.973 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013123\
Data File : FB029190.D
Signal(s) : FID2B.CH
Acq On : 31 Jan 2023 10:03
Operator : AJ/MA
Sample : 10 GRO STD
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jan 31 11:15:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB013123.M
Quant Title :
QLast Update : Tue Jan 31 11:15:04 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

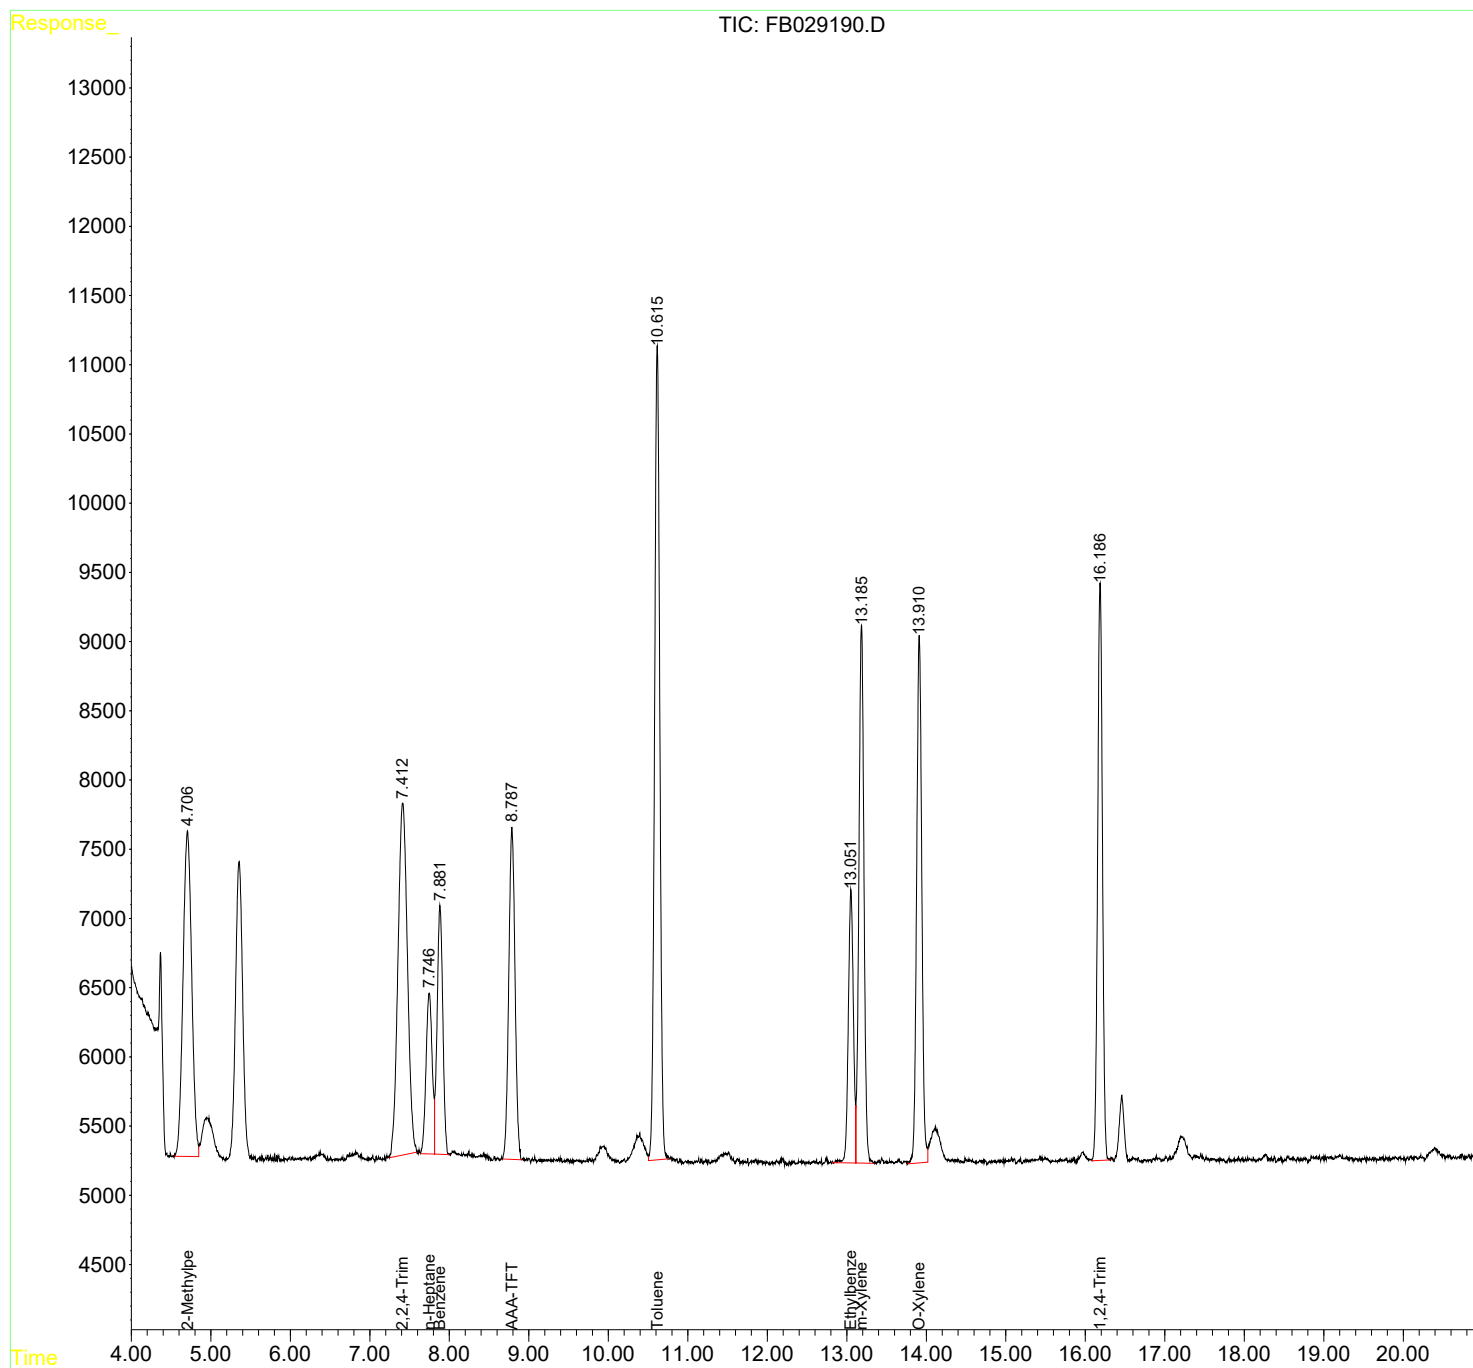

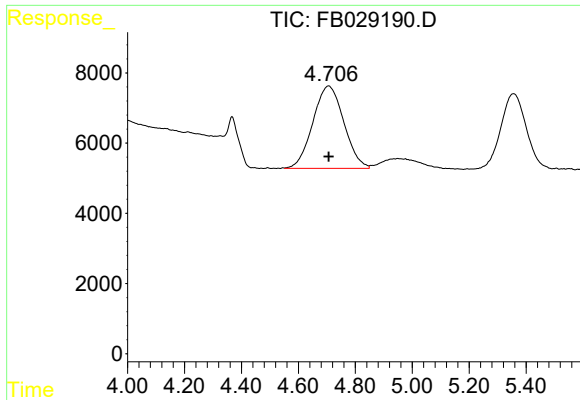


#1 2-Methylpentane

R.T.: 4.707 min
Delta R.T.: 0.000 min
Response: 177481
Conc: 15.77 ng/ml

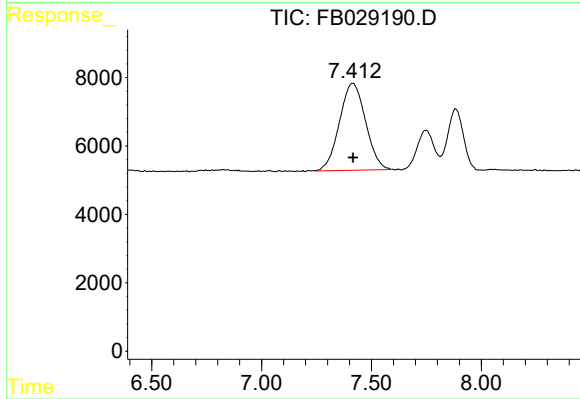


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: -0.003 min
Response: 209770
Conc: 15.18 ng/ml

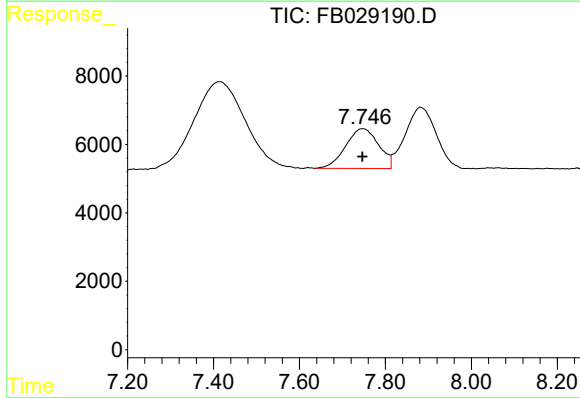


#3 n-Heptane

R.T.: 7.748 min
Delta R.T.: 0.001 min
Response: 62107
Conc: 5.14 ng/ml

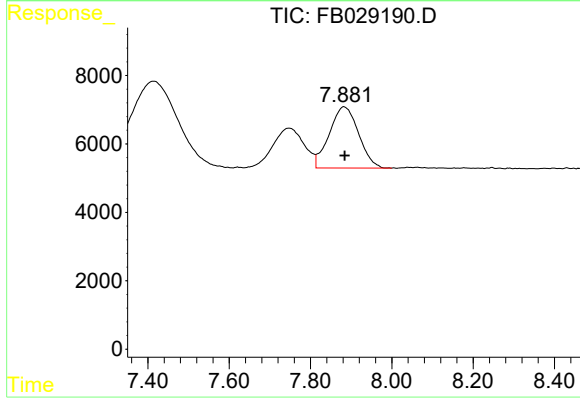


#4 Benzene

R.T.: 7.883 min
Delta R.T.: -0.002 min
Response: 89561
Conc: 5.22 ng/ml

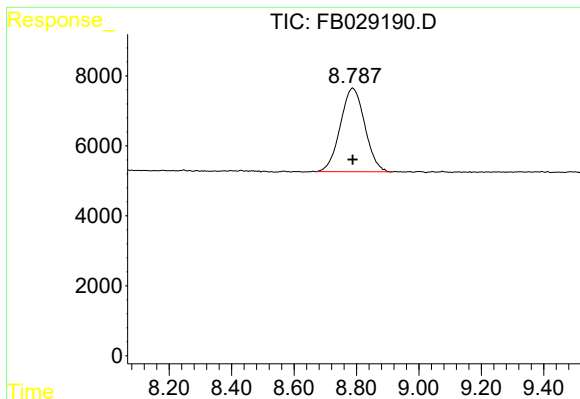


#5 AAA-TFT

R.T.: 8.788 min
Delta R.T.: 0.000 min
Response: 130421
Conc: 11.05 ng/ml

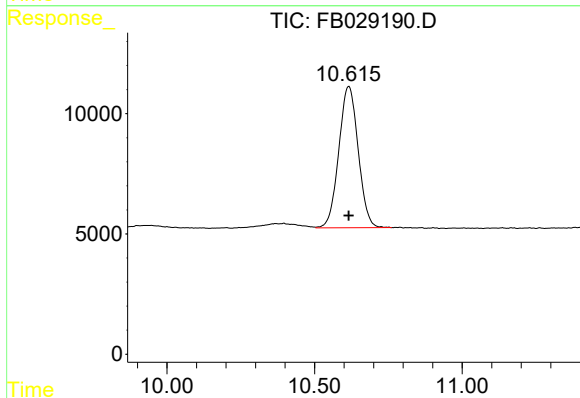


#6 Toluene

R.T.: 10.617 min
Delta R.T.: 0.000 min
Response: 268168
Conc: 16.02 ng/ml

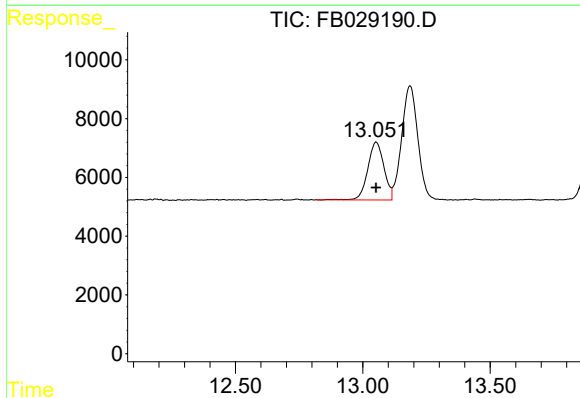


#7 Ethylbenzene

R.T.: 13.053 min
Delta R.T.: 0.000 min
Response: 86811
Conc: 5.24 ng/ml

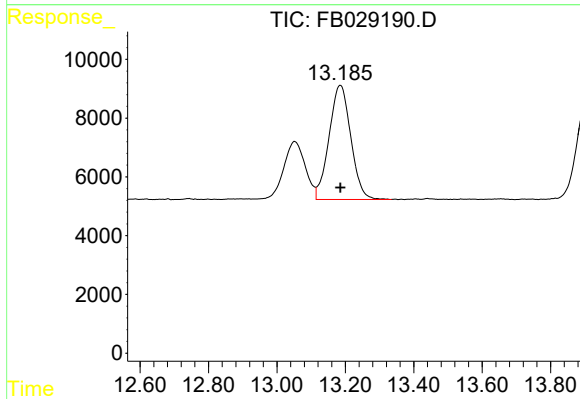


#8 m-Xylene

R.T.: 13.186 min
Delta R.T.: 0.000 min
Response: 171632
Conc: 10.40 ng/ml

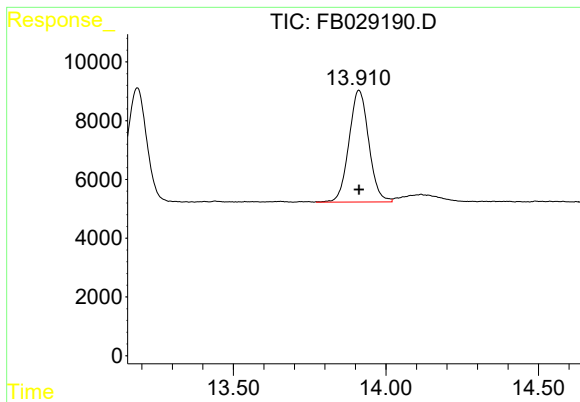

#9 O-Xylene

R.T.: 13.912 min
Delta R.T.: 0.000 min
Response: 171086
Conc: 10.41 ng/ml

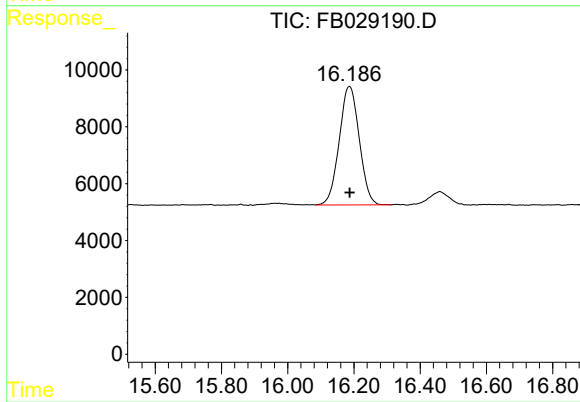

#10 1,2,4-Trimethylbenzene

R.T.: 16.187 min
Delta R.T.: 0.000 min
Response: 175039
Conc: 9.97 ng/ml