

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013123\
 Data File : FB029191.D
 Signal(s) : FID2B.CH
 Acq On : 31 Jan 2023 10:40
 Operator : AJ/MA
 Sample : 20 GRO STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 20 GRO STD

Integration File: Calibration.e
 Quant Time: Jan 31 11:11:08 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB013123.M
 Quant Title :
 QLast Update : Tue Jan 31 11:10:44 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.788	185381	20.000 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.707	322804	30.000 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	408446	30.000 ng/ml
3) t n-Heptane	7.747	113778	10.000 ng/ml
4) t Benzene	7.884	161764	10.000 ng/ml
6) t Toluene	10.616	471703	30.000 ng/ml
7) t Ethylbenzene	13.052	154229	10.000 ng/ml
8) t m-Xylene	13.185	308062	20.000 ng/ml
9) t O-Xylene	13.912	307646	20.000 ng/ml
10) t 1,2,4-Trimethylbenzene	16.187	320140	20.000 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013123\
Data File : FB029191.D
Signal(s) : FID2B.CH
Acq On : 31 Jan 2023 10:40
Operator : AJ/MA
Sample : 20 GRO STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
20 GRO STD

Integration File: Calibration.e
Quant Time: Jan 31 11:11:08 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB013123.M
Quant Title :
QLast Update : Tue Jan 31 11:10:44 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

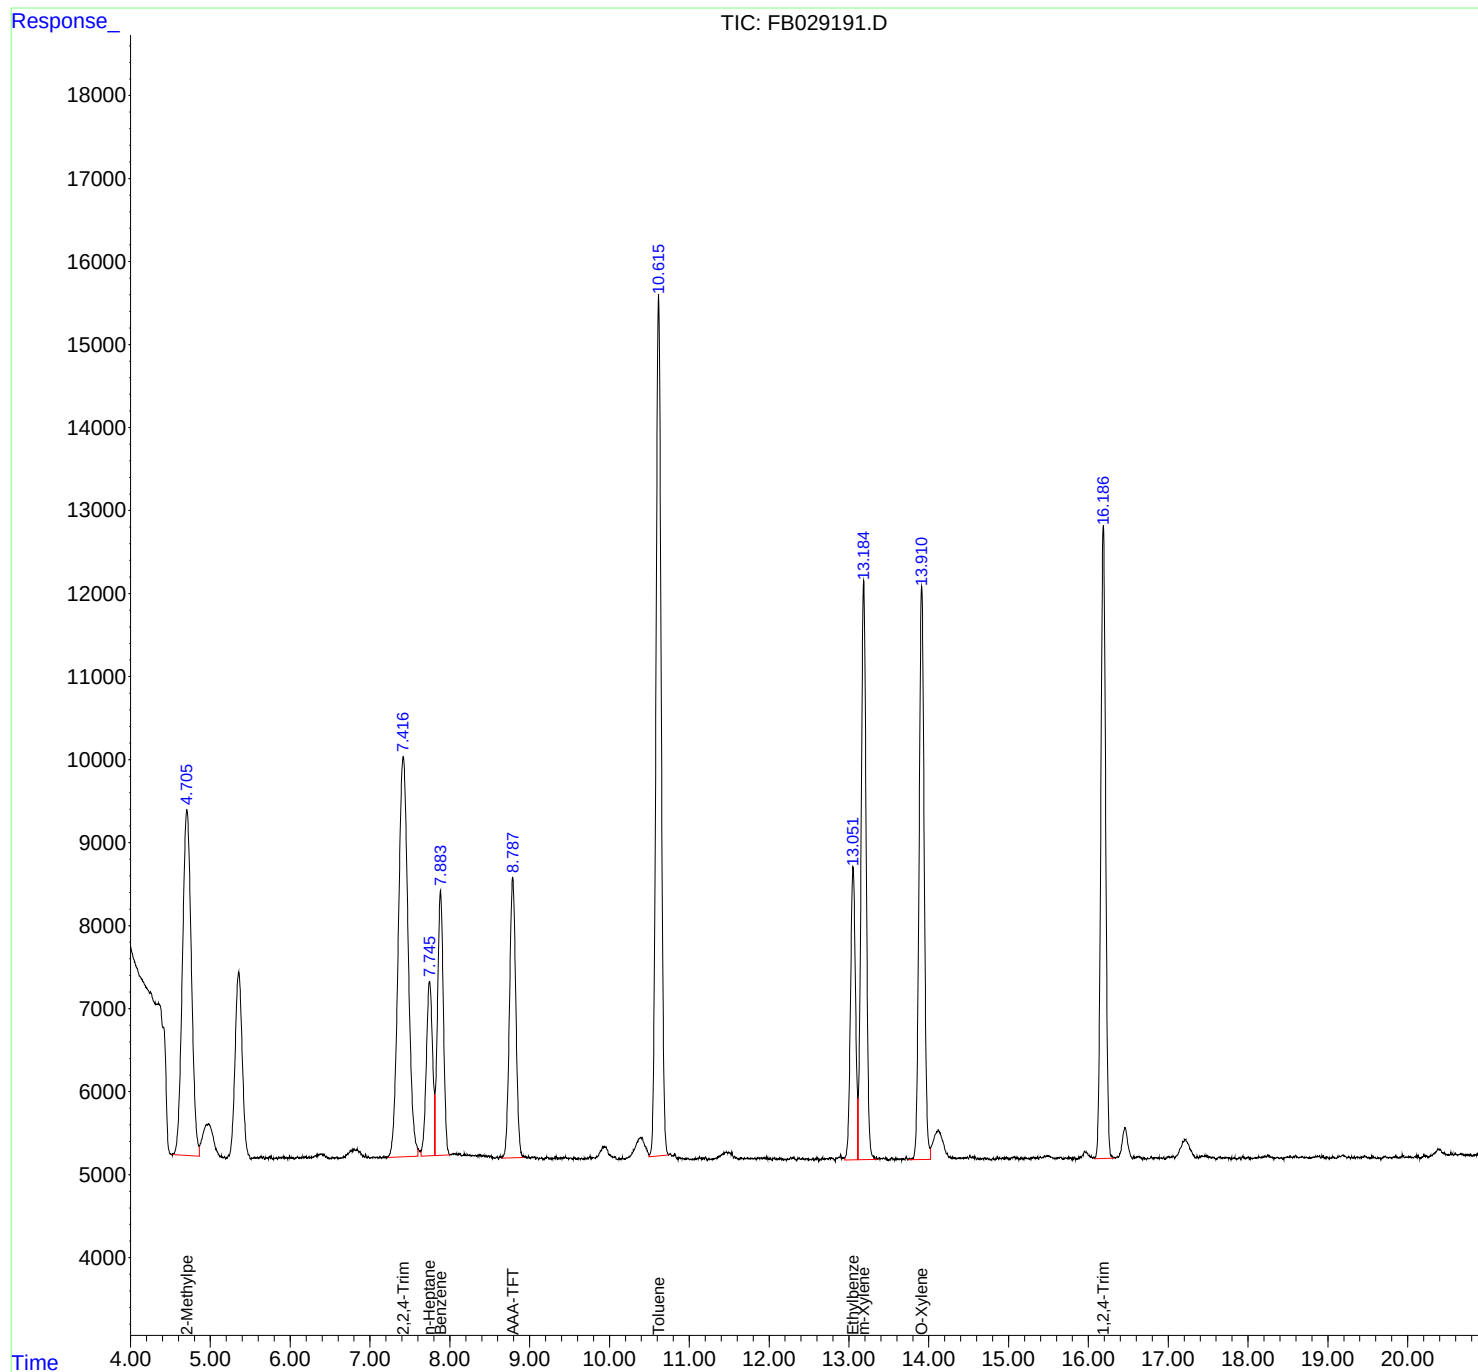


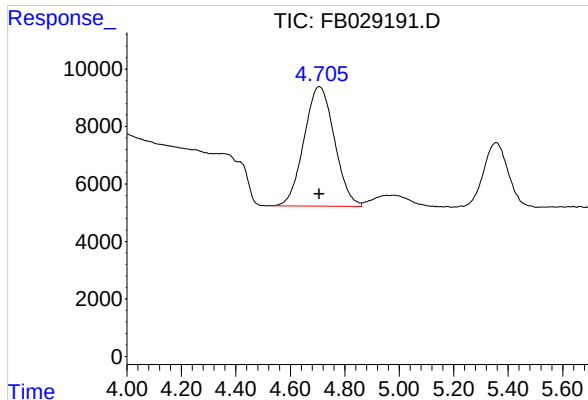

#1 2-Methylpentane


R.T.: 4.707 min
Delta R.T.: 0.000 min
Response: 322804
Conc: 30.00 ng/ml

Instrument :
FID_B
ClientSampleId :
20 GRO STD

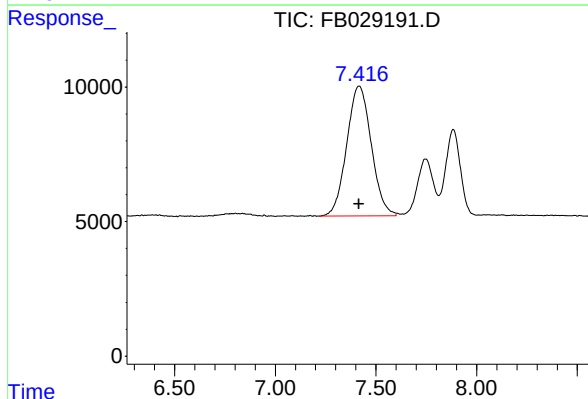


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: 0.000 min
Response: 408446
Conc: 30.00 ng/ml

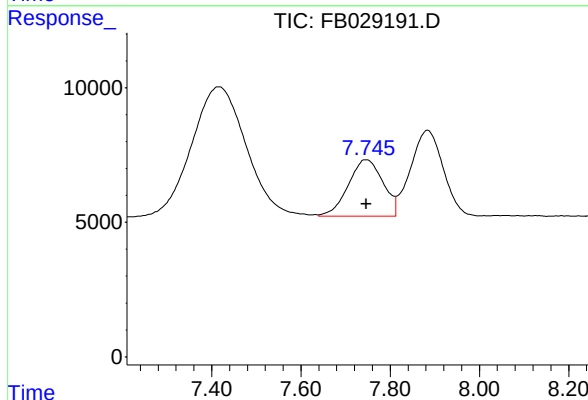


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: 0.000 min
Response: 113778
Conc: 10.00 ng/ml

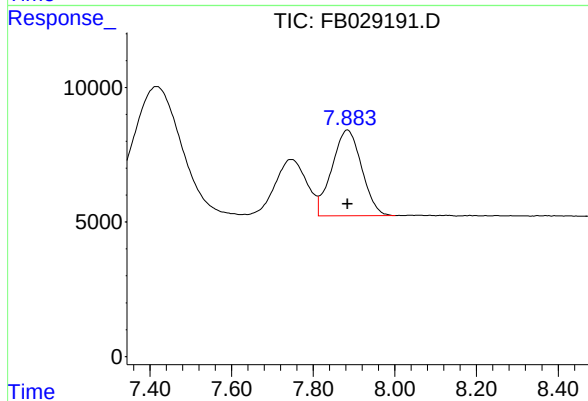

#4 Benzene


R.T.: 7.884 min
Delta R.T.: 0.000 min
Response: 161764
Conc: 10.00 ng/ml

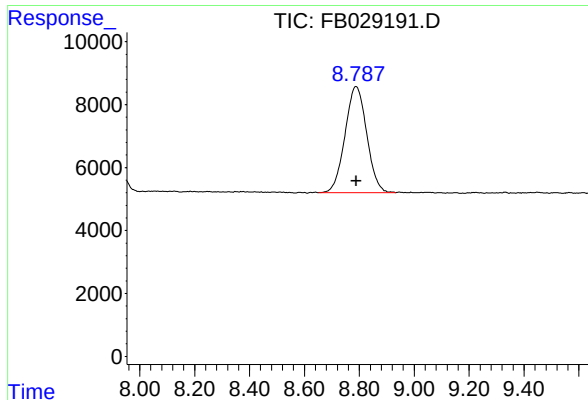

#5 AAA-TFT


R.T.: 8.788 min
Delta R.T.: 0.000 min
Response: 185381
Conc: 20.00 ng/ml

Instrument :
FID_B
ClientSampleId :
20 GRO STD

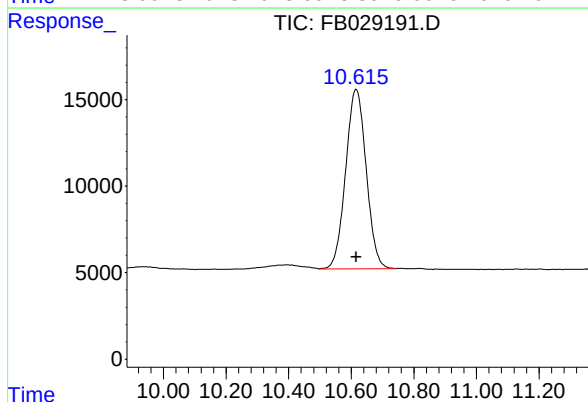


#6 Toluene

R.T.: 10.616 min
Delta R.T.: 0.000 min
Response: 471703
Conc: 30.00 ng/ml

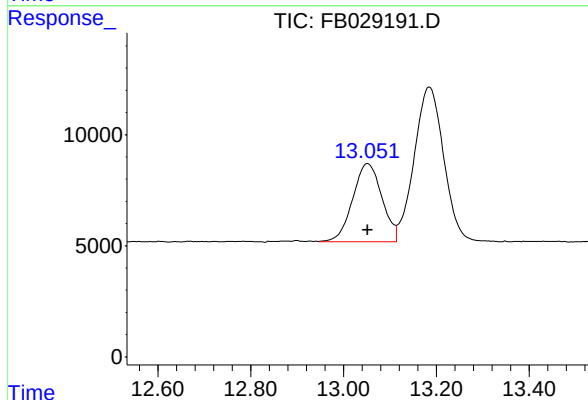


#7 Ethylbenzene

R.T.: 13.052 min
Delta R.T.: 0.000 min
Response: 154229
Conc: 10.00 ng/ml

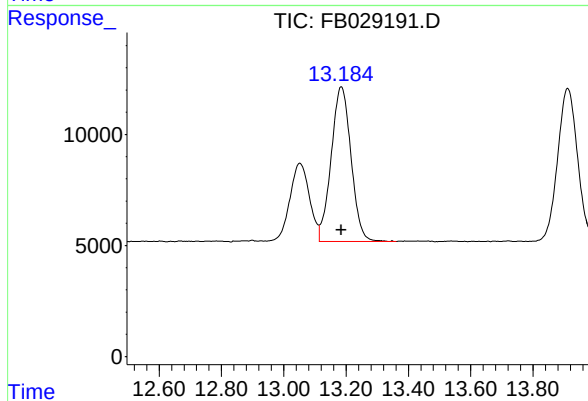

#8 m-Xylene


R.T.: 13.185 min
Delta R.T.: 0.000 min
Response: 308062
Conc: 20.00 ng/ml

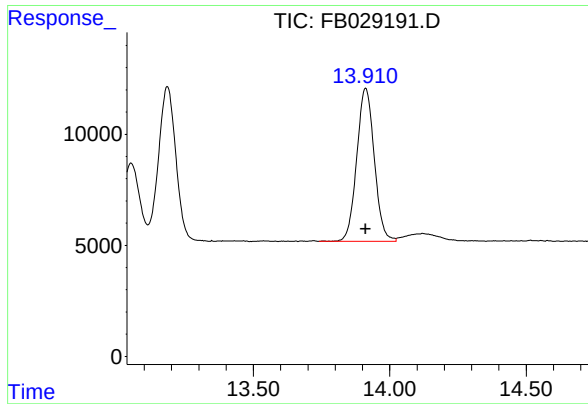

#9 O-Xylene

R.T.: 13.912 min
Delta R.T.: 0.000 min
Response: 307646
Conc: 20.00 ng/ml

Instrument :
FID_B
ClientSampleId :
20 GRO STD

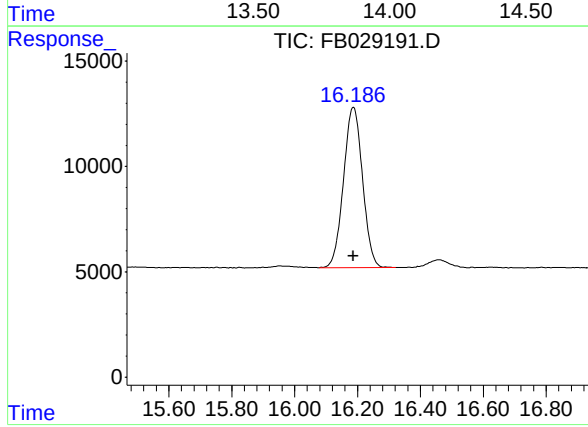

#10 1,2,4-Trimethylbenzene

R.T.: 16.187 min
Delta R.T.: 0.000 min
Response: 320140
Conc: 20.00 ng/ml