

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013125\
Data File : FB031433.D
Signal(s) : FID2B.CH
Acq On : 31 Jan 2025 19:52
Operator : YP/AJ
Sample : Q1241-09
Misc : 5.48G/5.00 ML DI WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Feb 01 00:17:11 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011525.M
Quant Title :
QLast Update : Wed Jan 15 12:01:08 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	444455	18.633 ng/ml
Target Compounds			
6) t Toluene	10.627	19022	0.487 ng/ml
7) t Ethylbenzene	13.047	4657	0.134 ng/ml
8) t m-Xylene	13.191	6398	0.171 ng/ml
9) t O-Xylene	13.922	10892	0.306 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	42560	1.503 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB013125\
Data File : FB031433.D
Signal(s) : FID2B.CH
Acq On : 31 Jan 2025 19:52
Operator : YP/AJ
Sample : Q1241-09
Misc : 5.48G/5.00 ML DI WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Feb 01 00:17:11 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011525.M
Quant Title :
QLast Update : Wed Jan 15 12:01:08 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

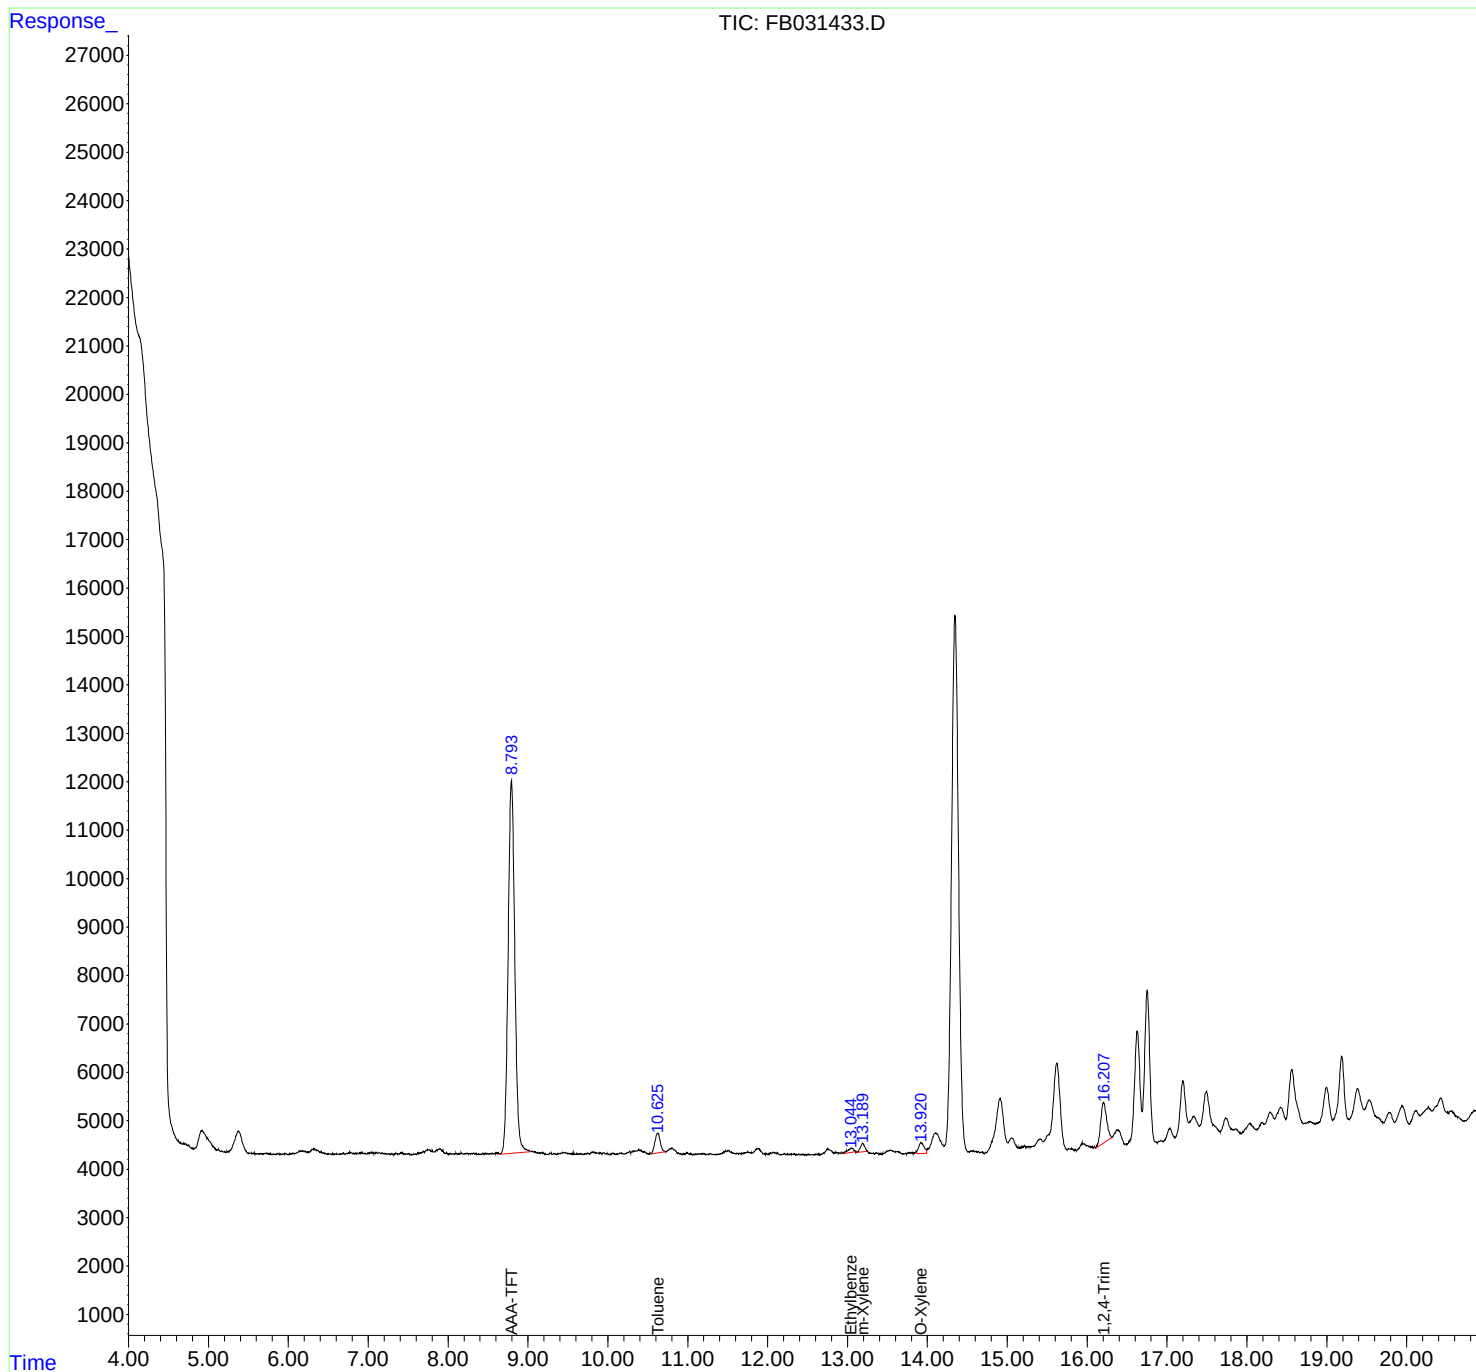


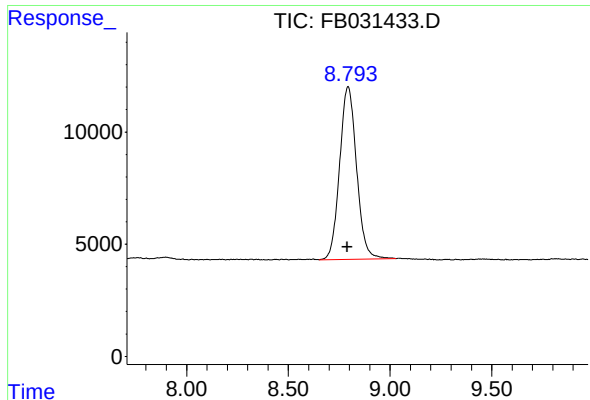

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: 0.005 min
Response: 444455
Conc: 18.63 ng/ml

Instrument :
FID_B
ClientSampleId :

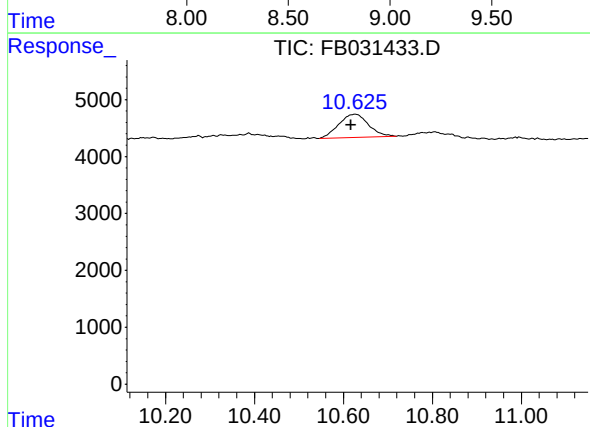


#6 Toluene

R.T.: 10.627 min
Delta R.T.: 0.009 min
Response: 19022
Conc: 0.49 ng/ml

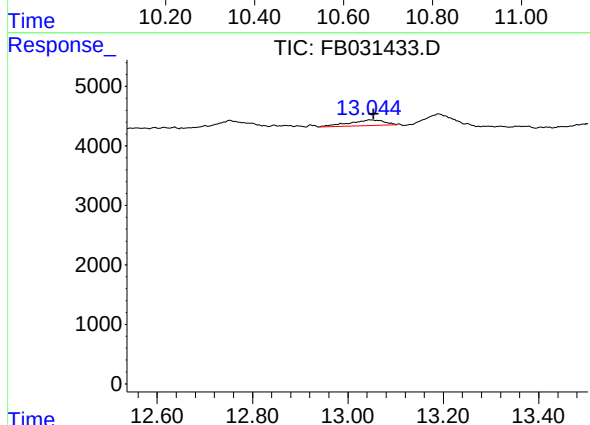


#7 Ethylbenzene

R.T.: 13.047 min
Delta R.T.: -0.008 min
Response: 4657
Conc: 0.13 ng/ml

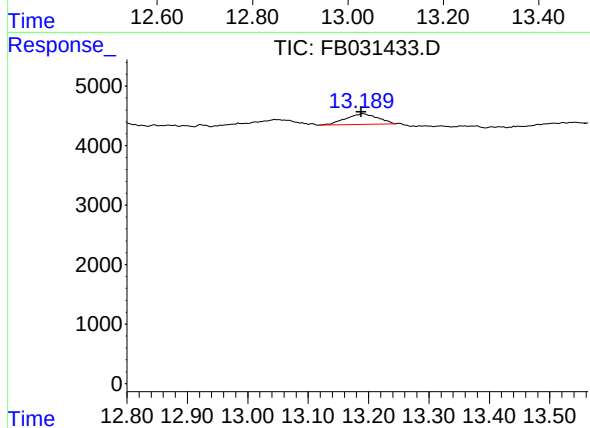

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: 0.002 min
Response: 6398
Conc: 0.17 ng/ml

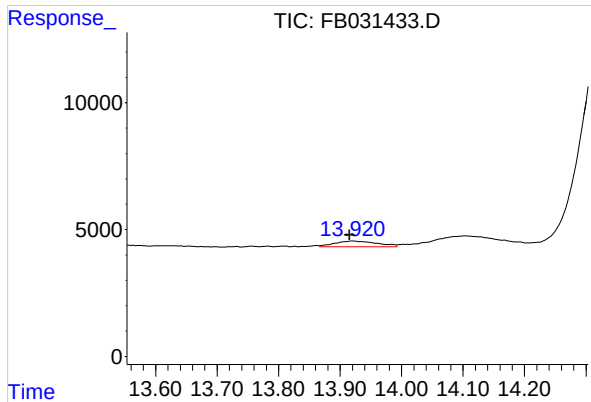

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: 0.006 min
Response: 10892
Conc: 0.31 ng/ml

Instrument :
FID_B
ClientSampleId :

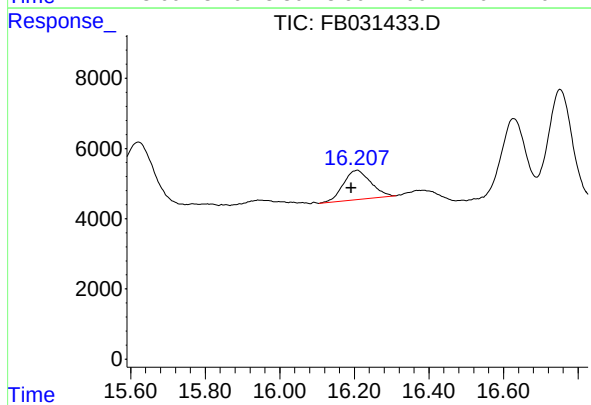

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.017 min
Response: 42560
Conc: 1.50 ng/ml