

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_B\Data\FB020119\
 Data File : FB019605.D
 Signal(s) : FID2B.CH
 Acq On : 1 Feb 2019 10:36
 Operator : MJ/SJ
 Sample : BSF0201S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 01 13:48:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
 Quant Title :
 QLast Update : Tue Jan 29 12:07:12 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.043	190415	17.025 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.897	498567	27.210 ng/ml
2) t 2,2,4-Trimethylpentane	7.657	497960	28.507 ng/ml
3) t n-Heptane	7.997	154281	9.267 ng/ml
4) t Benzene	8.135	175127	9.095 ng/ml
6) t Toluene	10.889	506629	29.109 ng/ml
7) t Ethylbenzene	13.341	208366	9.623 ng/ml
8) t m-Xylene	13.474	436173	19.312 ng/ml
9) t O-Xylene	14.206	427620	19.338 ng/ml
10) t 1,2,4-Trimethylbenzene	16.492	429835	18.885 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_B\Data\FB020119\
Data File : FB019605.D
Signal(s) : FID2B.CH
Acq On : 1 Feb 2019 10:36
Operator : MJ/SJ
Sample : BSF0201S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 01 13:48:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
Quant Title :
QLast Update : Tue Jan 29 12:07:12 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

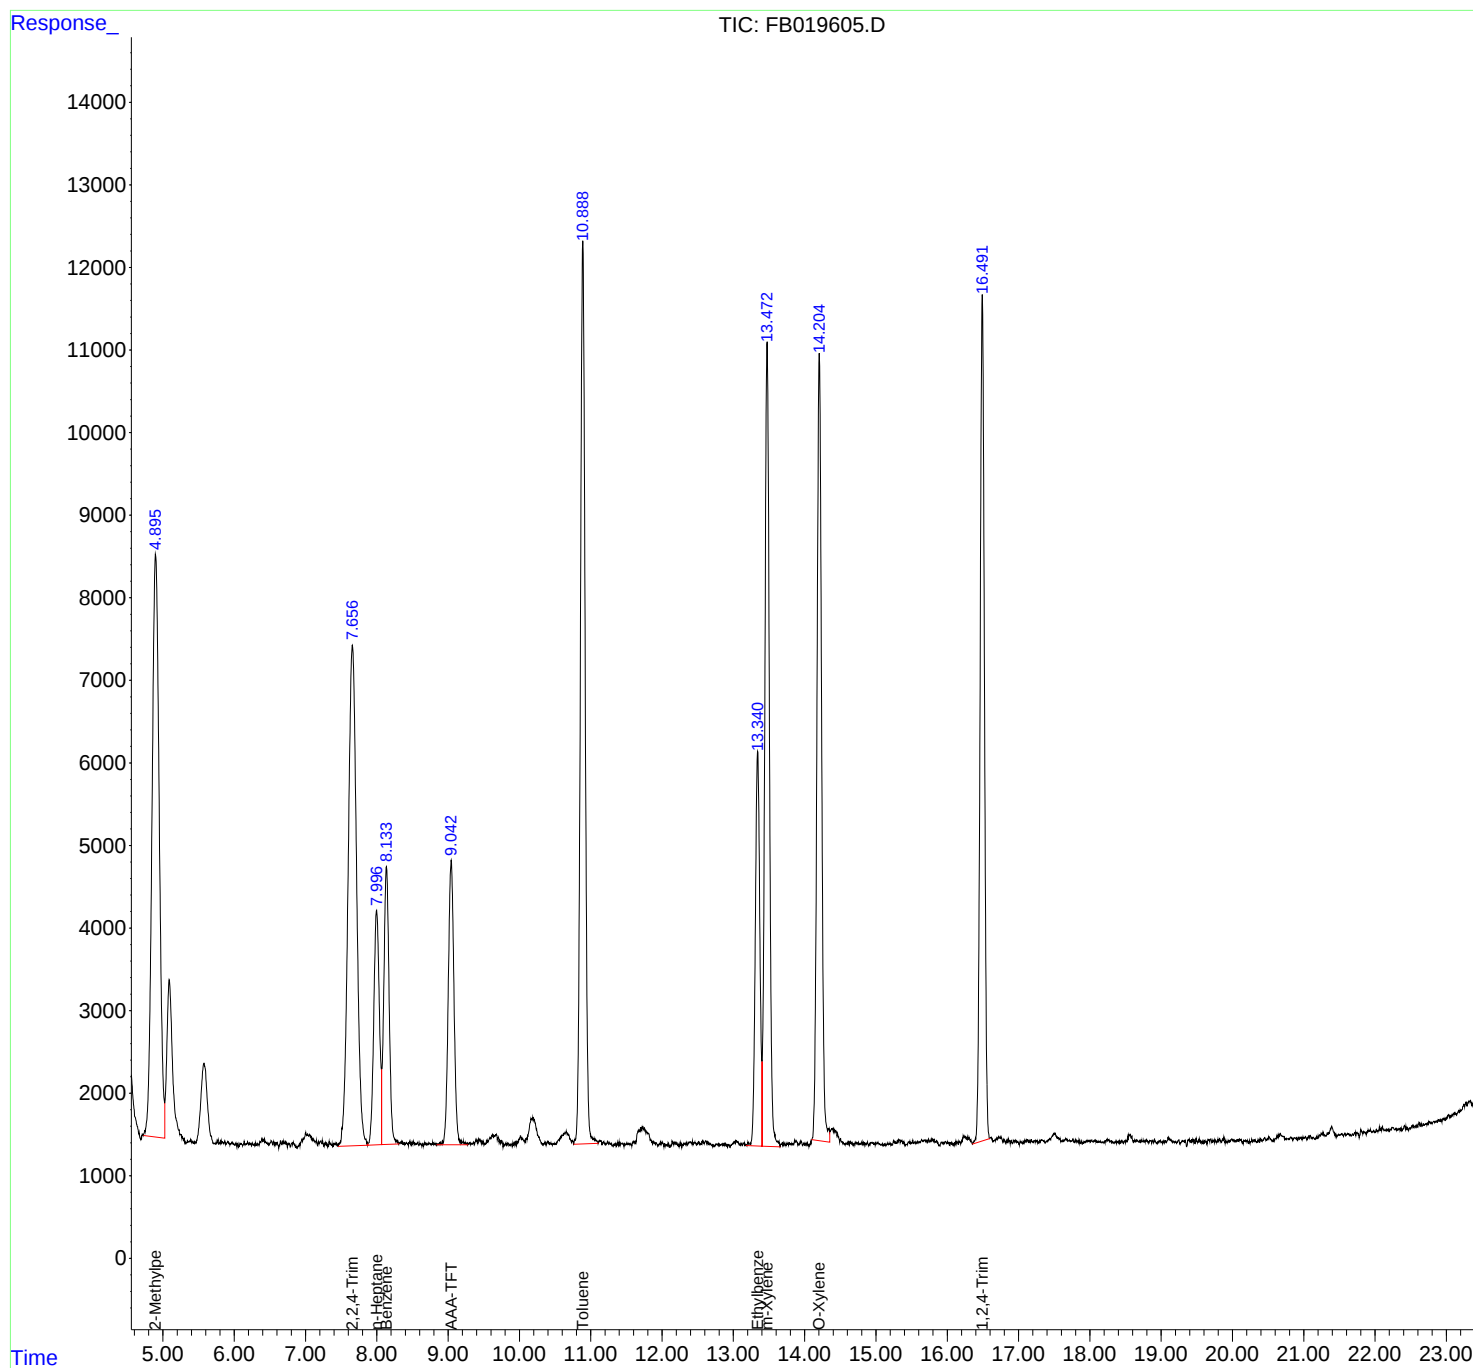

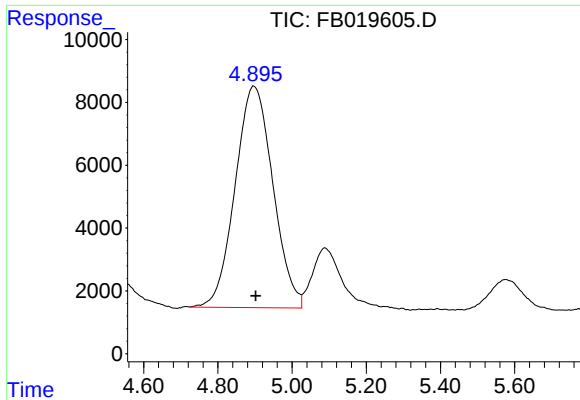


#1 2-Methylpentane

R.T.: 4.897 min
Delta R.T.: -0.005 min
Response: 498567
Conc: 27.21 ng/ml

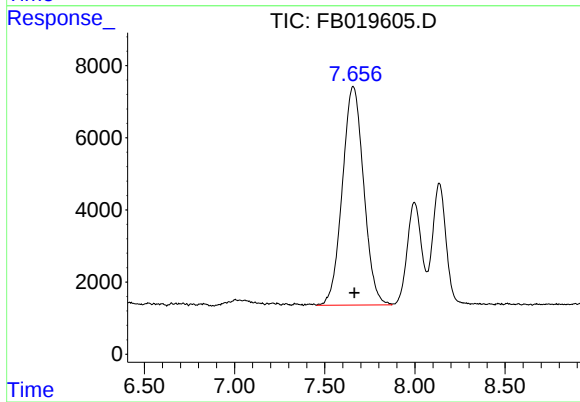


#2 2,2,4-Trimethylpentane

R.T.: 7.657 min
Delta R.T.: -0.007 min
Response: 497960
Conc: 28.51 ng/ml

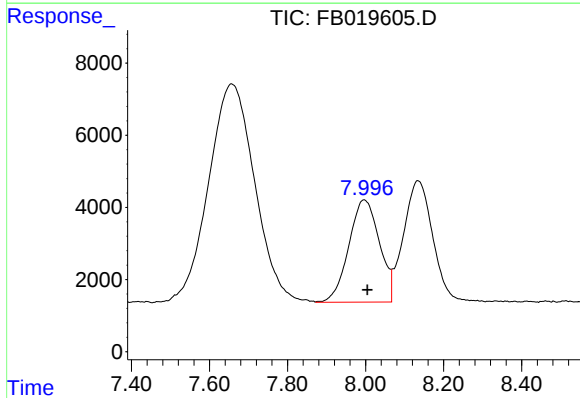


#3 n-Heptane

R.T.: 7.997 min
Delta R.T.: -0.008 min
Response: 154281
Conc: 9.27 ng/ml

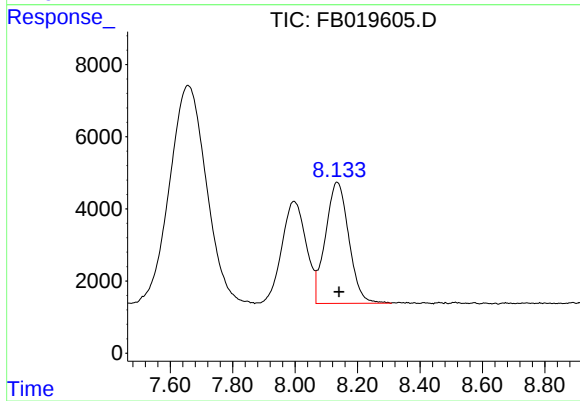


#4 Benzene

R.T.: 8.135 min
Delta R.T.: -0.006 min
Response: 175127
Conc: 9.09 ng/ml

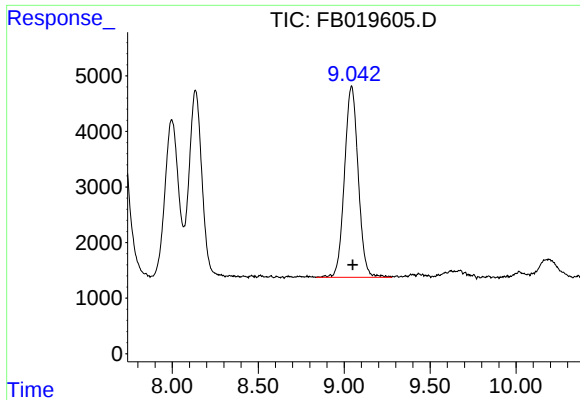


#5 AAA-TFT

R.T.: 9.043 min
Delta R.T.: -0.006 min
Response: 190415
Conc: 17.03 ng/ml

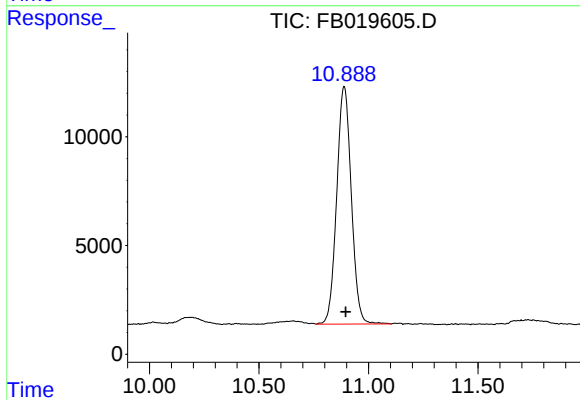


#6 Toluene

R.T.: 10.889 min
Delta R.T.: -0.007 min
Response: 506629
Conc: 29.11 ng/ml

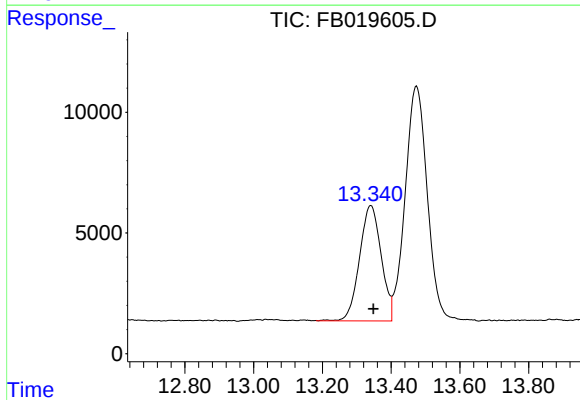


#7 Ethylbenzene

R.T.: 13.341 min
Delta R.T.: -0.007 min
Response: 208366
Conc: 9.62 ng/ml

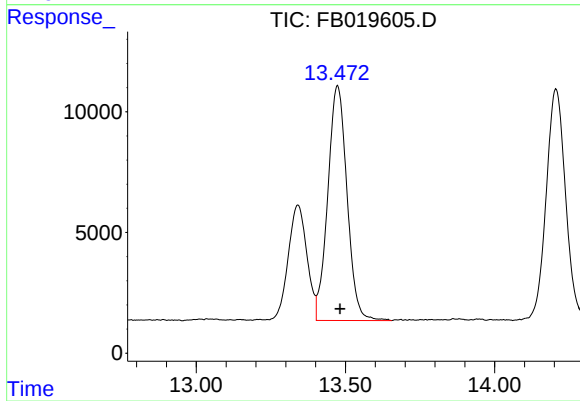


#8 m-Xylene

R.T.: 13.474 min
Delta R.T.: -0.008 min
Response: 436173
Conc: 19.31 ng/ml

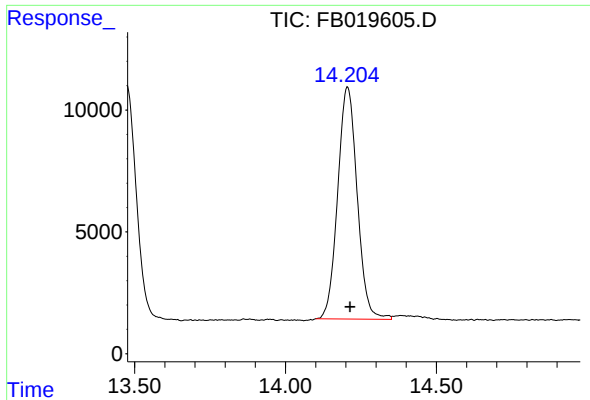

#9 O-Xylene

R.T.: 14.206 min
Delta R.T.: -0.008 min
Response: 427620
Conc: 19.34 ng/ml

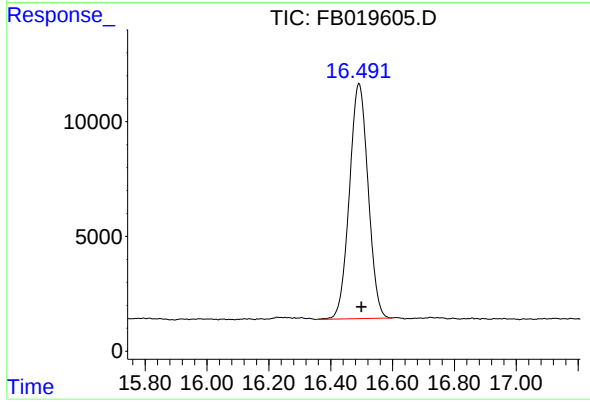

#10 1,2,4-Trimethylbenzene

R.T.: 16.492 min
Delta R.T.: -0.008 min
Response: 429835
Conc: 18.89 ng/ml