

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_B\Data\FB020119\
 Data File : FB019609.D
 Signal(s) : FID2B.CH
 Acq On : 1 Feb 2019 12:37
 Operator : MJ/SJ
 Sample : K1011-13MSD
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 01 13:48:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
 Quant Title :
 QLast Update : Tue Jan 29 12:07:12 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.044	167038	14.935 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.899	396455	21.637 ng/ml
2) t 2,2,4-Trimethylpentane	7.658	311491	17.832 ng/ml
3) t n-Heptane	7.999	101224	6.080 ng/ml
4) t Benzene	8.136	162916	8.461 ng/ml
6) t Toluene	10.890	464590	26.693 ng/ml
7) t Ethylbenzene	13.342	175706	8.115 ng/ml
8) t m-Xylene	13.475	376678	16.678 ng/ml
9) t O-Xylene	14.207	364366	16.477 ng/ml
10) t 1,2,4-Trimethylbenzene	16.493	330128	14.504 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_B\Data\FB020119\
Data File : FB019609.D
Signal(s) : FID2B.CH
Acq On : 1 Feb 2019 12:37
Operator : MJ/SJ
Sample : K1011-13MSD
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 01 13:48:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
Quant Title :
QLast Update : Tue Jan 29 12:07:12 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

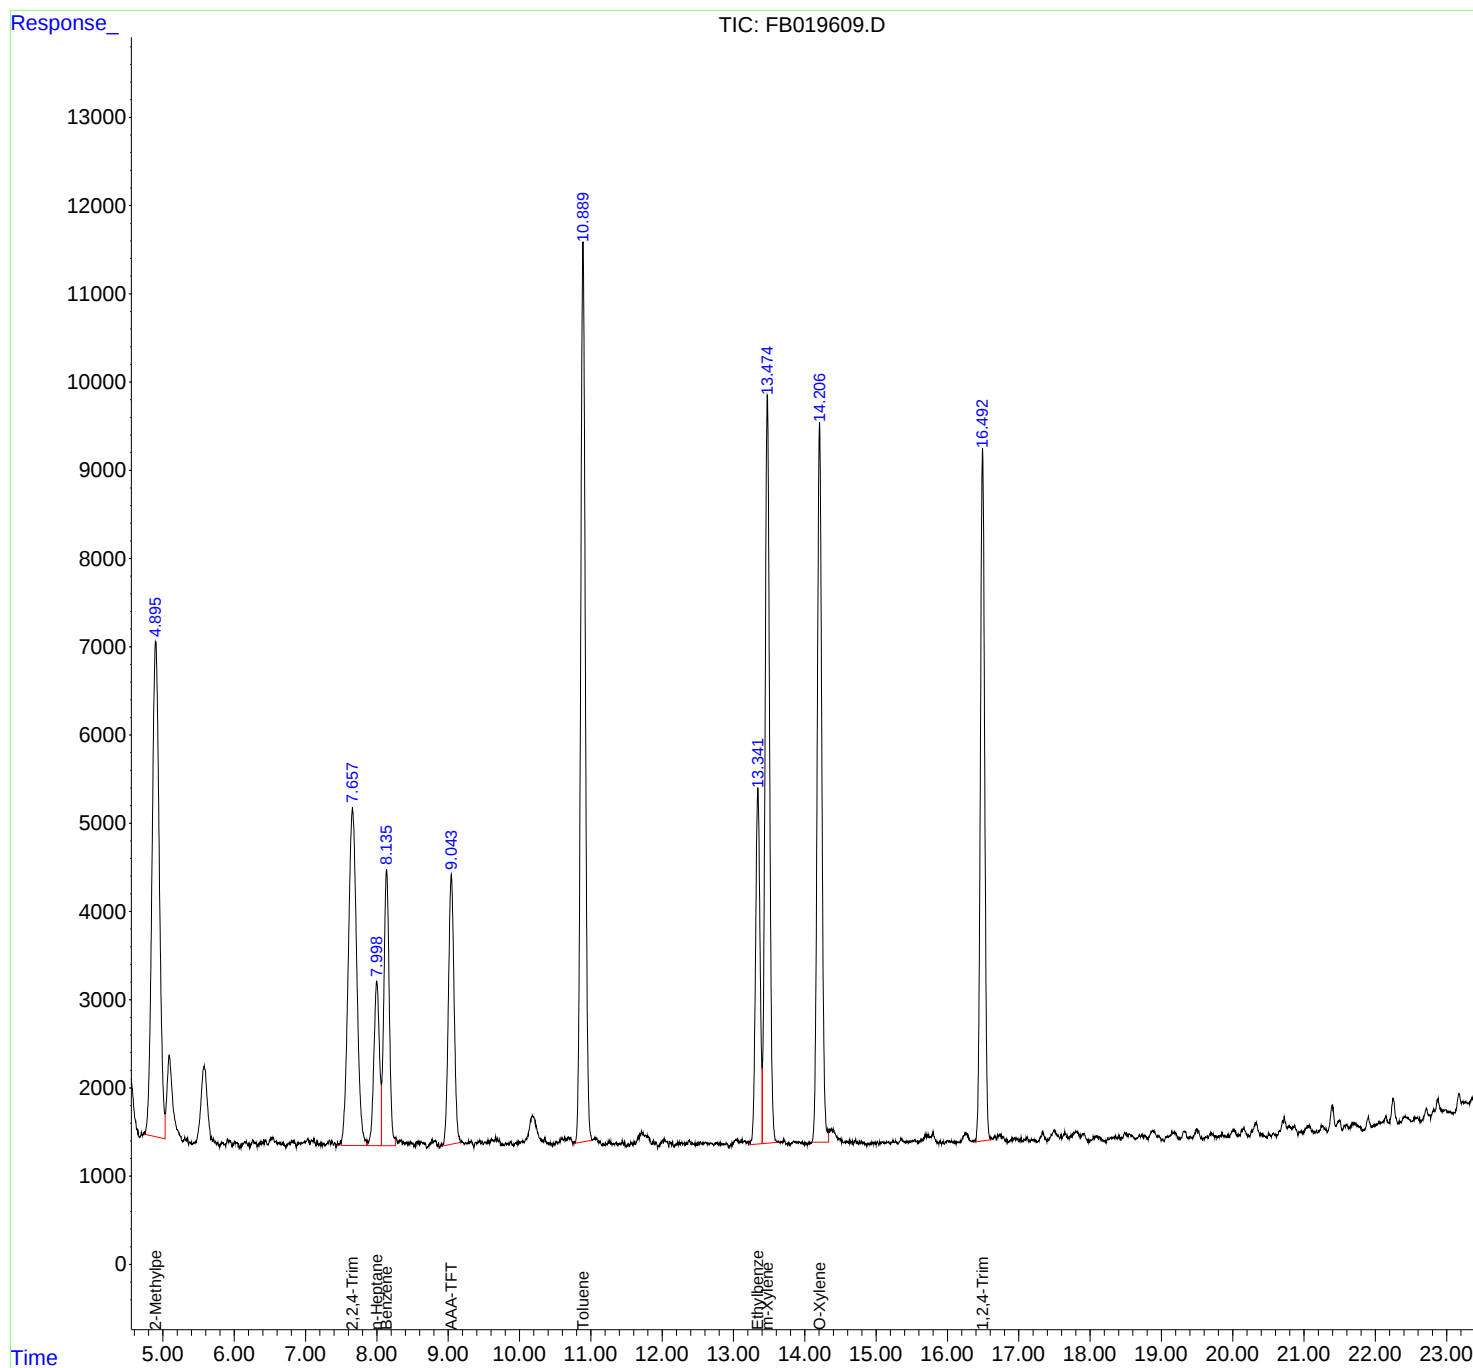

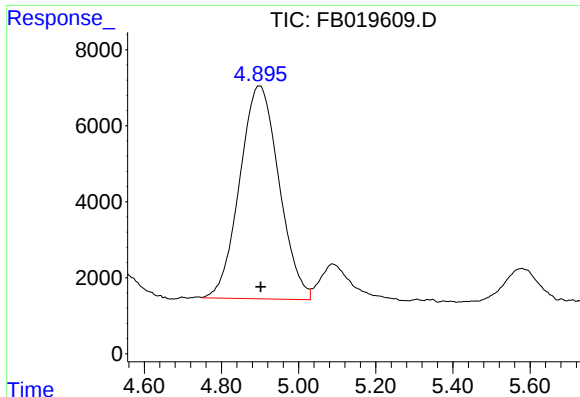


#1 2-Methylpentane

R.T.: 4.899 min
Delta R.T.: -0.003 min
Response: 396455
Conc: 21.64 ng/ml

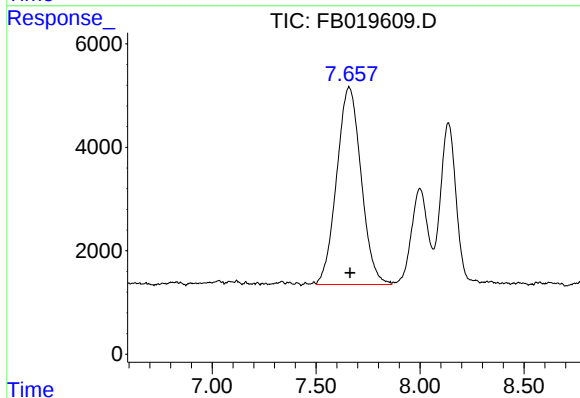


#2 2,2,4-Trimethylpentane

R.T.: 7.658 min
Delta R.T.: -0.006 min
Response: 311491
Conc: 17.83 ng/ml

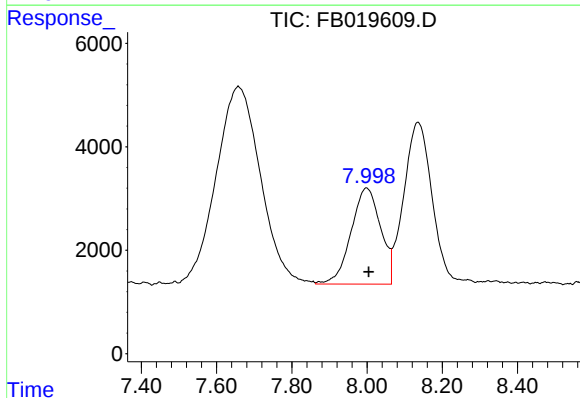


#3 n-Heptane

R.T.: 7.999 min
Delta R.T.: -0.006 min
Response: 101224
Conc: 6.08 ng/ml

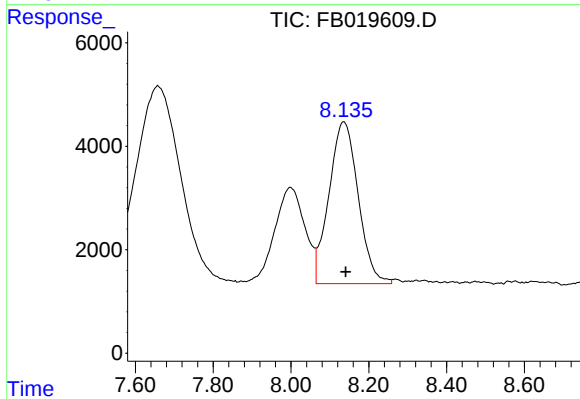


#4 Benzene

R.T.: 8.136 min
Delta R.T.: -0.005 min
Response: 162916
Conc: 8.46 ng/ml

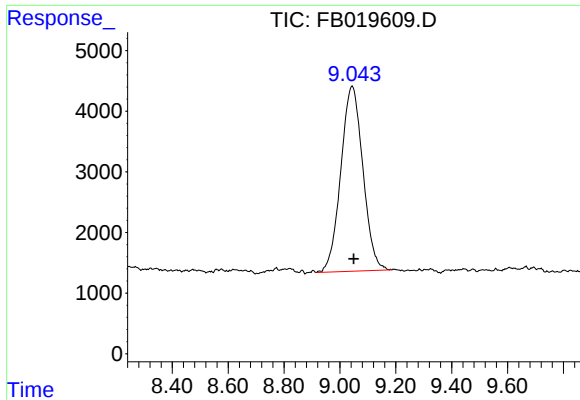


#5 AAA-TFT

R.T.: 9.044 min
Delta R.T.: -0.005 min
Response: 167038
Conc: 14.94 ng/ml

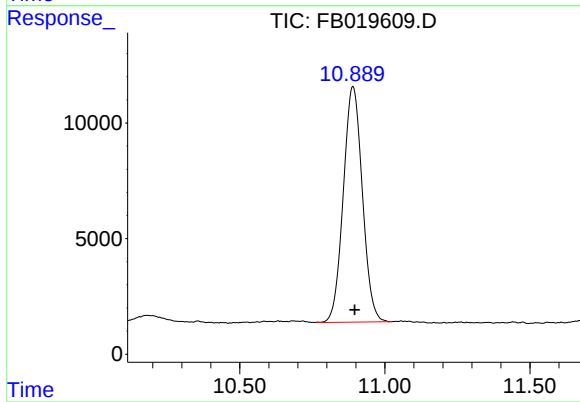


#6 Toluene

R.T.: 10.890 min
Delta R.T.: -0.006 min
Response: 464590
Conc: 26.69 ng/ml

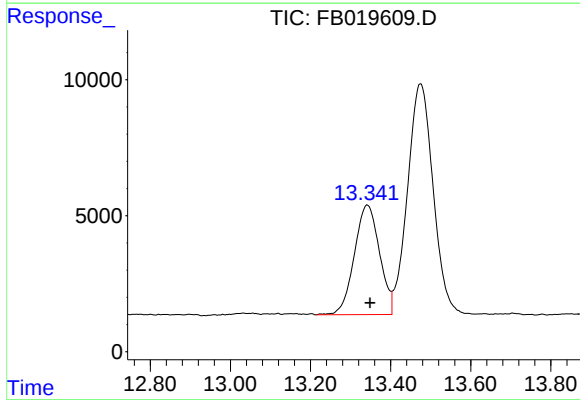


#7 Ethylbenzene

R.T.: 13.342 min
Delta R.T.: -0.006 min
Response: 175706
Conc: 8.11 ng/ml

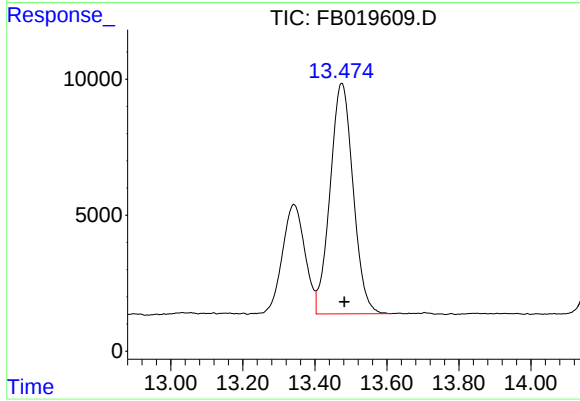


#8 m-Xylene

R.T.: 13.475 min
Delta R.T.: -0.007 min
Response: 376678
Conc: 16.68 ng/ml

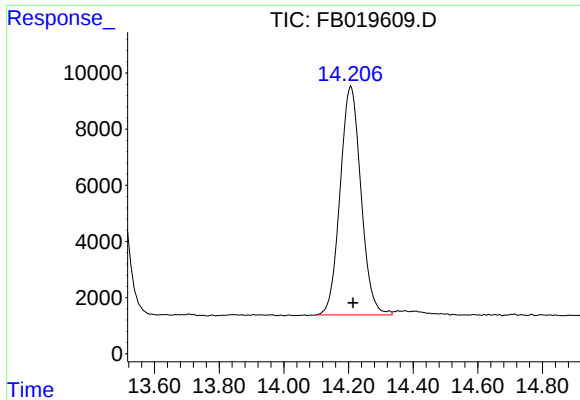

#9 O-Xylene

R.T.: 14.207 min
Delta R.T.: -0.007 min
Response: 364366
Conc: 16.48 ng/ml

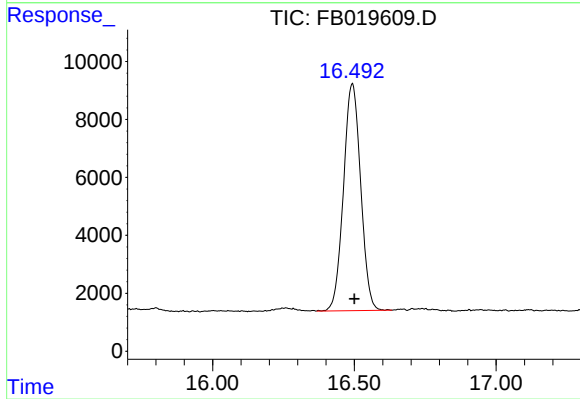

#10 1,2,4-Trimethylbenzene

R.T.: 16.493 min
Delta R.T.: -0.007 min
Response: 330128
Conc: 14.50 ng/ml