

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020123\
Data File : FB029202.D
Signal(s) : FID2B.CH
Acq On : 1 Feb 2023 15:44
Operator : AJ/MA
Sample : 01386-15
Misc : 6.44G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Feb 02 04:43:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB013123.M
Quant Title :
QLast Update : Tue Jan 31 12:31:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.788	210732	17.654 ng/ml
Target Compounds			
6) t Toluene	10.614	6154	0.351 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020123\
Data File : FB029202.D
Signal(s) : FID2B.CH
Acq On : 1 Feb 2023 15:44
Operator : AJ/MA
Sample : 01386-15
Misc : 6.44G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Feb 02 04:43:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB013123.M
Quant Title :
QLast Update : Tue Jan 31 12:31:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

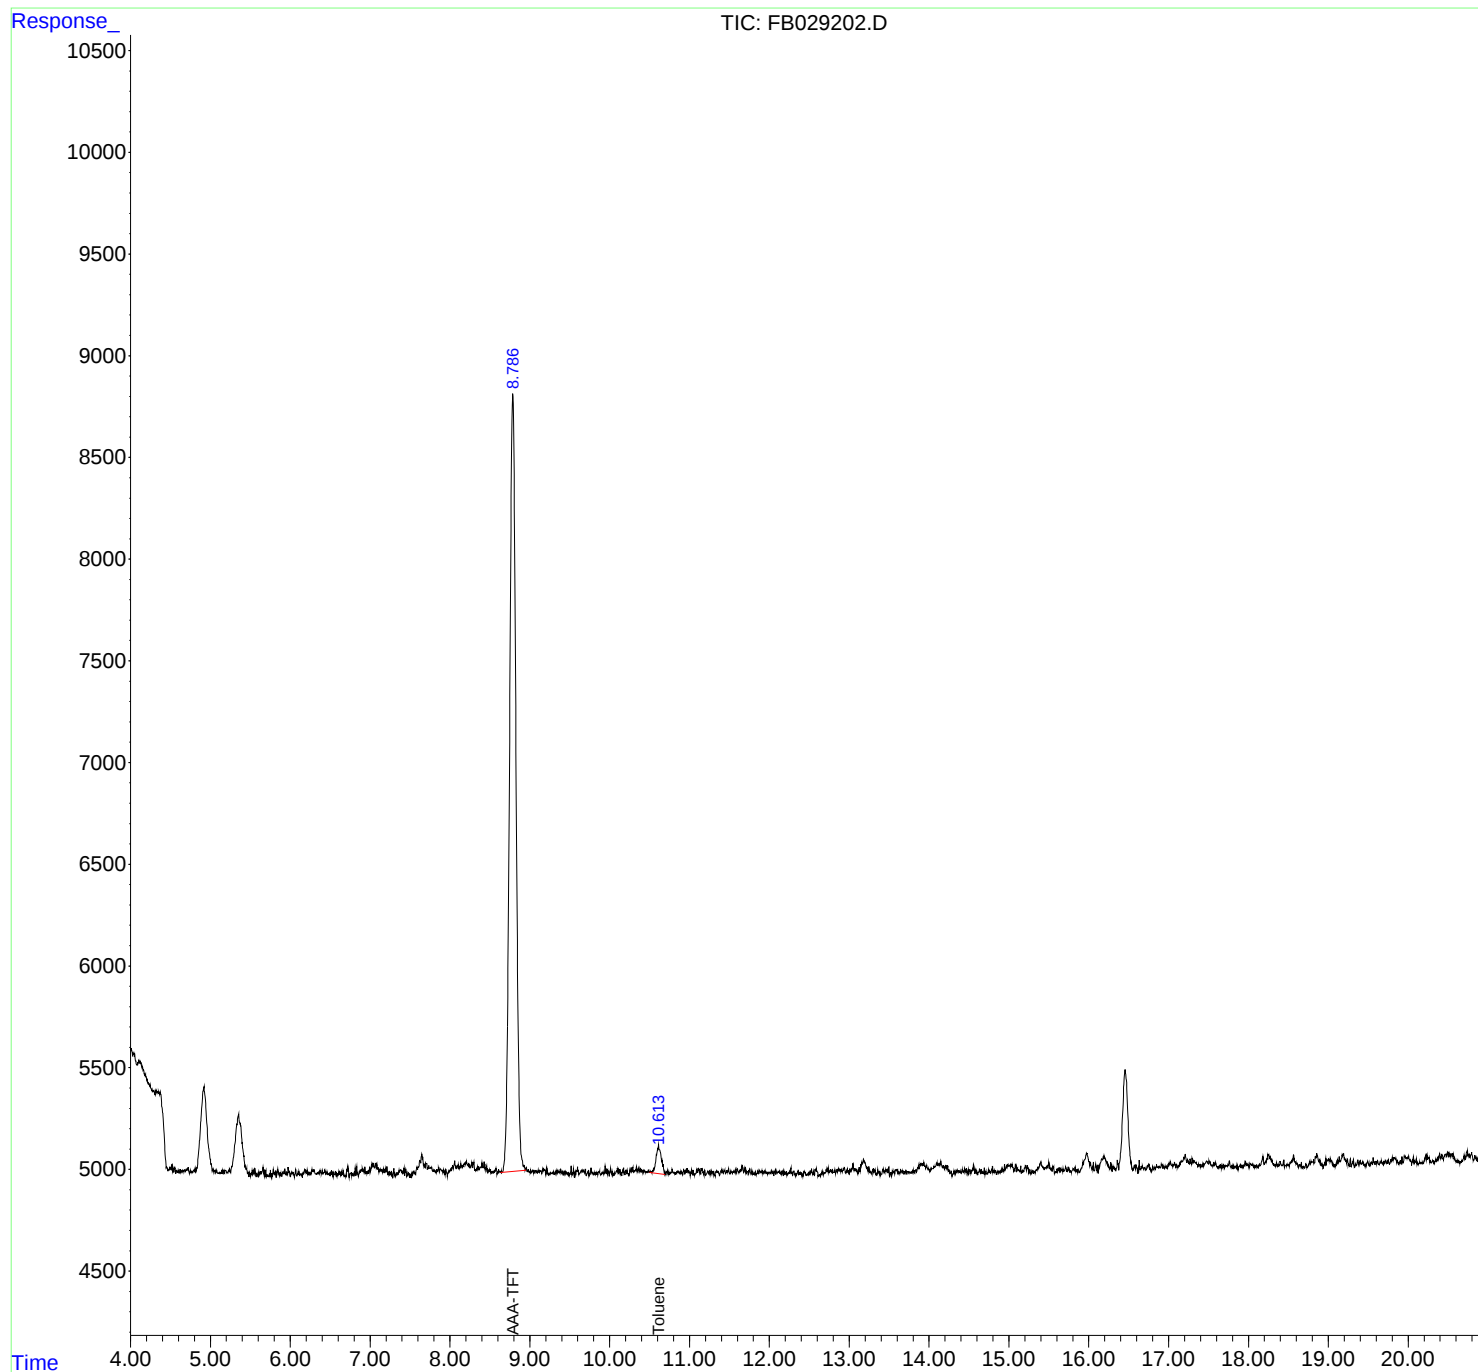

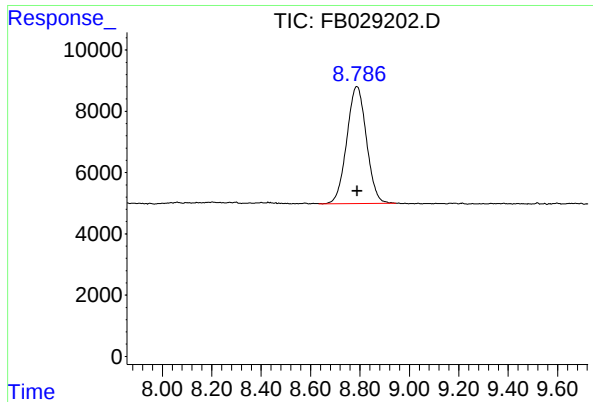


#5 AAA-TFT

R.T.: 8.788 min
Delta R.T.: 0.000 min
Response: 210732
Conc: 17.65 ng/ml

Instrument :

FID_B

ClientSampleId :

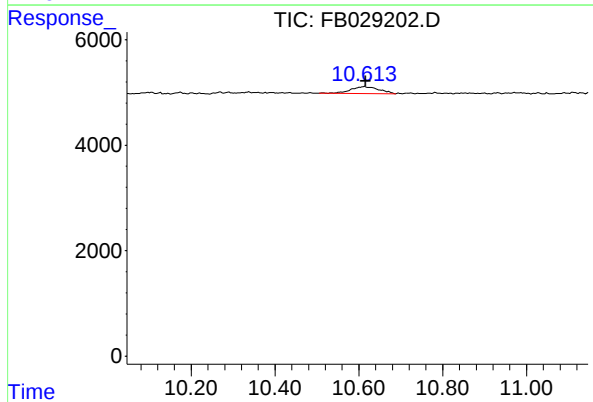

#6 Toluene

R.T.: 10.614 min
Delta R.T.: -0.002 min
Response: 6154
Conc: 0.35 ng/ml