

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020123\
 Data File : FB029203.D
 Signal(s) : FID2B.CH
 Acq On : 1 Feb 2023 16:21
 Operator : AJ/MA
 Sample : BSF0201S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0201S2

Integration File: Calibration.e
 Quant Time: Feb 02 04:43:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB013123.M
 Quant Title :
 QLast Update : Tue Jan 31 12:31:55 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.788	199928	16.748 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.704	329781	28.697 ng/ml
2) t 2,2,4-Trimethylpentane	7.413	404545	28.573 ng/ml
3) t n-Heptane	7.747	119983	9.644 ng/ml
4) t Benzene	7.883	181219	10.056 ng/ml
6) t Toluene	10.616	548458	31.277 ng/ml
7) t Ethylbenzene	13.053	174113	10.303 ng/ml
8) t m-Xylene	13.185	344393	20.556 ng/ml
9) t O-Xylene	13.912	334734	20.155 ng/ml
10) t 1,2,4-Trimethylbenzene	16.187	335182	19.762 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020123\
Data File : FB029203.D
Signal(s) : FID2B.CH
Acq On : 1 Feb 2023 16:21
Operator : AJ/MA
Sample : BSF0201S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0201S2

Integration File: Calibration.e
Quant Time: Feb 02 04:43:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB013123.M
Quant Title :
QLast Update : Tue Jan 31 12:31:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

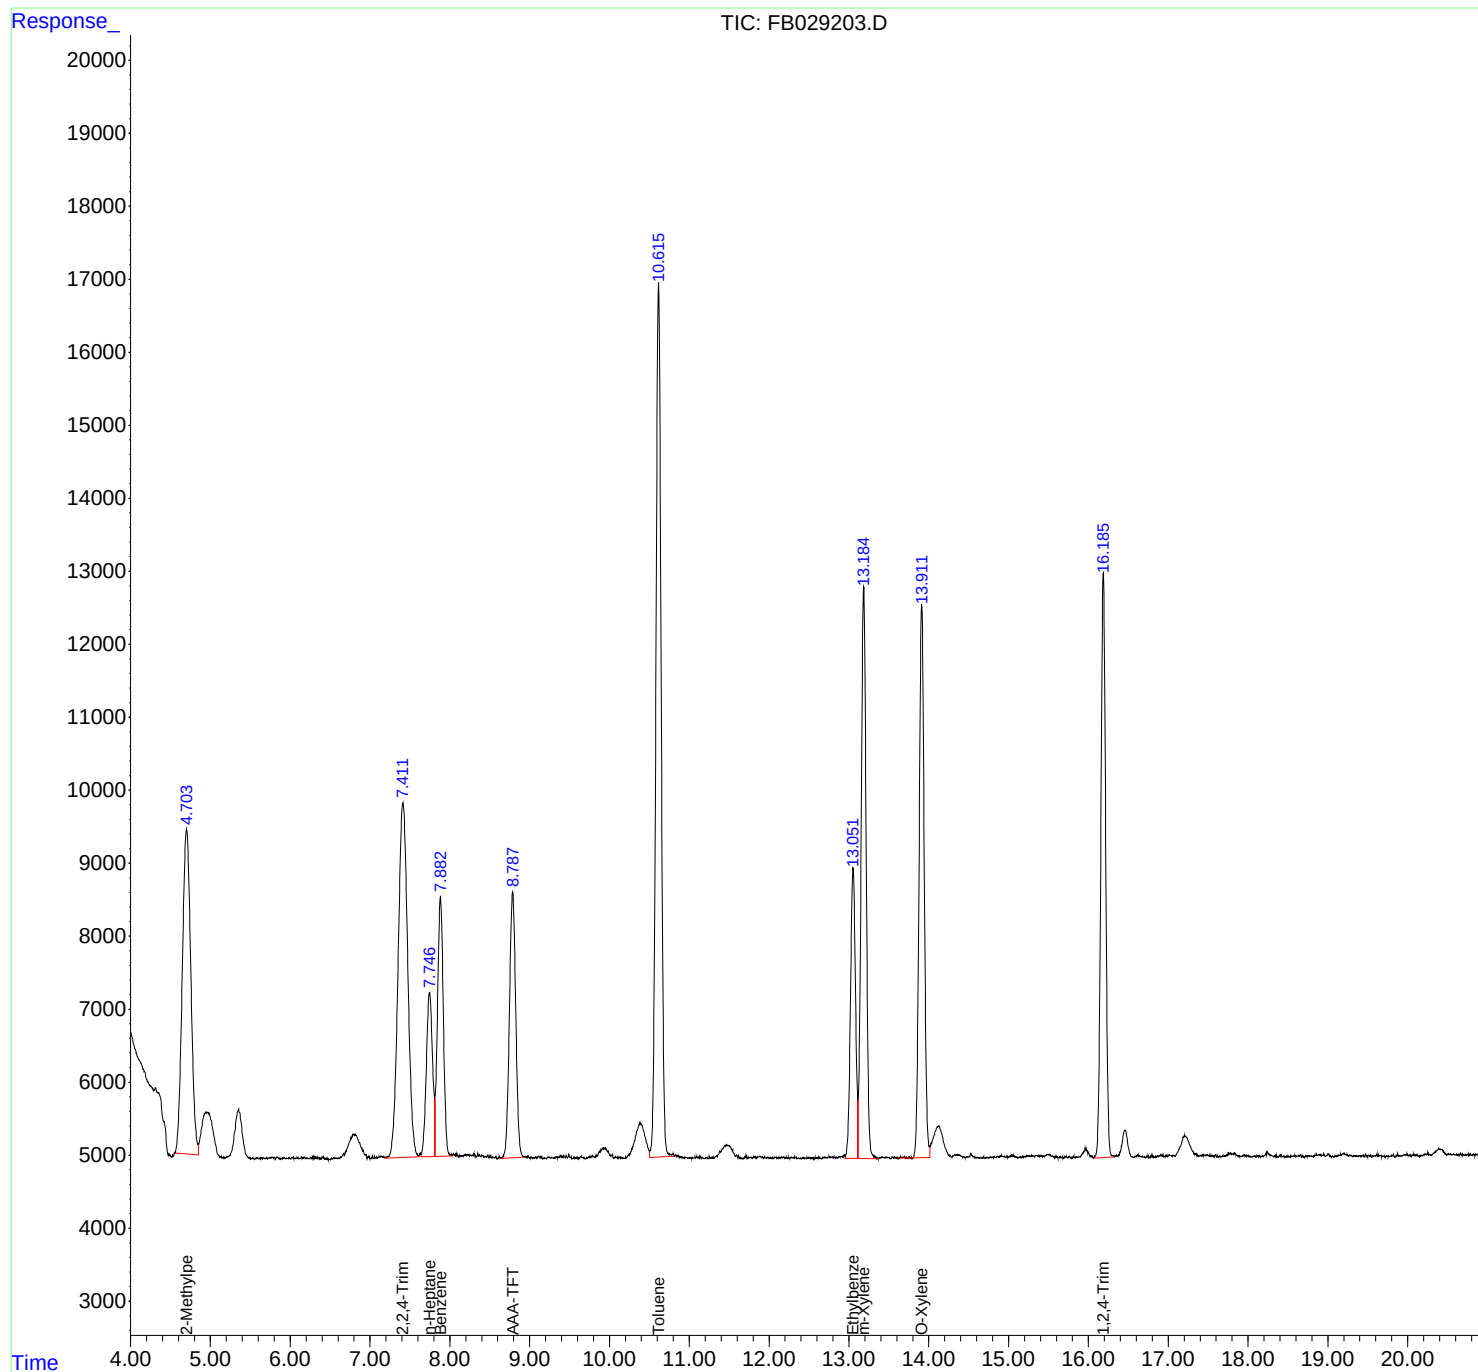


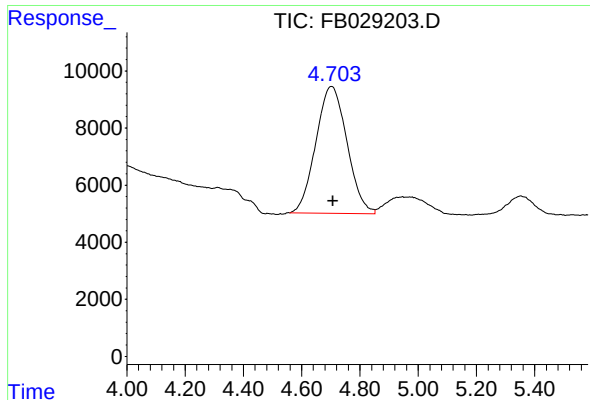

#1 2-Methylpentane


R.T.: 4.704 min
Delta R.T.: -0.003 min
Response: 329781
Conc: 28.70 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0201S2

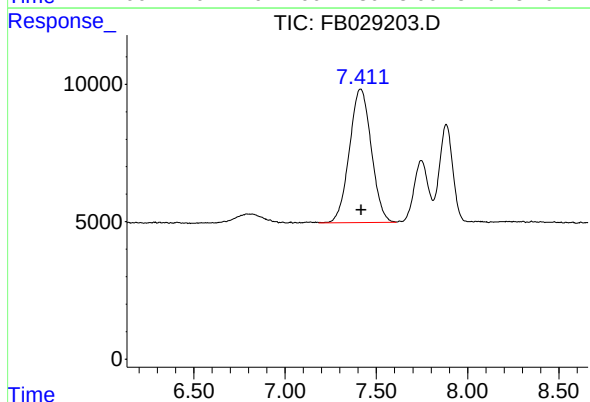


#2 2,2,4-Trimethylpentane

R.T.: 7.413 min
Delta R.T.: -0.004 min
Response: 404545
Conc: 28.57 ng/ml

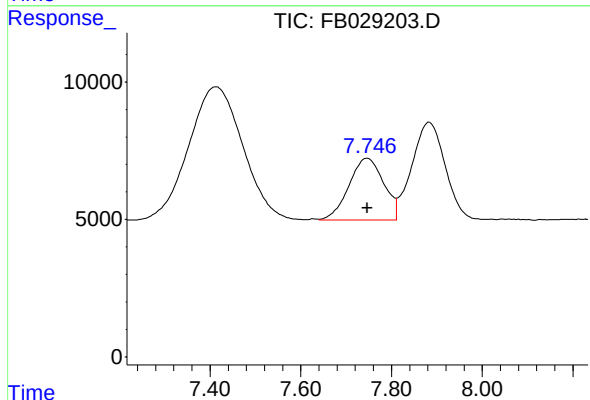


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: 0.000 min
Response: 119983
Conc: 9.64 ng/ml

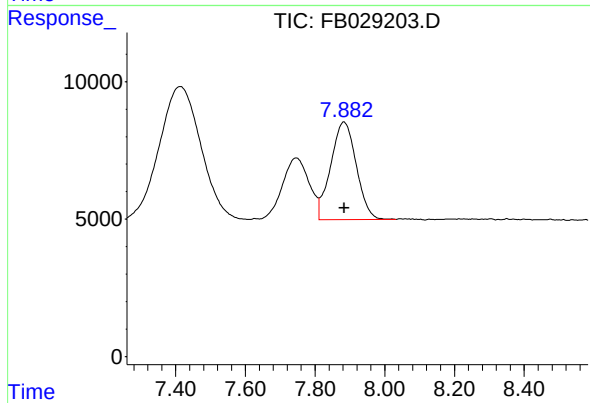

#4 Benzene


R.T.: 7.883 min
Delta R.T.: 0.000 min
Response: 181219
Conc: 10.06 ng/ml

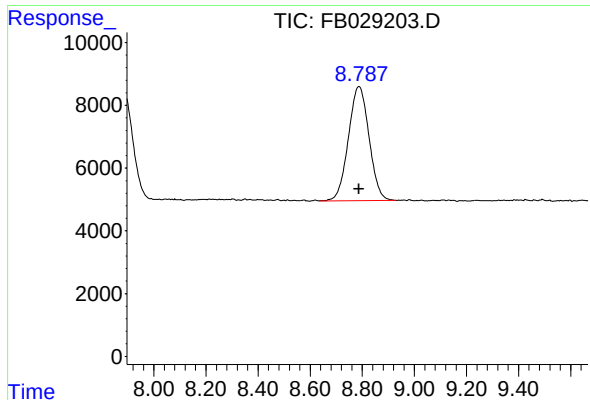

#5 AAA-TFT


R.T.: 8.788 min
Delta R.T.: 0.000 min
Response: 199928
Conc: 16.75 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0201S2

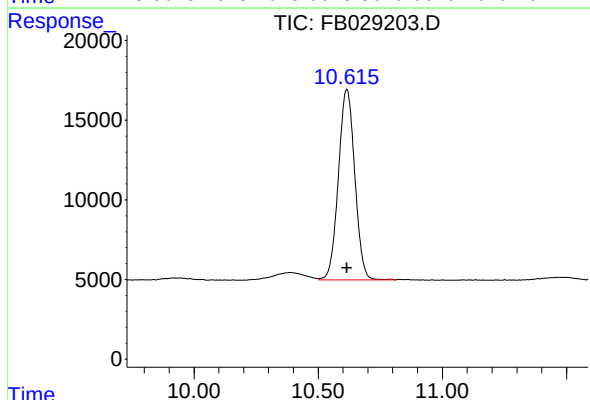


#6 Toluene

R.T.: 10.616 min
Delta R.T.: 0.000 min
Response: 548458
Conc: 31.28 ng/ml

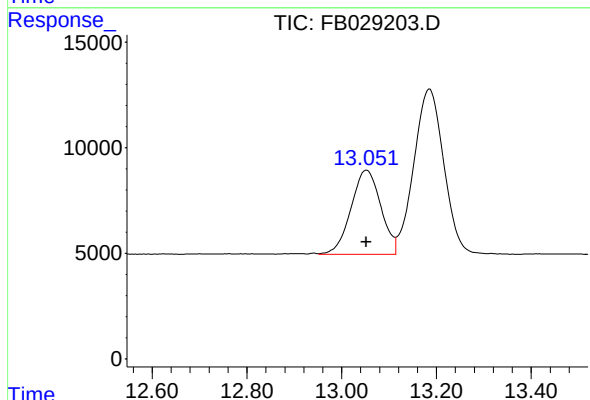


#7 Ethylbenzene

R.T.: 13.053 min
Delta R.T.: 0.000 min
Response: 174113
Conc: 10.30 ng/ml

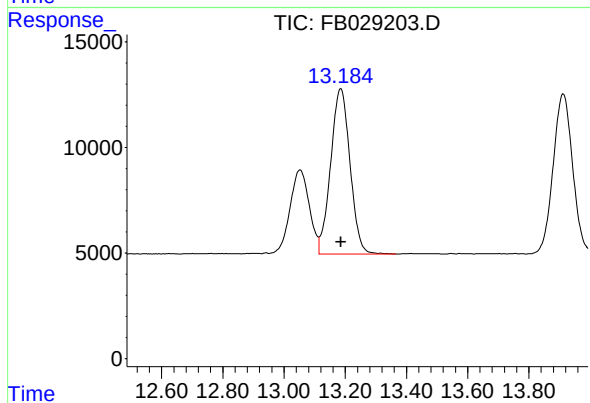

#8 m-Xylene


R.T.: 13.185 min
Delta R.T.: 0.000 min
Response: 344393
Conc: 20.56 ng/ml

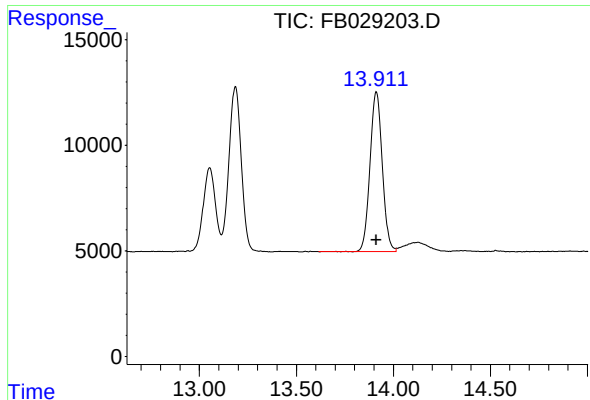

#9 O-Xylene

R.T.: 13.912 min
Delta R.T.: 0.000 min
Response: 334734
Conc: 20.16 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0201S2

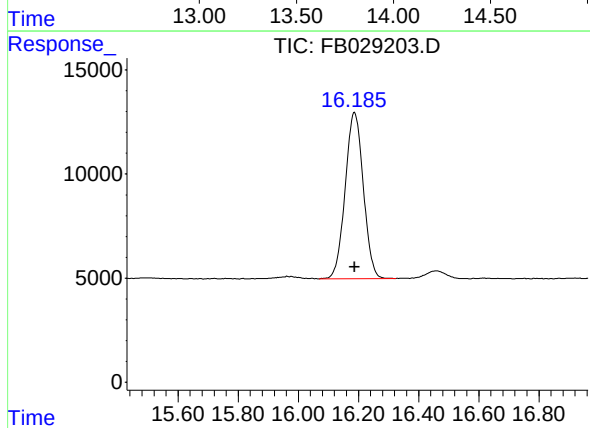

#10 1,2,4-Trimethylbenzene

R.T.: 16.187 min
Delta R.T.: 0.000 min
Response: 335182
Conc: 19.76 ng/ml