

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020123\
 Data File : FB029207.D
 Signal(s) : FID2B.CH
 Acq On : 1 Feb 2023 20:04
 Operator : AJ/MA
 Sample : BSF0201S3
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0201S3

Integration File: Calibration.e
 Quant Time: Feb 02 04:43:32 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB013123.M
 Quant Title :
 QLast Update : Tue Jan 31 12:31:55 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	228613	19.151 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.709	296448	25.796 ng/ml
2) t 2,2,4-Trimethylpentane	7.421	415260	29.329 ng/ml
3) t n-Heptane	7.748	99469	7.995 ng/ml
4) t Benzene	7.884	159893	8.873 ng/ml
6) t Toluene	10.617	479501	27.345 ng/ml
7) t Ethylbenzene	13.054	158113	9.356 ng/ml
8) t m-Xylene	13.186	317892	18.975 ng/ml
9) t O-Xylene	13.913	321823	19.378 ng/ml
10) t 1,2,4-Trimethylbenzene	16.188	349313	20.595 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020123\
Data File : FB029207.D
Signal(s) : FID2B.CH
Acq On : 1 Feb 2023 20:04
Operator : AJ/MA
Sample : BSF0201S3
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0201S3

Integration File: Calibration.e
Quant Time: Feb 02 04:43:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB013123.M
Quant Title :
QLast Update : Tue Jan 31 12:31:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

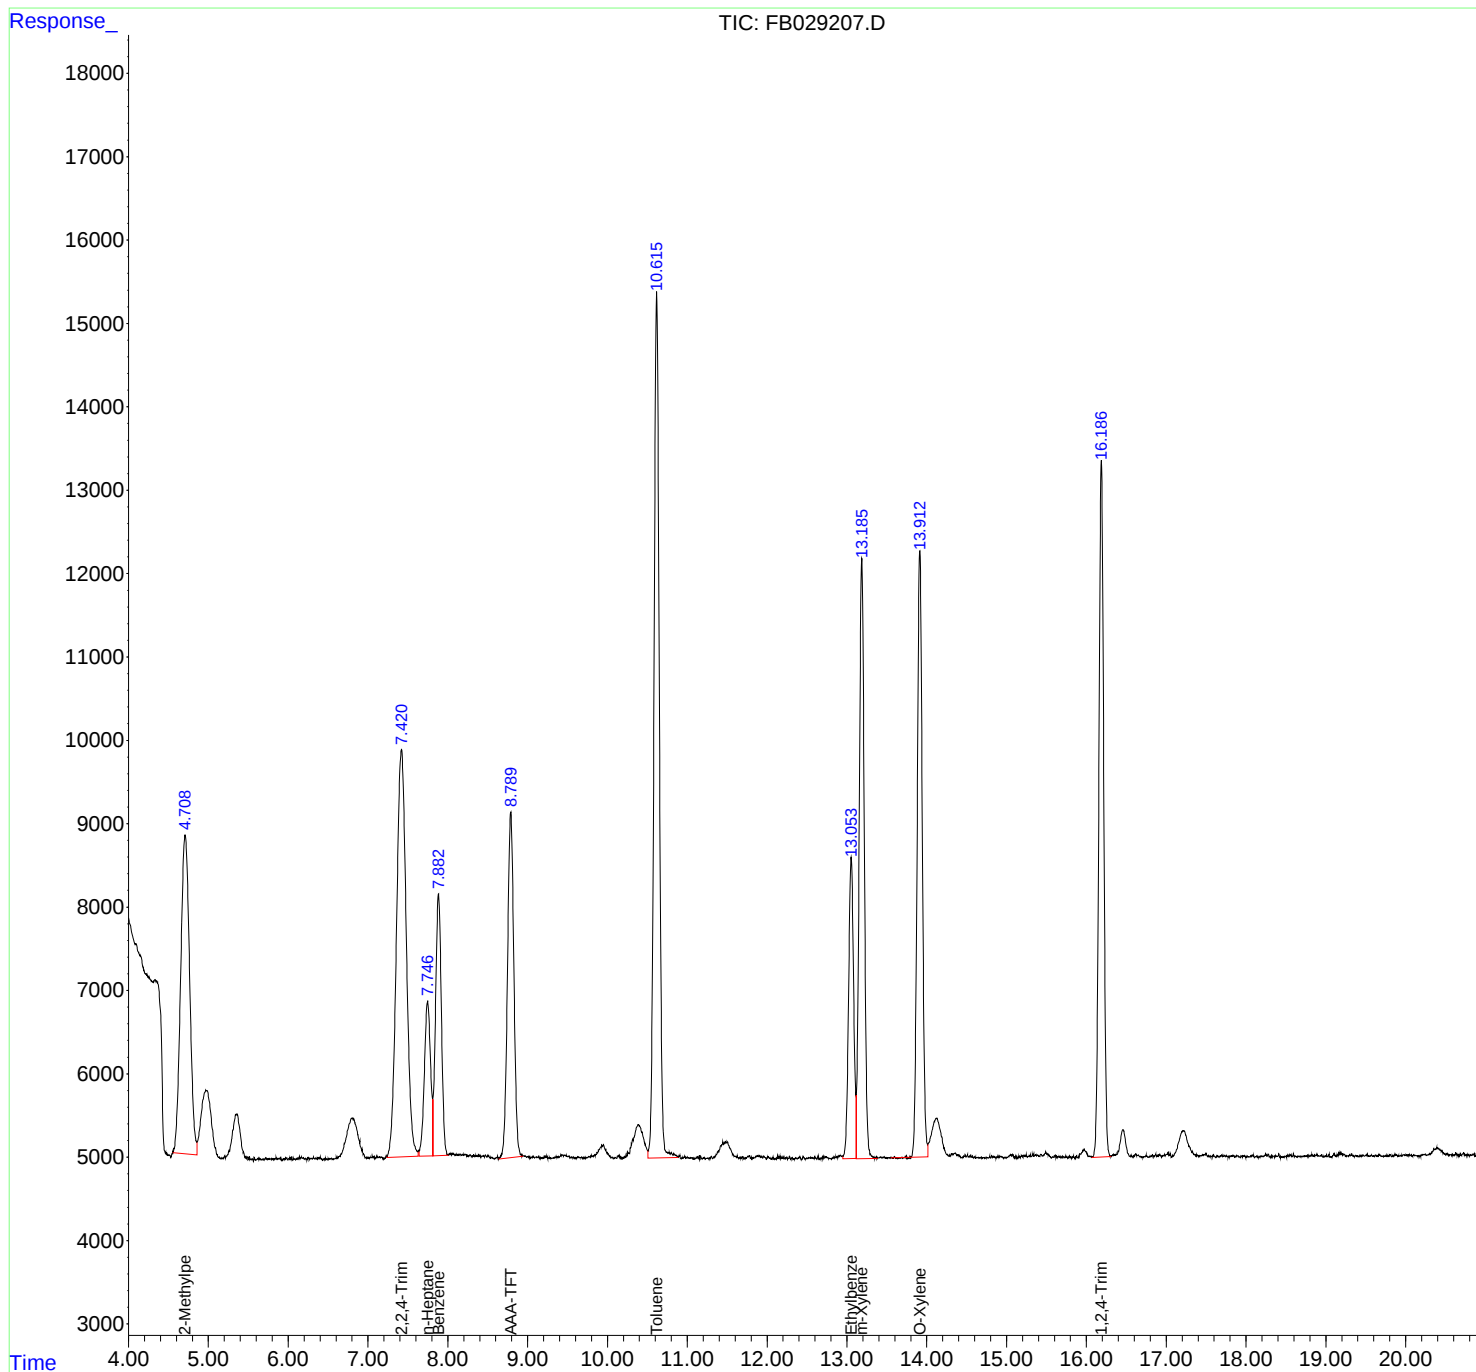


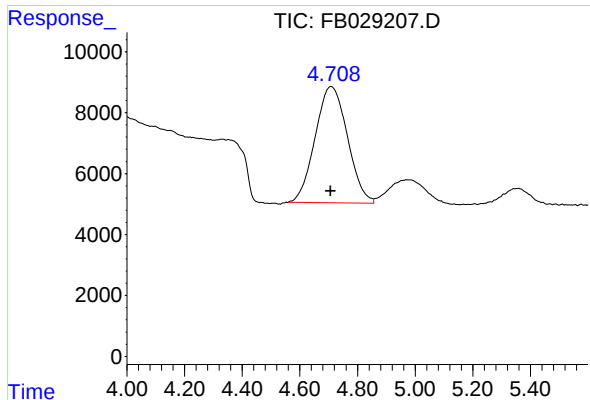

#1 2-Methylpentane


R.T.: 4.709 min
Delta R.T.: 0.002 min
Response: 296448
Conc: 25.80 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0201S3

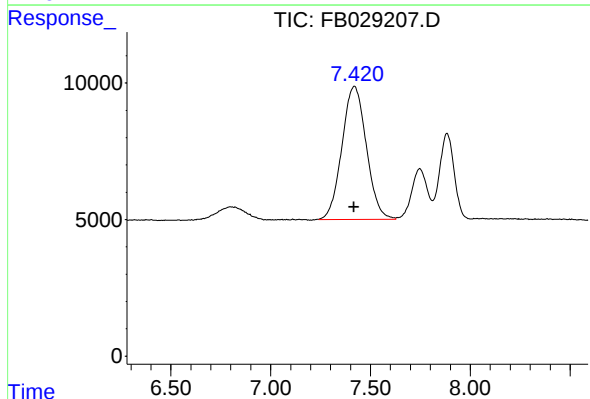


#2 2,2,4-Trimethylpentane

R.T.: 7.421 min
Delta R.T.: 0.004 min
Response: 415260
Conc: 29.33 ng/ml

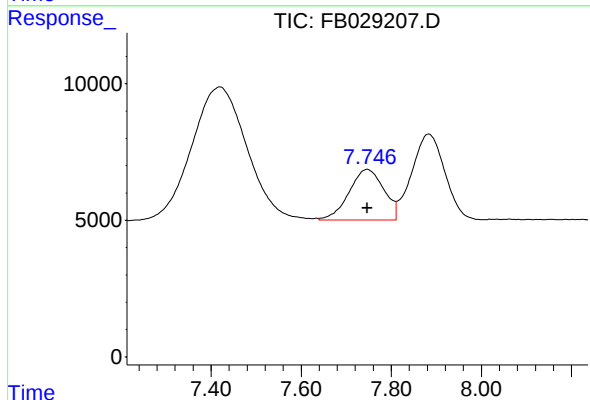


#3 n-Heptane

R.T.: 7.748 min
Delta R.T.: 0.001 min
Response: 99469
Conc: 8.00 ng/ml

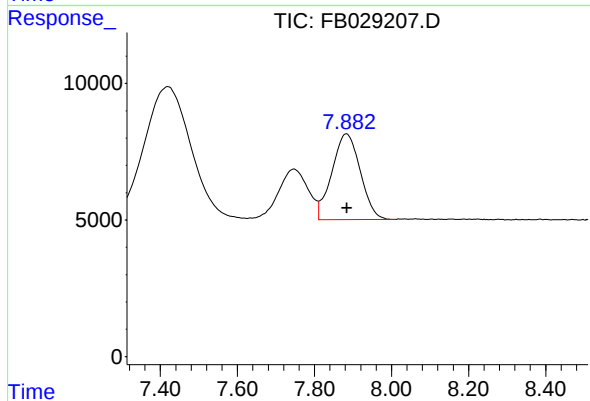

#4 Benzene


R.T.: 7.884 min
Delta R.T.: 0.000 min
Response: 159893
Conc: 8.87 ng/ml

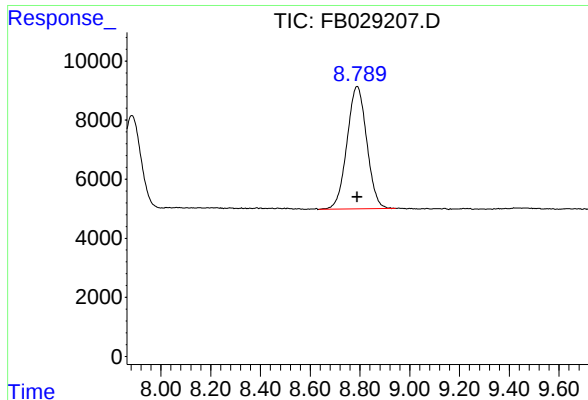

#5 AAA-TFT


R.T.: 8.789 min
Delta R.T.: 0.001 min
Response: 228613
Conc: 19.15 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0201S3

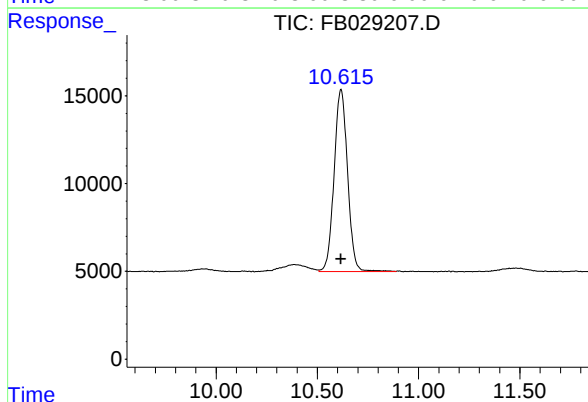


#6 Toluene

R.T.: 10.617 min
Delta R.T.: 0.000 min
Response: 479501
Conc: 27.34 ng/ml

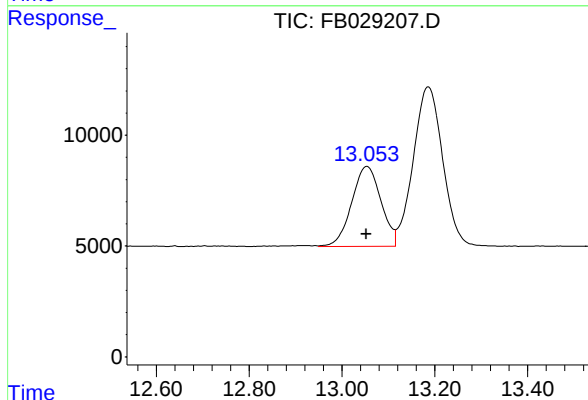


#7 Ethylbenzene

R.T.: 13.054 min
Delta R.T.: 0.002 min
Response: 158113
Conc: 9.36 ng/ml

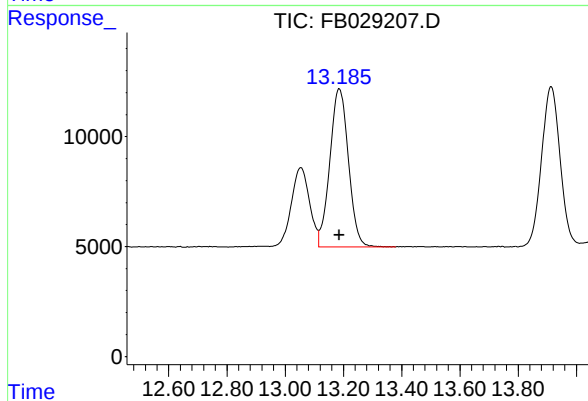

#8 m-Xylene


R.T.: 13.186 min
Delta R.T.: 0.001 min
Response: 317892
Conc: 18.97 ng/ml

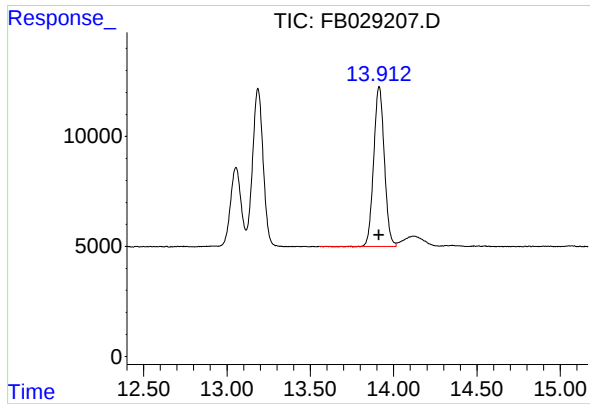

#9 O-Xylene

R.T.: 13.913 min
Delta R.T.: 0.001 min
Response: 321823
Conc: 19.38 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0201S3

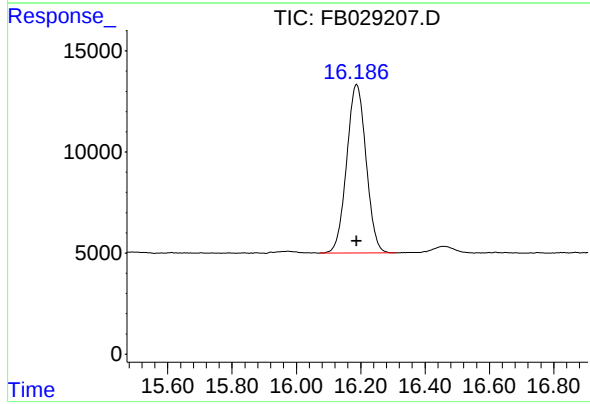

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: 0.000 min
Response: 349313
Conc: 20.60 ng/ml