

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020323\
Data File : FB029213.D
Signal(s) : FID2B.CH
Acq On : 3 Feb 2023 11:12
Operator : AJ/MA
Sample : 01418-03
Misc : 5.63G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Feb 04 00:53:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB013123.M
Quant Title :
QLast Update : Tue Jan 31 12:31:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	199433	16.707 ng/ml
Target Compounds			
6) t Toluene	10.611	1179	0.067 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020323\
Data File : FB029213.D
Signal(s) : FID2B.CH
Acq On : 3 Feb 2023 11:12
Operator : AJ/MA
Sample : 01418-03
Misc : 5.63G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Feb 04 00:53:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB013123.M
Quant Title :
QLast Update : Tue Jan 31 12:31:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

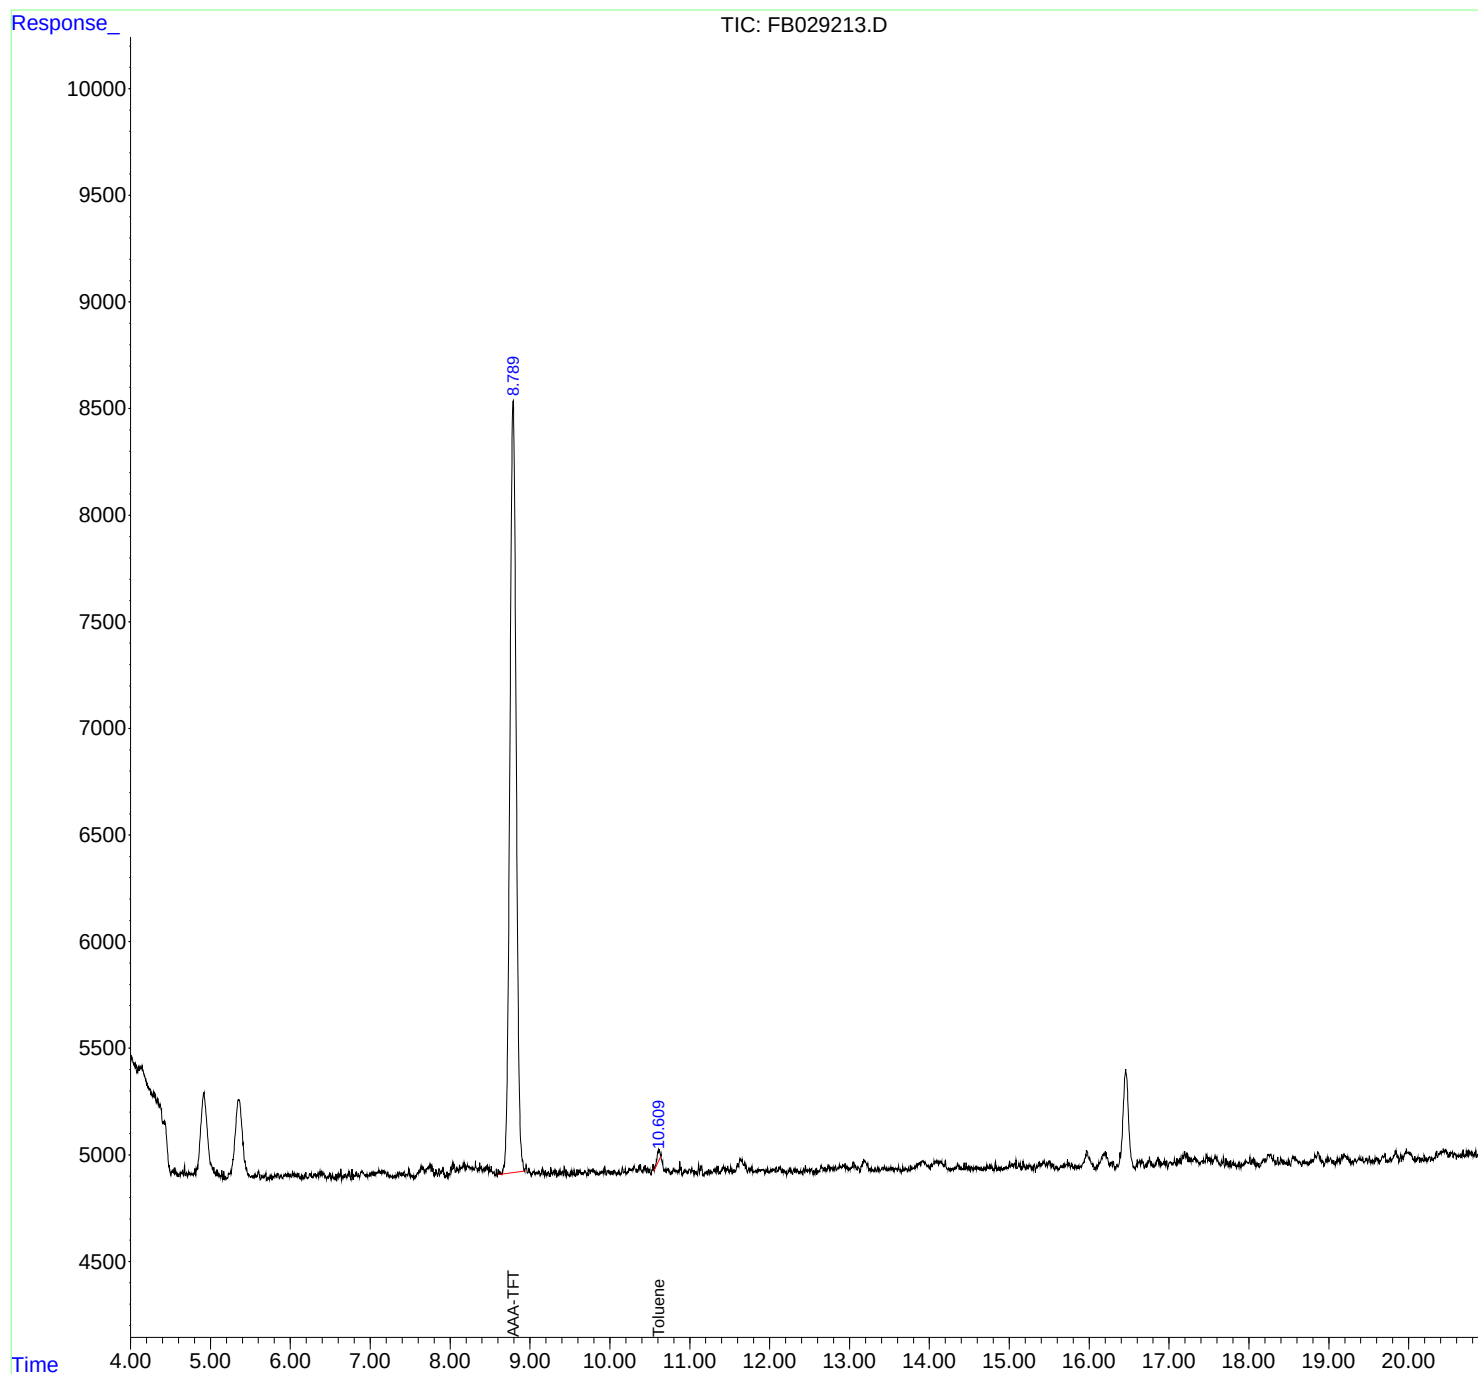


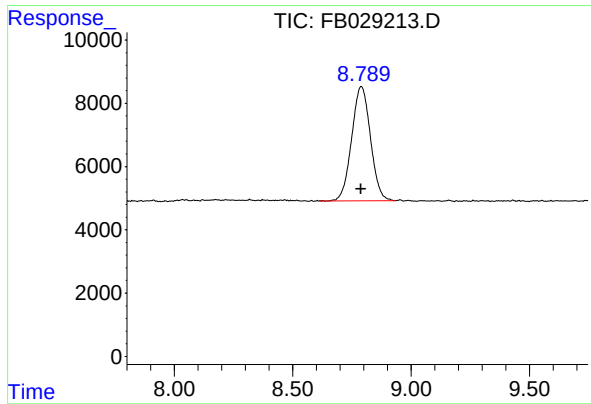

#5 AAA-TFT

R.T.: 8.790 min
Delta R.T.: 0.002 min
Response: 199433
Conc: 16.71 ng/ml

Instrument :
FID_B
ClientSampleId :

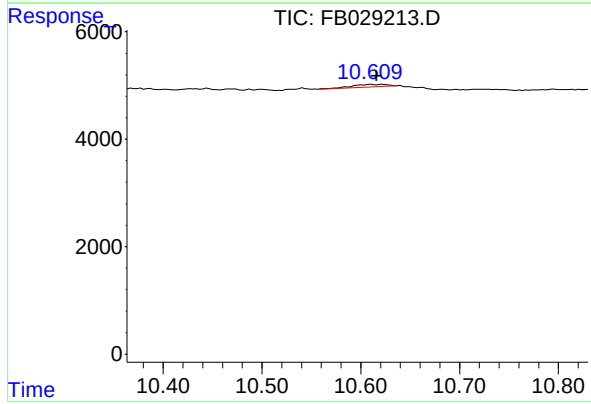

#6 Toluene

R.T.: 10.611 min
Delta R.T.: -0.005 min
Response: 1179
Conc: 0.07 ng/ml