

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020323\
 Data File : FB029223.D
 Signal(s) : FID2B.CH
 Acq On : 3 Feb 2023 17:26
 Operator : AJ/MA
 Sample : 01414-06MSD
 Misc : 5.07G/5.00 ML DI WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SASP2-123-2(75-80)MSD

Integration File: Calibration.e
 Quant Time: Feb 04 00:54:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB013123.M
 Quant Title :
 QLast Update : Tue Jan 31 12:31:55 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	167985	14.073 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.704	210744	18.339 ng/ml
2) t 2,2,4-Trimethylpentane	7.411	261709	18.484 ng/ml
3) t n-Heptane	7.747	59409	4.775 ng/ml
4) t Benzene	7.884	126930	7.044 ng/ml
6) t Toluene	10.617	357212	20.371 ng/ml
7) t Ethylbenzene	13.054	112680	6.668 ng/ml
8) t m-Xylene	13.187	221334	13.211 ng/ml
9) t O-Xylene	13.913	227918	13.723 ng/ml
10) t 1,2,4-Trimethylbenzene	16.188	211477	12.468 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020323\
Data File : FB029223.D
Signal(s) : FID2B.CH
Acq On : 3 Feb 2023 17:26
Operator : AJ/MA
Sample : 01414-06MSD
Misc : 5.07G/5.00 ML DI WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SASP2-123-2(75-80)MSD

Integration File: Calibration.e
Quant Time: Feb 04 00:54:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB013123.M
Quant Title :
QLast Update : Tue Jan 31 12:31:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

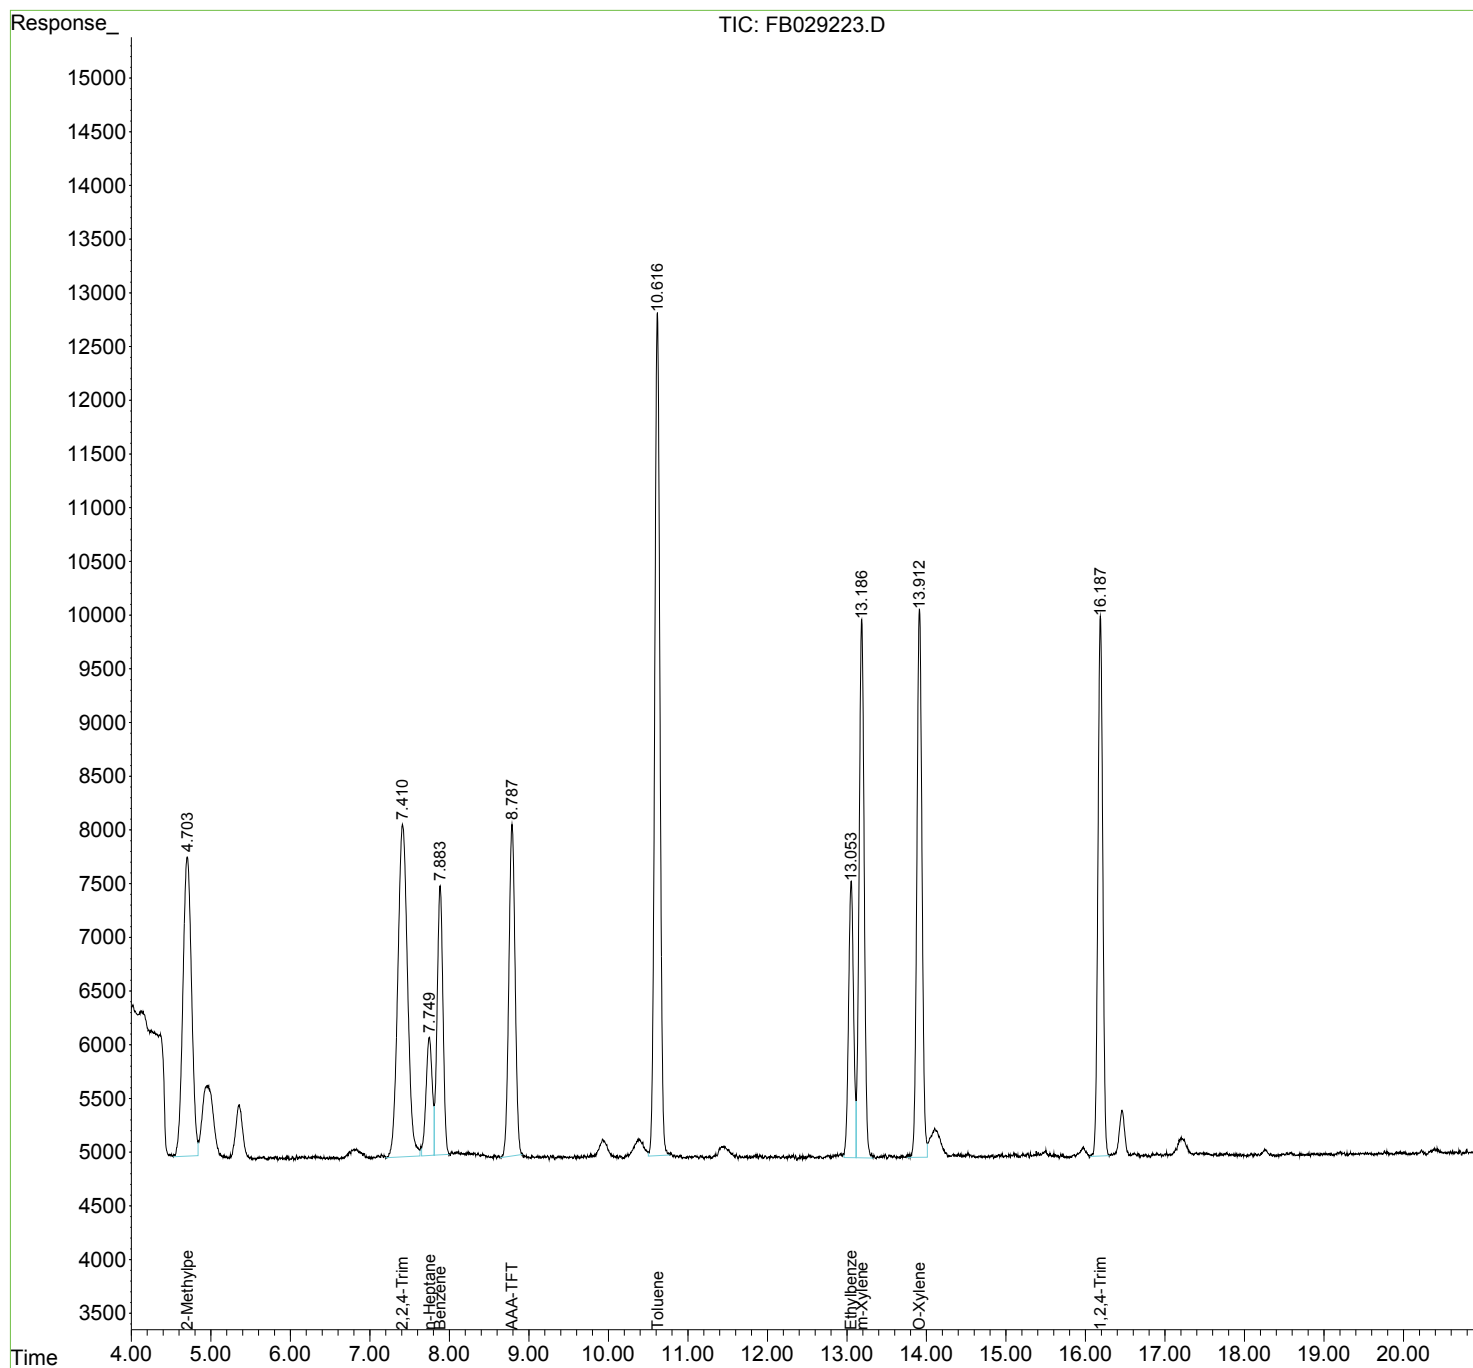


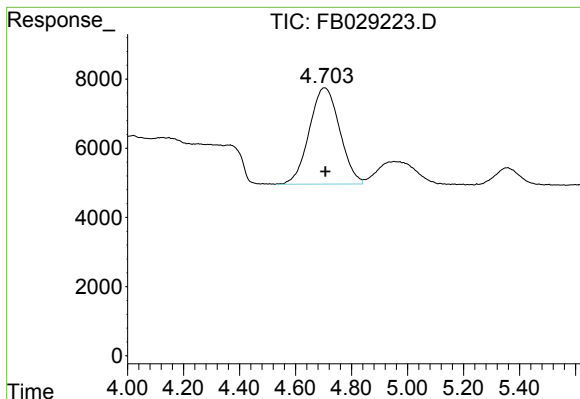

#1 2-Methylpentane


R.T.: 4.704 min
Delta R.T.: -0.003 min
Response: 210744
Conc: 18.34 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-123-2(75-80)MSD

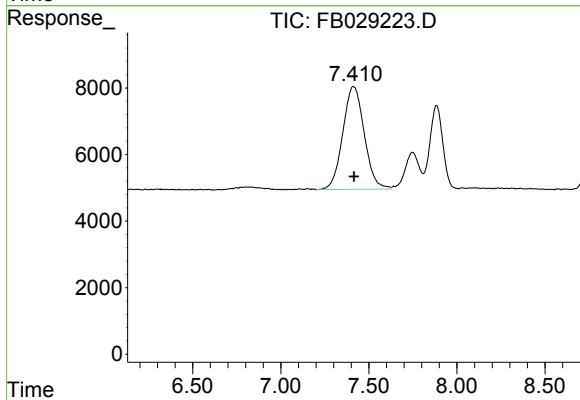


#2 2,2,4-Trimethylpentane

R.T.: 7.411 min
Delta R.T.: -0.006 min
Response: 261709
Conc: 18.48 ng/ml

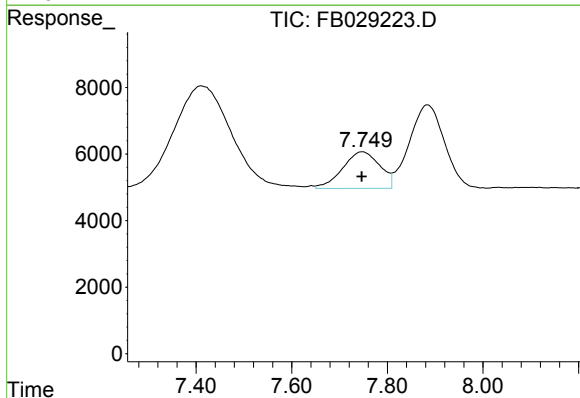


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: 0.000 min
Response: 59409
Conc: 4.78 ng/ml

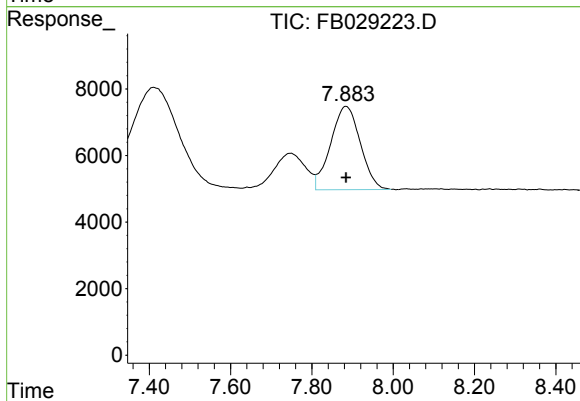

#4 Benzene


R.T.: 7.884 min
Delta R.T.: 0.000 min
Response: 126930
Conc: 7.04 ng/ml

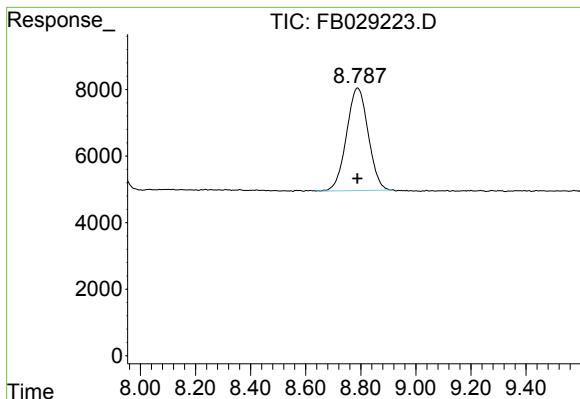

#5 AAA-TFT


R.T.: 8.789 min
Delta R.T.: 0.000 min
Response: 167985
Conc: 14.07 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-123-2(75-80)MSD

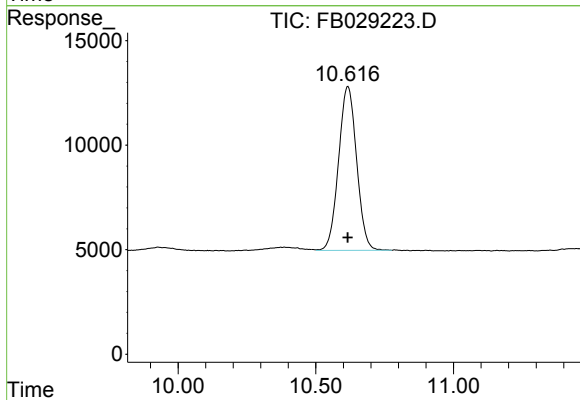


#6 Toluene

R.T.: 10.617 min
Delta R.T.: 0.000 min
Response: 357212
Conc: 20.37 ng/ml

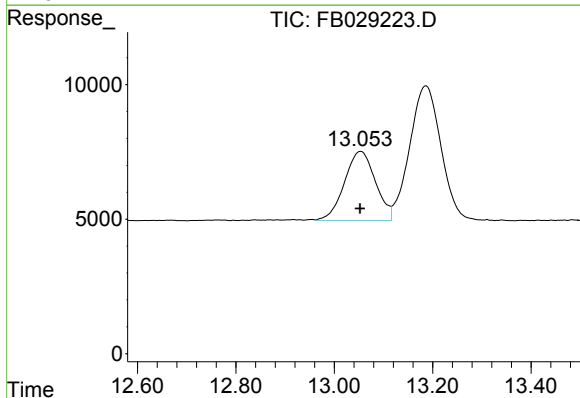


#7 Ethylbenzene

R.T.: 13.054 min
Delta R.T.: 0.002 min
Response: 112680
Conc: 6.67 ng/ml

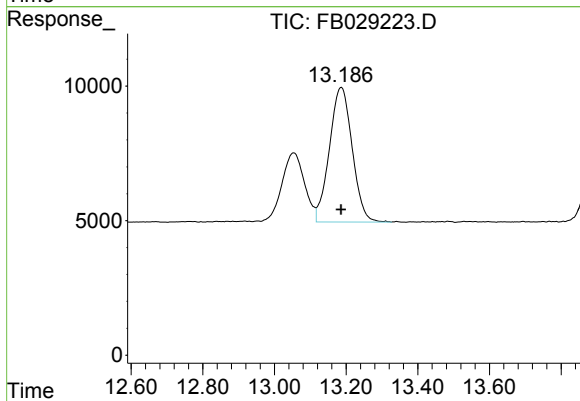

#8 m-Xylene


R.T.: 13.187 min
Delta R.T.: 0.002 min
Response: 221334
Conc: 13.21 ng/ml

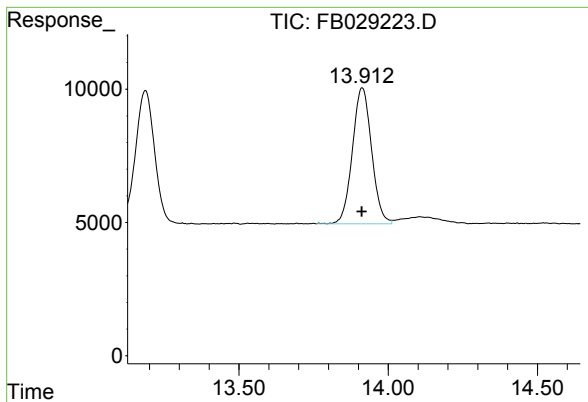

#9 O-Xylene

R.T.: 13.913 min
Delta R.T.: 0.001 min
Response: 227918
Conc: 13.72 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-123-2(75-80)MSD

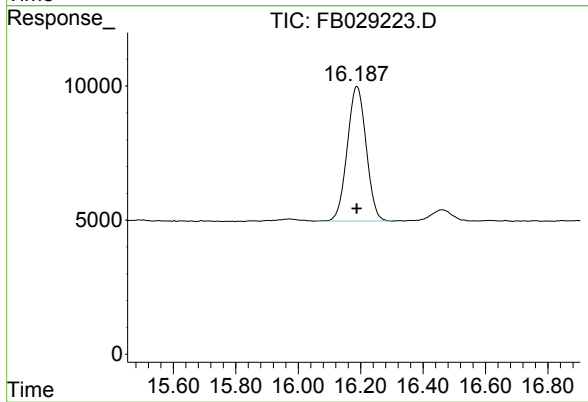

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: 0.001 min
Response: 211477
Conc: 12.47 ng/ml