

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020323\
Data File : FB029226.D
Signal(s) : FID2B.CH
Acq On : 3 Feb 2023 19:16
Operator : AJ/MA
Sample : 01414-06MSD
Misc : 5.02G/5.00 ML DI WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SASP2-123-2(75-80)MSD

Integration File: Calibration.e
Quant Time: Feb 04 00:54:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB013123.M
Quant Title :
QLast Update : Tue Jan 31 12:31:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020323\
Data File : FB029226.D
Signal(s) : FID2B.CH
Acq On : 3 Feb 2023 19:16
Operator : AJ/MA
Sample : 01414-06MSD
Misc : 5.02G/5.00 ML DI WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SASP2-123-2(75-80)MSD

Integration File: Calibration.e
Quant Time: Feb 04 00:54:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB013123.M
Quant Title :
QLast Update : Tue Jan 31 12:31:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

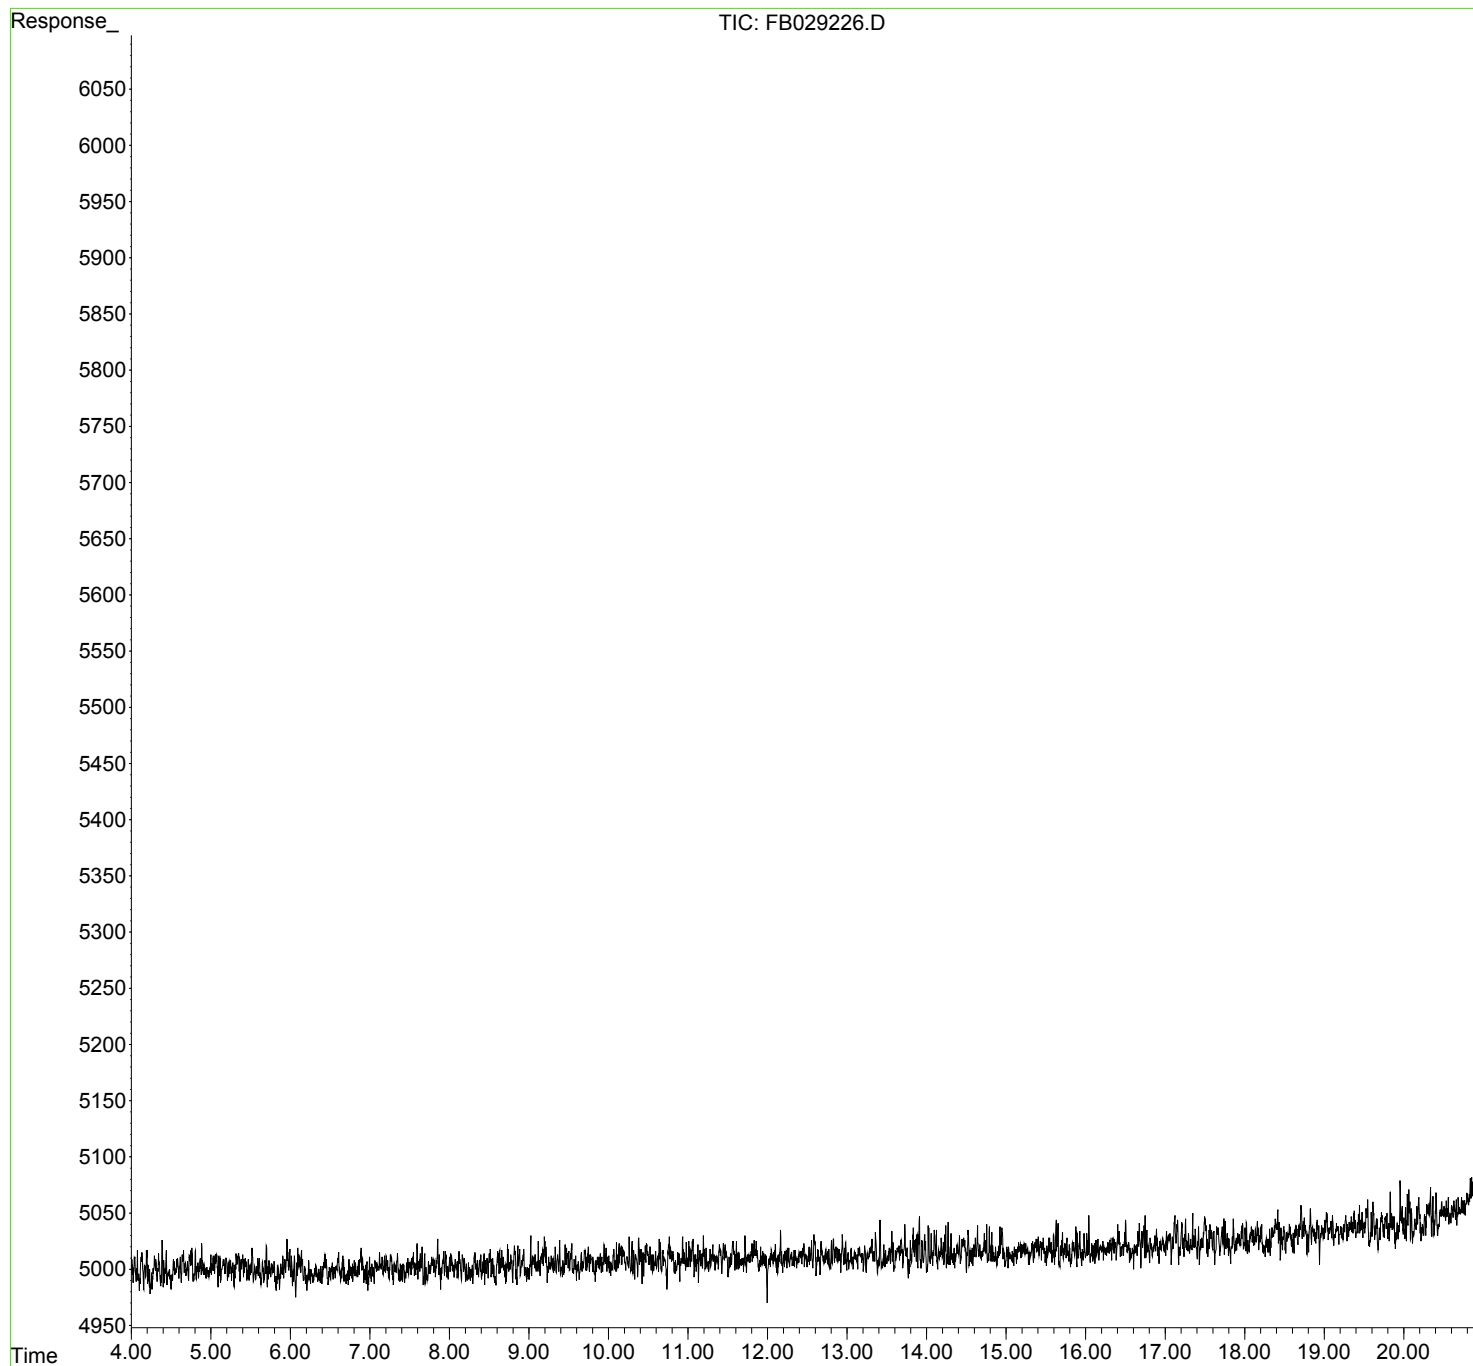

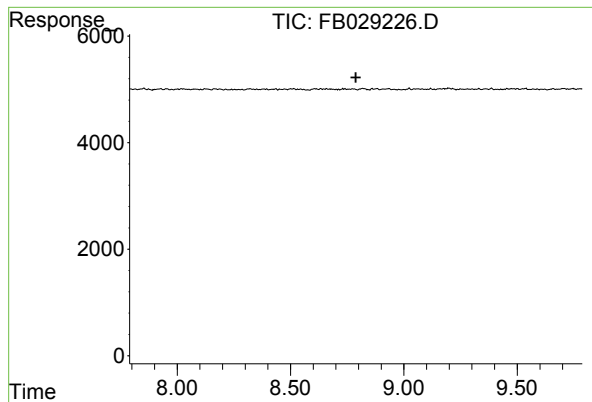

#5 AAA-TFT

R.T.: 0.000 min
Exp R.T.: 8.788 min
Response: 0
Conc: N.D.

Instrument :

FID_B

ClientSampleId :

SASP2-123-2(75-80)MSD