

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020323\
 Data File : FB029228.D
 Signal(s) : FID2B.CH
 Acq On : 3 Feb 2023 20:30
 Operator : AJ/MA
 Sample : 01414-06MS 50X
 Misc : 5.00G/5.00 ML MEOH
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SASP2-123-2(75-80)MS

Integration File: Calibration.e
 Quant Time: Feb 04 00:54:48 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB013123.M
 Quant Title :
 QLast Update : Tue Jan 31 12:31:55 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.783	184373	15.445 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.702	175992	15.314 ng/ml
2) t 2,2,4-Trimethylpentane	7.409	263115	18.584 ng/ml
3) t n-Heptane	7.744	67205	5.402 ng/ml
4) t Benzene	7.879	116889	6.486 ng/ml
6) t Toluene	10.613	347932	19.842 ng/ml
7) t Ethylbenzene	13.051	113858	6.737 ng/ml
8) t m-Xylene	13.183	226335	13.510 ng/ml
9) t O-Xylene	13.910	228529	13.760 ng/ml
10) t 1,2,4-Trimethylbenzene	16.185	228498	13.472 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020323\
Data File : FB029228.D
Signal(s) : FID2B.CH
Acq On : 3 Feb 2023 20:30
Operator : AJ/MA
Sample : 01414-06MS 50X
Misc : 5.00G/5.00 ML MEOH
ALS Vial : 20 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SASP2-123-2(75-80)MS

Integration File: Calibration.e
Quant Time: Feb 04 00:54:48 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB013123.M
Quant Title :
QLast Update : Tue Jan 31 12:31:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

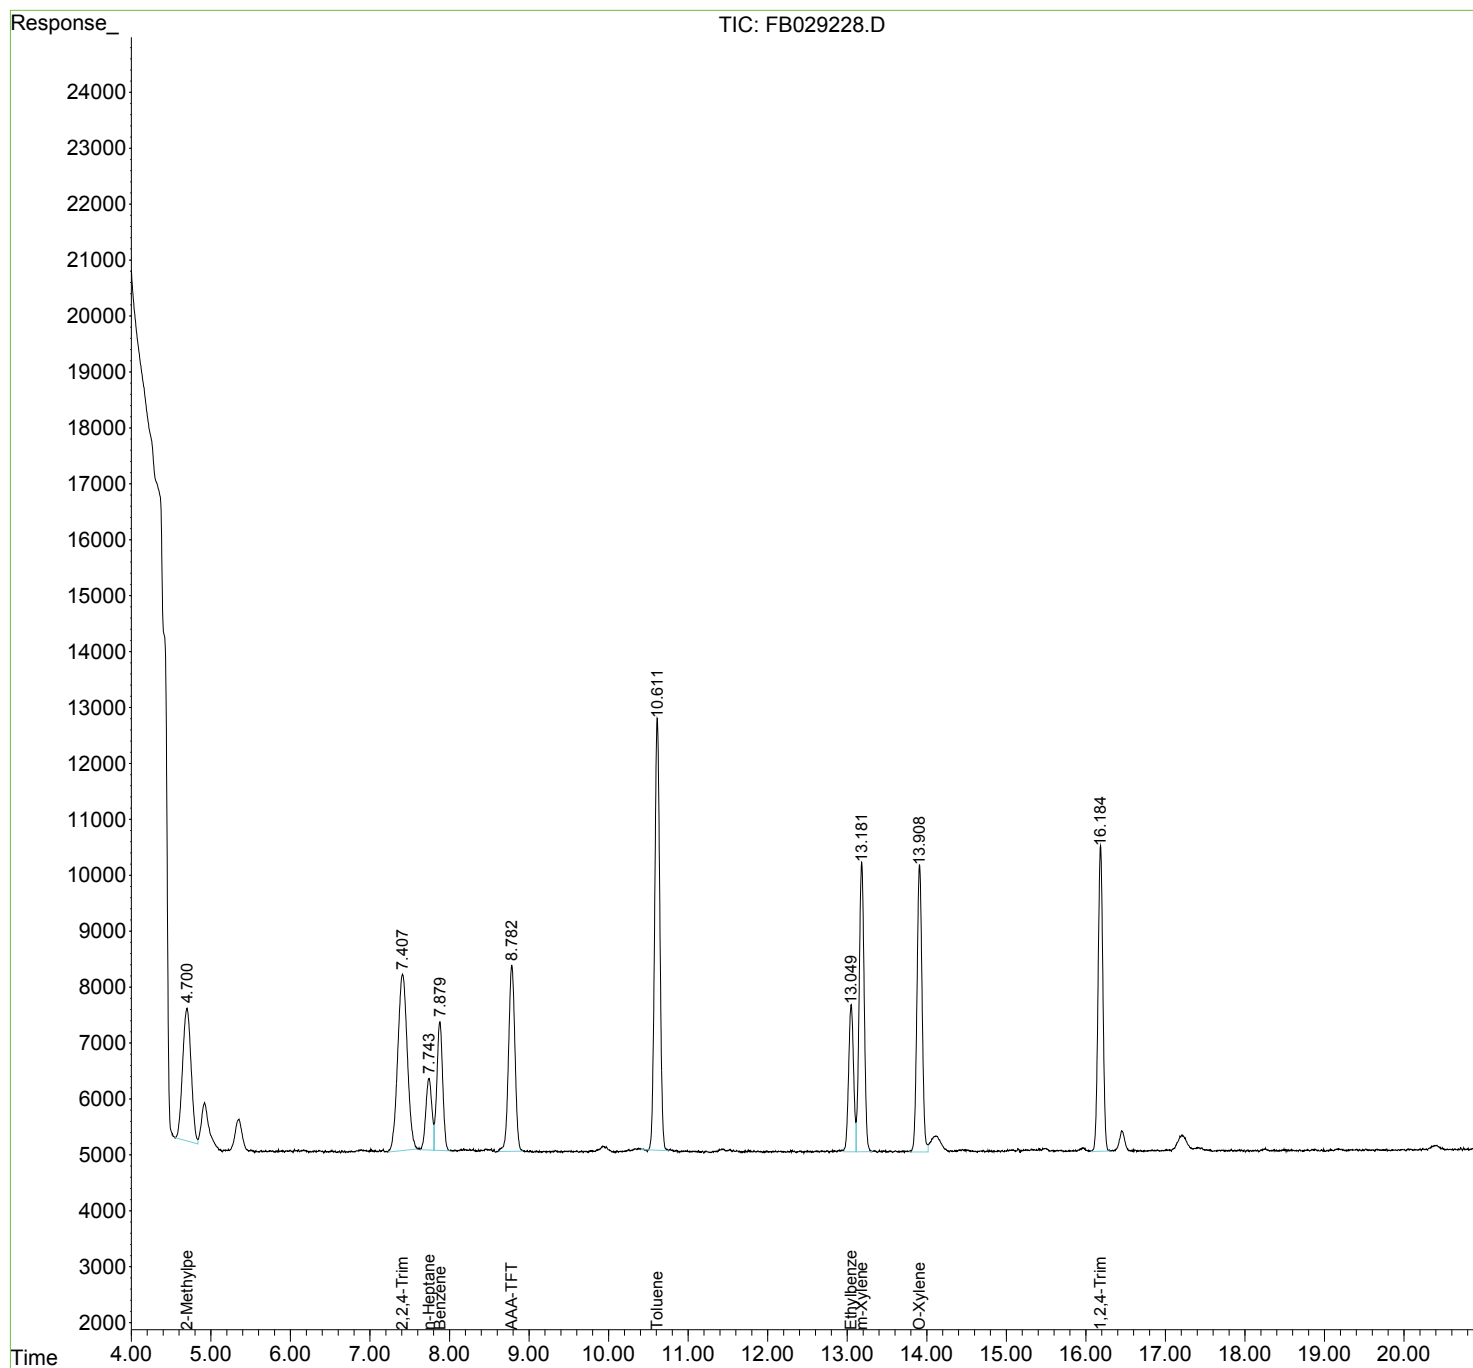


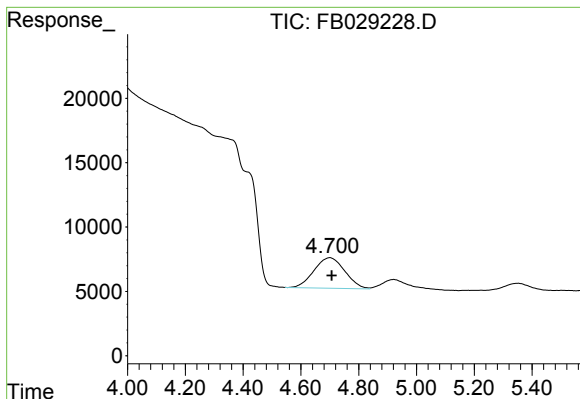

#1 2-Methylpentane


R.T.: 4.702 min
Delta R.T.: -0.005 min
Response: 175992
Conc: 15.31 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-123-2(75-80)MS

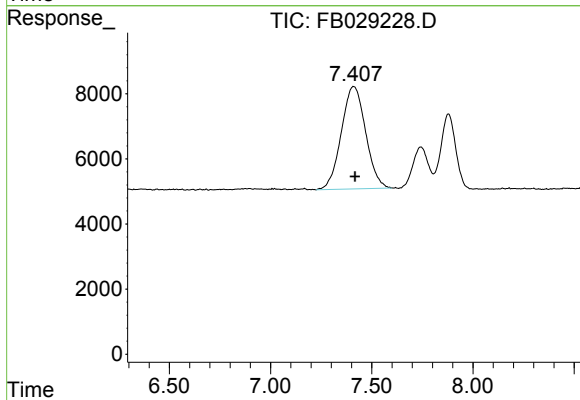


#2 2,2,4-Trimethylpentane

R.T.: 7.409 min
Delta R.T.: -0.008 min
Response: 263115
Conc: 18.58 ng/ml

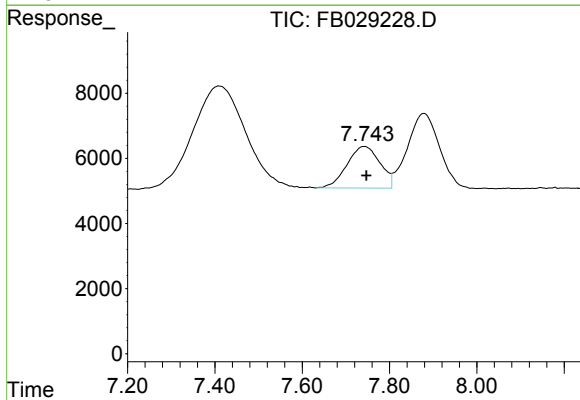


#3 n-Heptane

R.T.: 7.744 min
Delta R.T.: -0.003 min
Response: 67205
Conc: 5.40 ng/ml

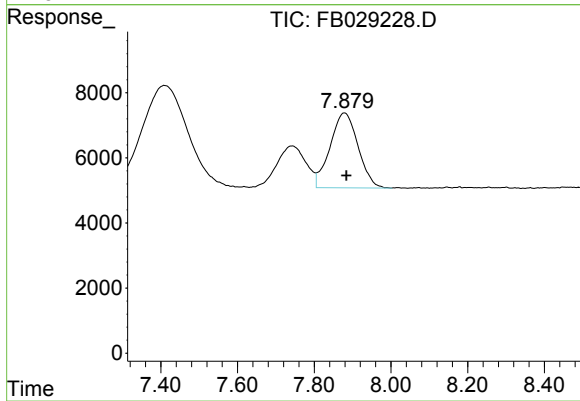

#4 Benzene


R.T.: 7.879 min
Delta R.T.: -0.005 min
Response: 116889
Conc: 6.49 ng/ml

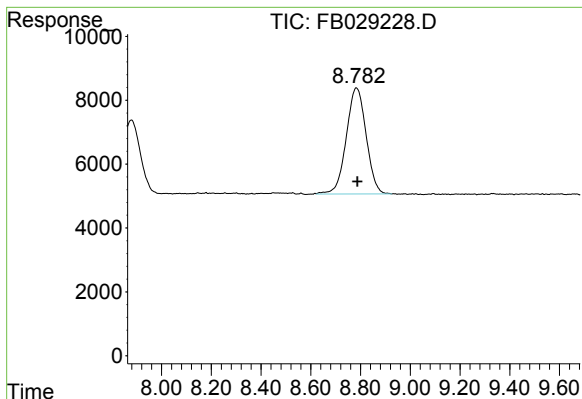

#5 AAA-TFT


R.T.: 8.783 min
Delta R.T.: -0.005 min
Response: 184373
Conc: 15.45 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-123-2(75-80)MS

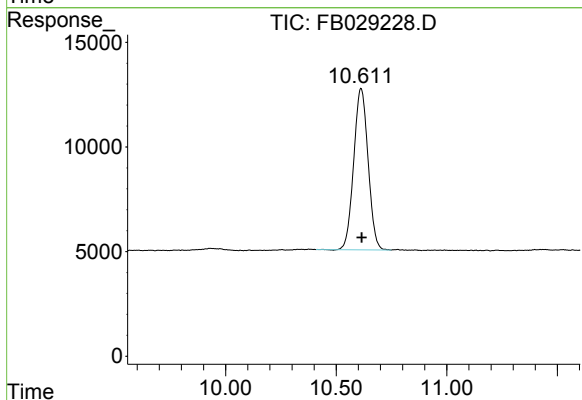


#6 Toluene

R.T.: 10.613 min
Delta R.T.: -0.004 min
Response: 347932
Conc: 19.84 ng/ml

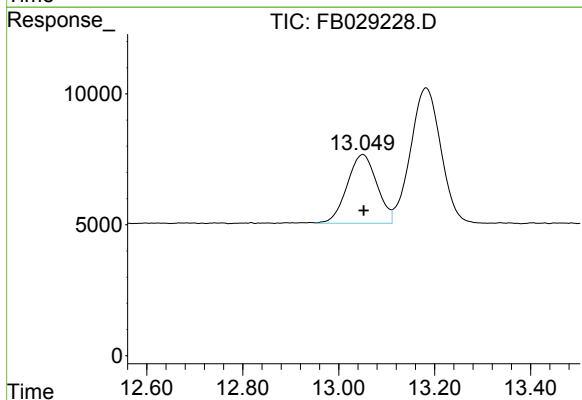


#7 Ethylbenzene

R.T.: 13.051 min
Delta R.T.: -0.002 min
Response: 113858
Conc: 6.74 ng/ml

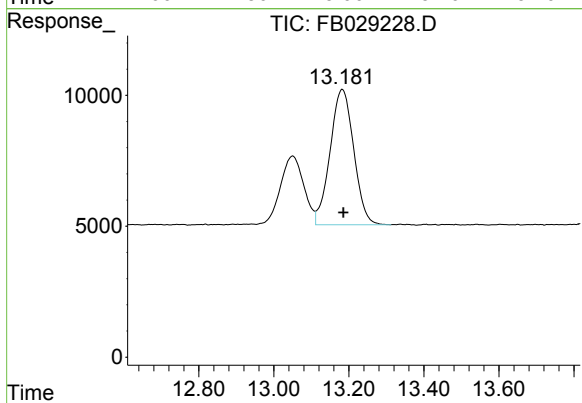

#8 m-Xylene


R.T.: 13.183 min
Delta R.T.: -0.002 min
Response: 226335
Conc: 13.51 ng/ml

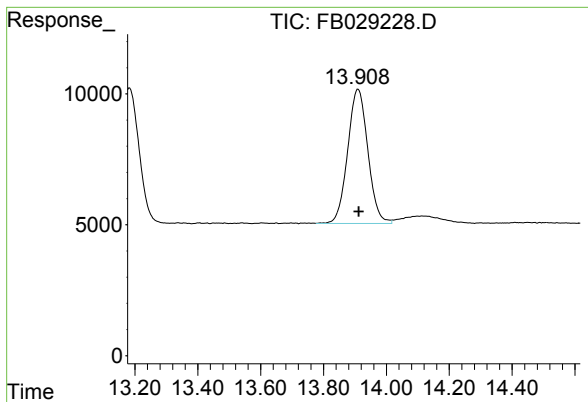

#9 O-Xylene

R.T.: 13.910 min
Delta R.T.: -0.002 min
Response: 228529
Conc: 13.76 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-123-2(75-80)MS

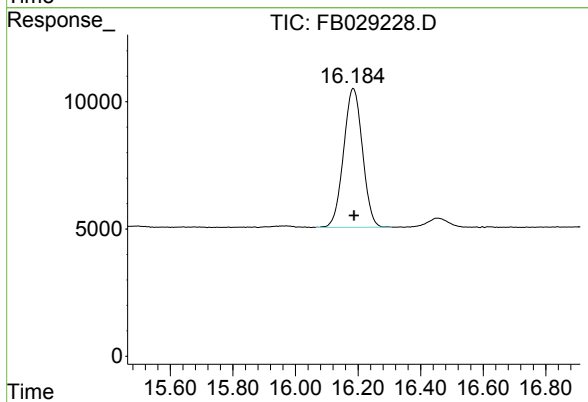

#10 1,2,4-Trimethylbenzene

R.T.: 16.185 min
Delta R.T.: -0.002 min
Response: 228498
Conc: 13.47 ng/ml