

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020325\
Data File : FB031440.D
Signal(s) : FID2B.CH
Acq On : 3 Feb 2025 11:47
Operator : YP/AJ
Sample : VBF0203S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Feb 04 00:18:25 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011525.M
Quant Title :
QLast Update : Wed Jan 15 12:01:08 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	440367	18.462 ng/ml
Target Compounds			
6) t Toluene	10.611	3981	0.102 ng/ml
8) t m-Xylene	13.188	5056	0.135 ng/ml
9) t O-Xylene	13.912	5864	0.165 ng/ml
10) t 1,2,4-Trimethylbenzene	16.199	10110	0.357 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020325\
Data File : FB031440.D
Signal(s) : FID2B.CH
Acq On : 3 Feb 2025 11:47
Operator : YP/AJ
Sample : VBF0203S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Feb 04 00:18:25 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011525.M
Quant Title :
QLast Update : Wed Jan 15 12:01:08 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

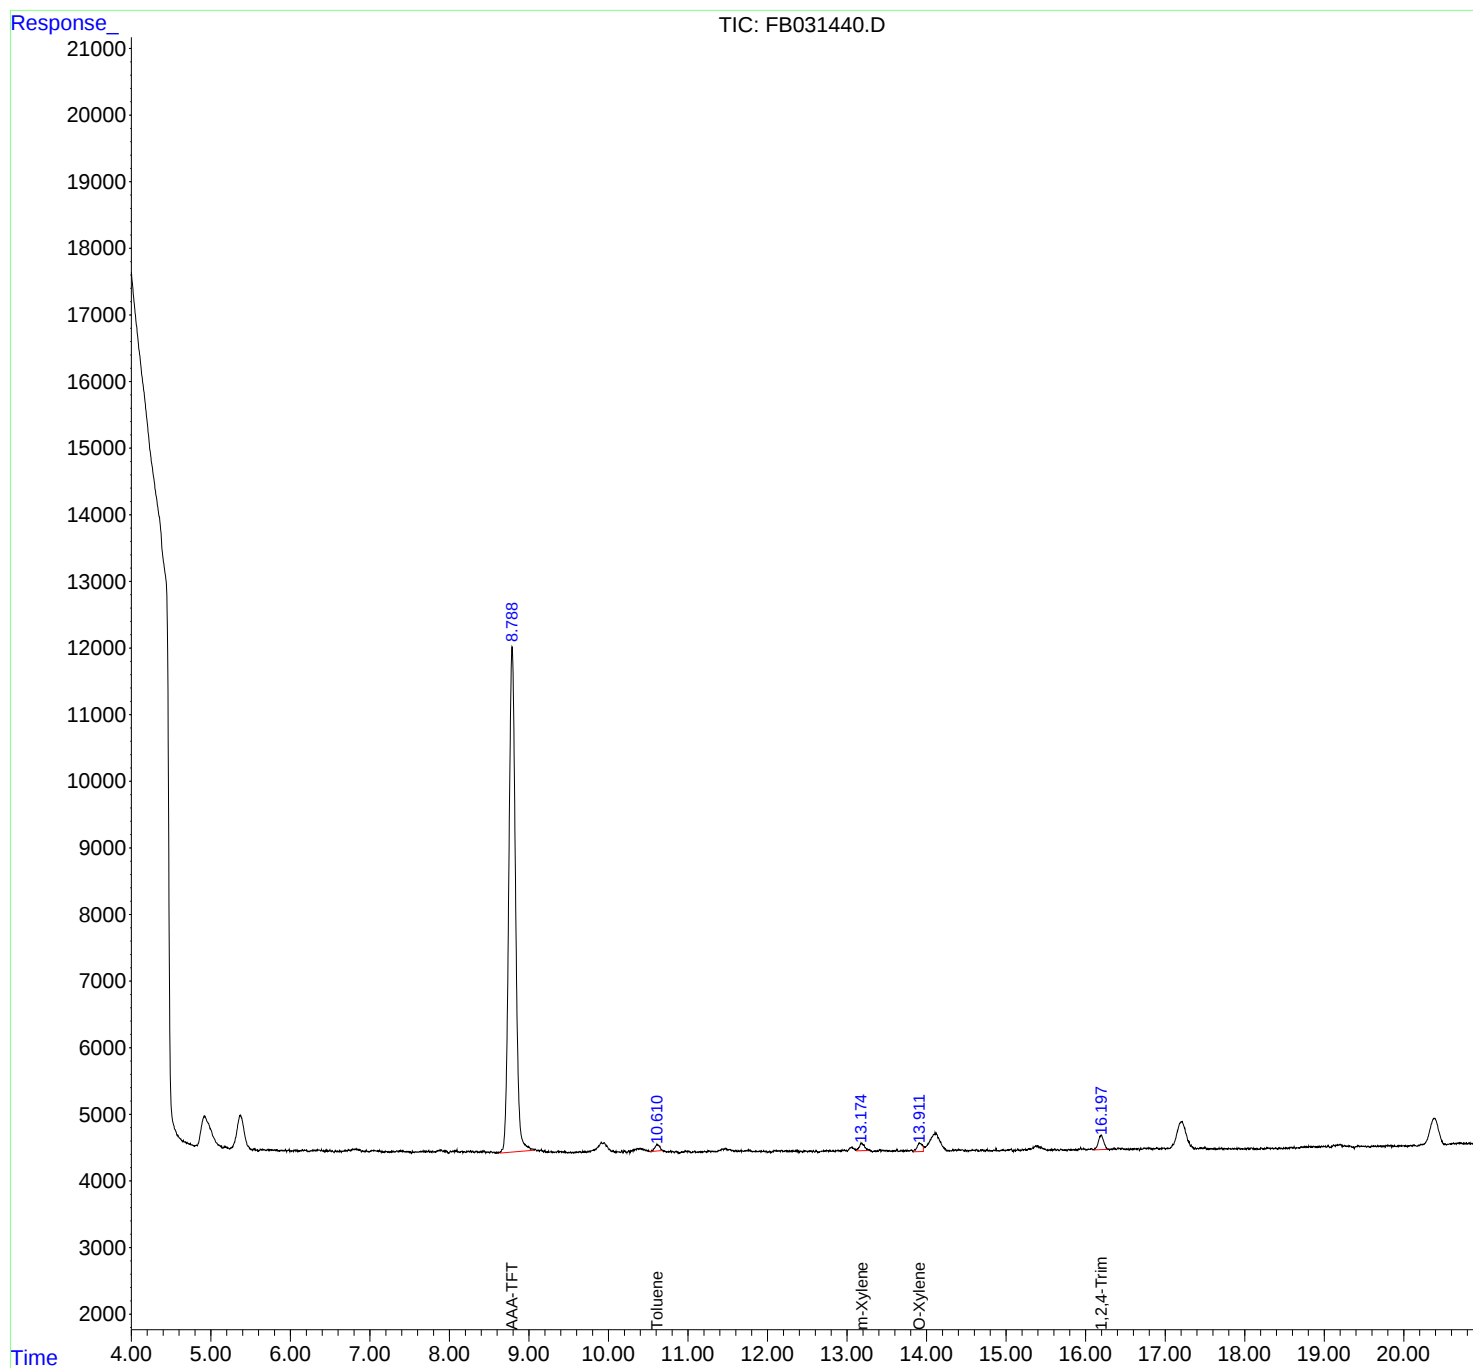


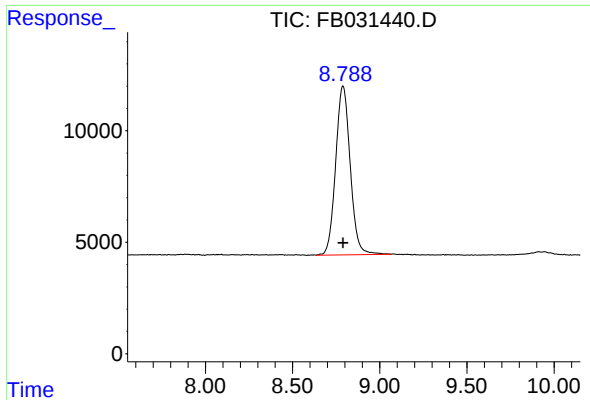

#5 AAA-TFT


R.T.: 8.789 min
Delta R.T.: 0.000 min
Response: 440367
Conc: 18.46 ng/ml

Instrument :
FID_B
ClientSampleId :

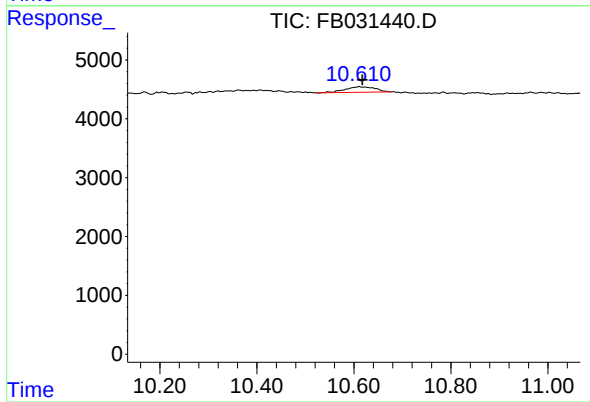


#6 Toluene

R.T.: 10.611 min
Delta R.T.: -0.006 min
Response: 3981
Conc: 0.10 ng/ml

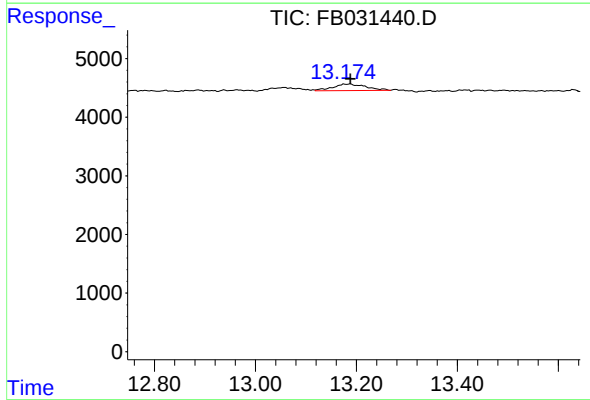


#8 m-Xylene

R.T.: 13.188 min
Delta R.T.: 0.000 min
Response: 5056
Conc: 0.14 ng/ml

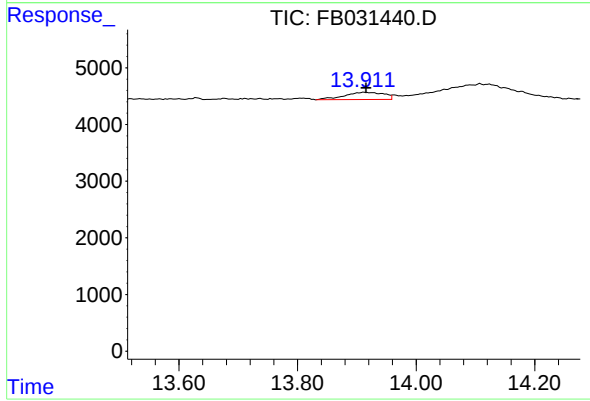

#9 O-Xylene

R.T.: 13.912 min
Delta R.T.: -0.003 min
Response: 5864
Conc: 0.16 ng/ml

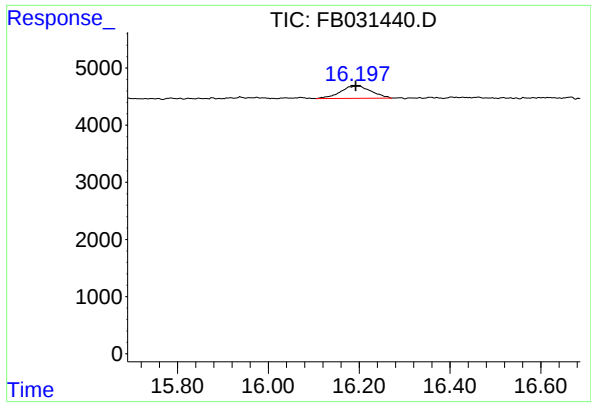

#10 1,2,4-Trimethylbenzene

R.T.: 16.199 min
Delta R.T.: 0.007 min
Response: 10110
Conc: 0.36 ng/ml

Instrument :
FID_B
ClientSampleId :