

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020325\
 Data File : FB031447.D
 Signal(s) : FID2B.CH
 Acq On : 3 Feb 2025 15:07
 Operator : YP/AJ
 Sample : BSF0203S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0203S2

Integration File: Calibration.e
 Quant Time: Feb 04 00:19:42 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011525.M
 Quant Title :
 QLast Update : Wed Jan 15 12:01:08 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	452091	18.953 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.719	622875	18.792 ng/ml
2) t 2,2,4-Trimethylpentane	7.421	893587	23.761 ng/ml
3) t n-Heptane	7.753	254122	7.040 ng/ml
4) t Benzene	7.892	375513	8.817 ng/ml
6) t Toluene	10.621	1068978	27.377 ng/ml
7) t Ethylbenzene	13.057	306856	8.861 ng/ml
8) t m-Xylene	13.191	663787	17.758 ng/ml
9) t O-Xylene	13.919	627752	17.627 ng/ml
10) t 1,2,4-Trimethylbenzene	16.195	493135	17.412 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020325\
Data File : FB031447.D
Signal(s) : FID2B.CH
Acq On : 3 Feb 2025 15:07
Operator : YP/AJ
Sample : BSF0203S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0203S2

Integration File: Calibration.e
Quant Time: Feb 04 00:19:42 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011525.M
Quant Title :
QLast Update : Wed Jan 15 12:01:08 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

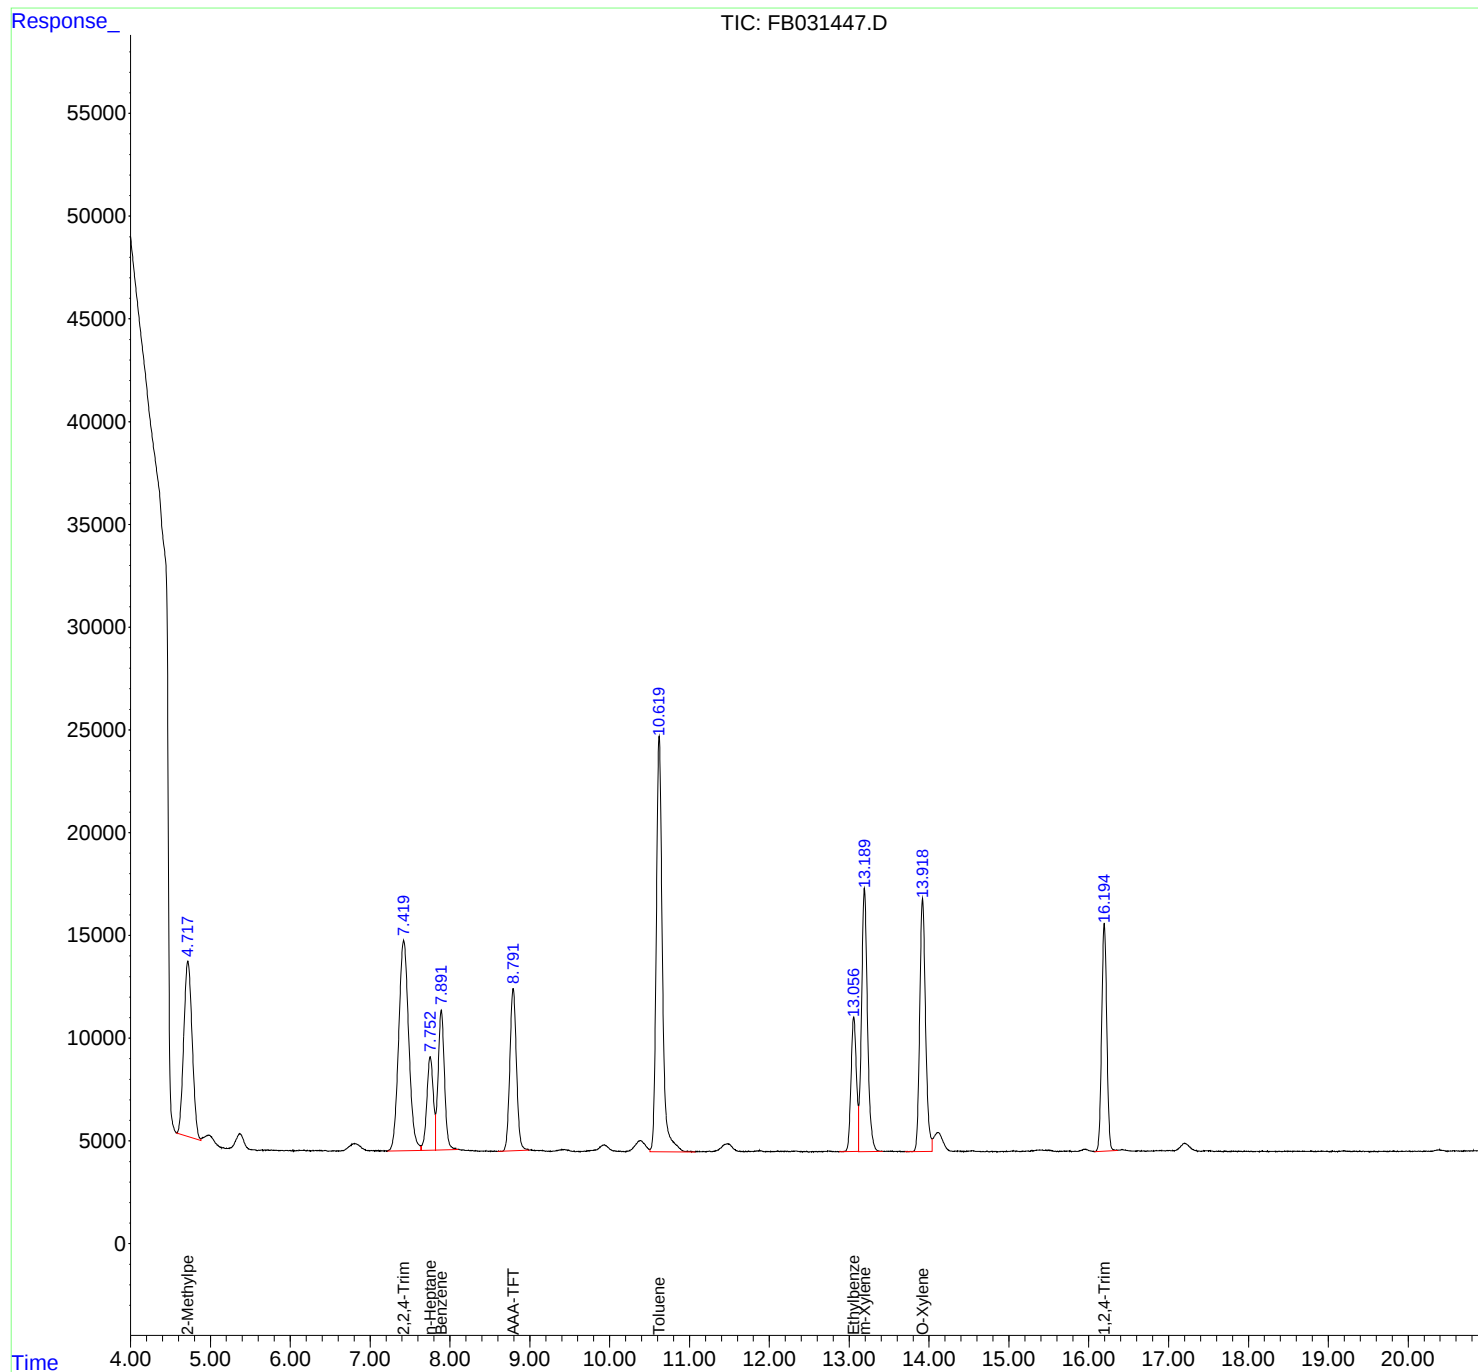


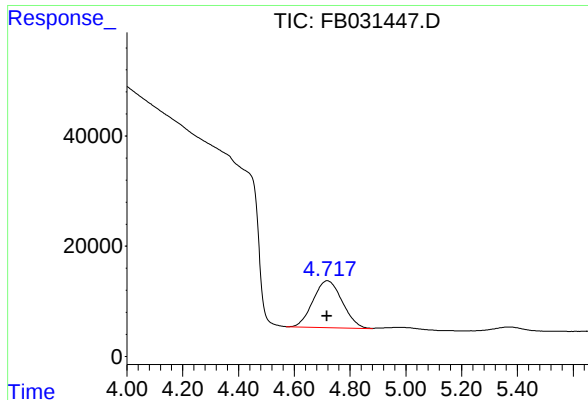

#1 2-Methylpentane


R.T.: 4.719 min
Delta R.T.: 0.000 min
Response: 622875
Conc: 18.79 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0203S2

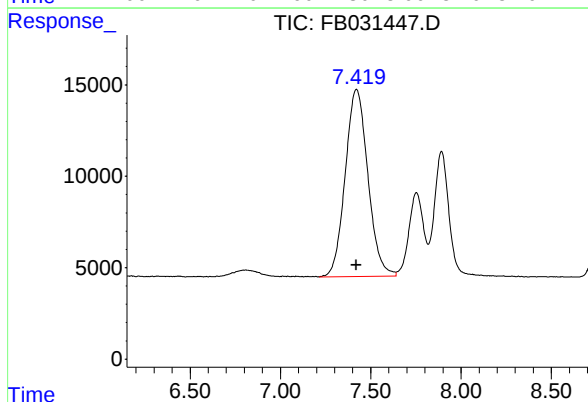


#2 2,2,4-Trimethylpentane

R.T.: 7.421 min
Delta R.T.: 0.001 min
Response: 893587
Conc: 23.76 ng/ml

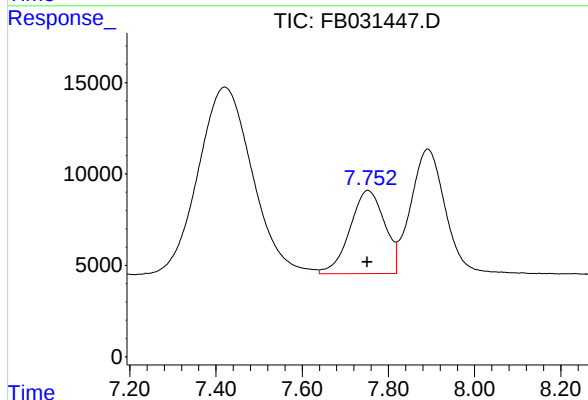


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: 0.002 min
Response: 254122
Conc: 7.04 ng/ml

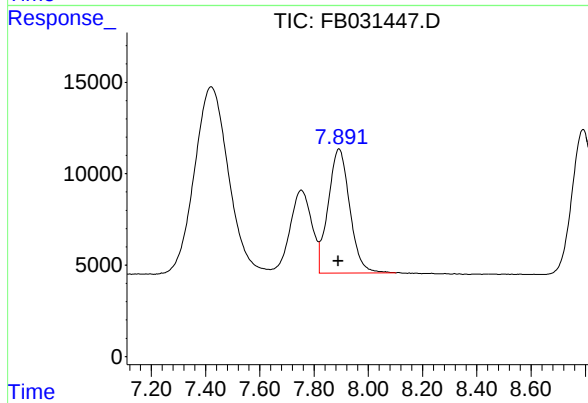

#4 Benzene


R.T.: 7.892 min
Delta R.T.: 0.002 min
Response: 375513
Conc: 8.82 ng/ml

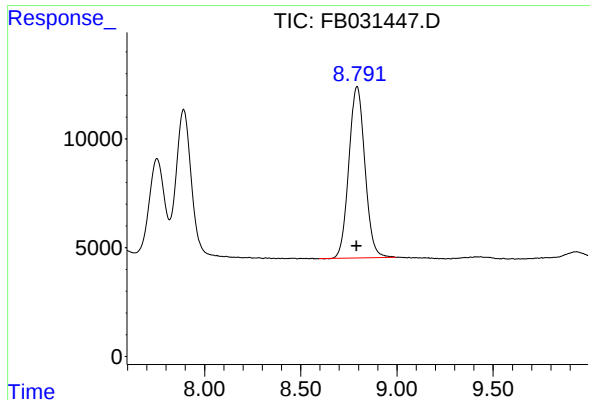

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: 0.003 min
Response: 452091
Conc: 18.95 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0203S2

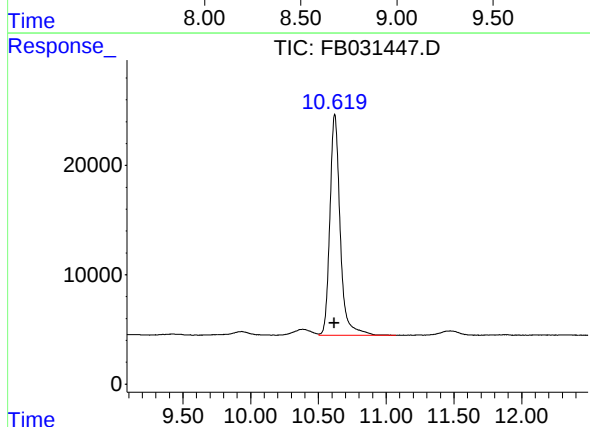


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.003 min
Response: 1068978
Conc: 27.38 ng/ml

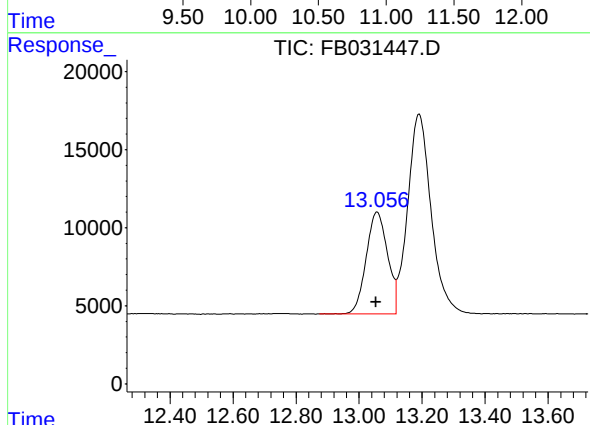


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: 0.003 min
Response: 306856
Conc: 8.86 ng/ml

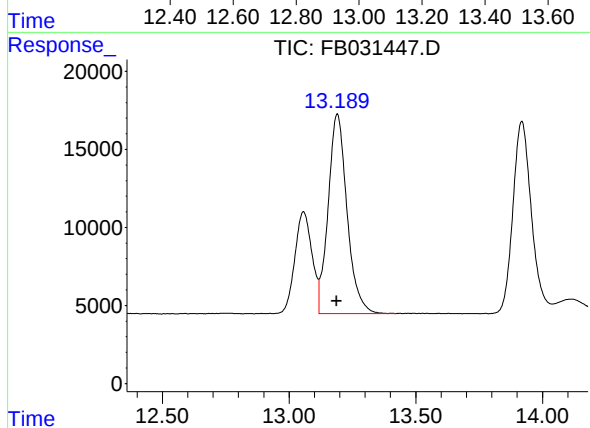

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: 0.003 min
Response: 663787
Conc: 17.76 ng/ml

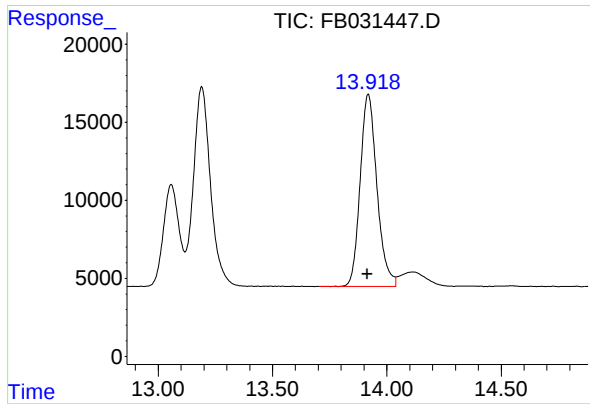

#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: 0.003 min
Response: 627752
Conc: 17.63 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0203S2

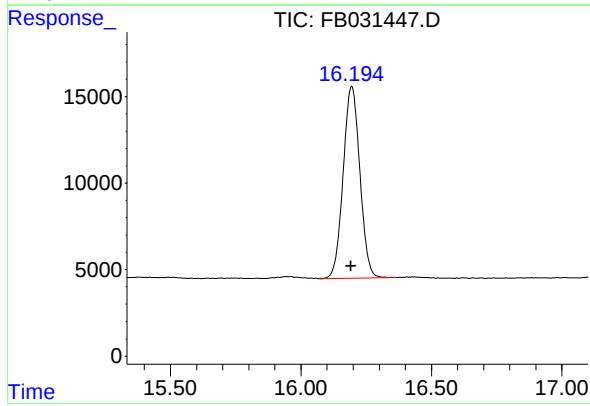

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min
Delta R.T.: 0.003 min
Response: 493135
Conc: 17.41 ng/ml