

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020420\
 Data File : FB023612.D
 Signal(s) : FID2B.CH
 Acq On : 4 Feb 2020 9:18
 Operator : DD/AJ
 Sample : BSF0204S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 04 14:41:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
 Quant Title :
 QLast Update : Thu Jan 16 11:42:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	489294	20.599 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	853279	27.002 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	954868	28.123 ng/ml
3) t n-Heptane	7.755	304062	9.080 ng/ml
4) t Benzene	7.890	398324	9.754 ng/ml
6) t Toluene	10.628	1150436	29.111 ng/ml
7) t Ethylbenzene	13.069	355307	9.513 ng/ml
8) t m-Xylene	13.202	680130	19.126 ng/ml
9) t O-Xylene	13.930	663184	19.193 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	572303	19.572 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020420\
Data File : FB023612.D
Signal(s) : FID2B.CH
Acq On : 4 Feb 2020 9:18
Operator : DD/AJ
Sample : BSF0204S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 04 14:41:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
Quant Title :
QLast Update : Thu Jan 16 11:42:55 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

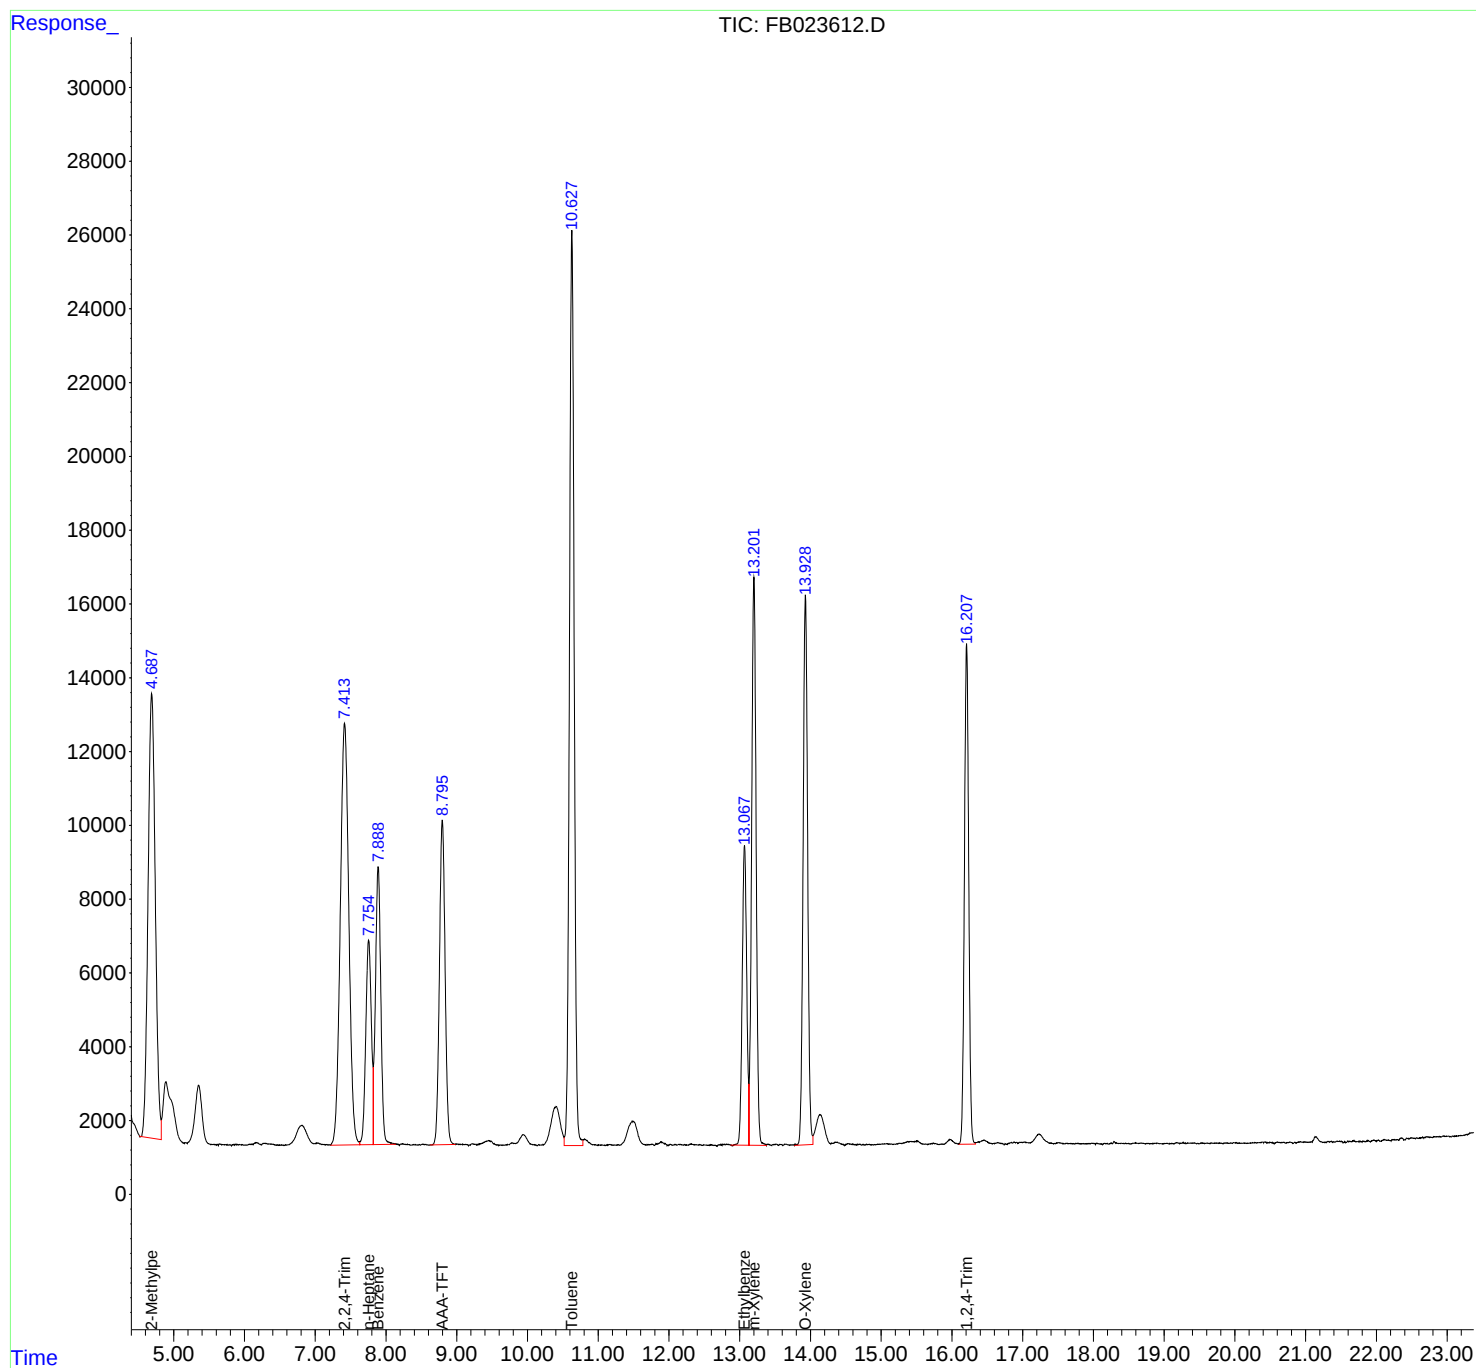

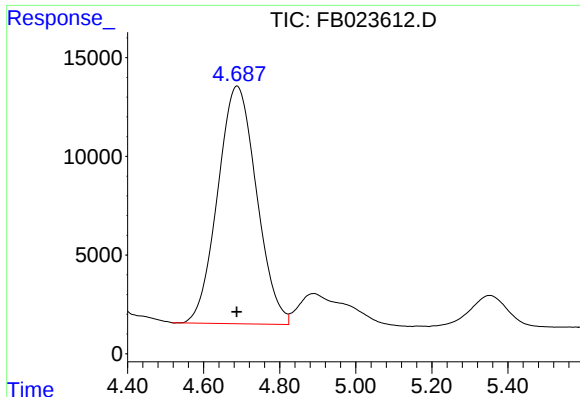


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: 0.001 min
Response: 853279
Conc: 27.00 ng/ml

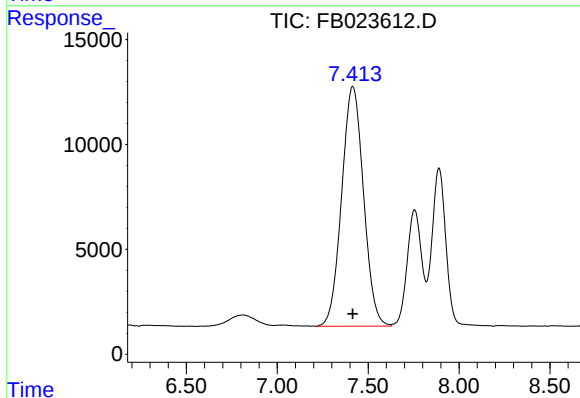


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: 0.000 min
Response: 954868
Conc: 28.12 ng/ml

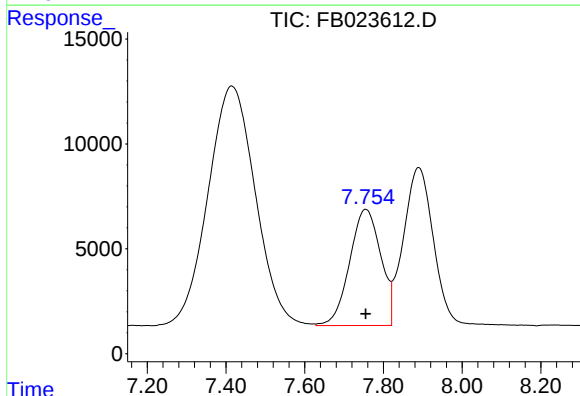


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.000 min
Response: 304062
Conc: 9.08 ng/ml

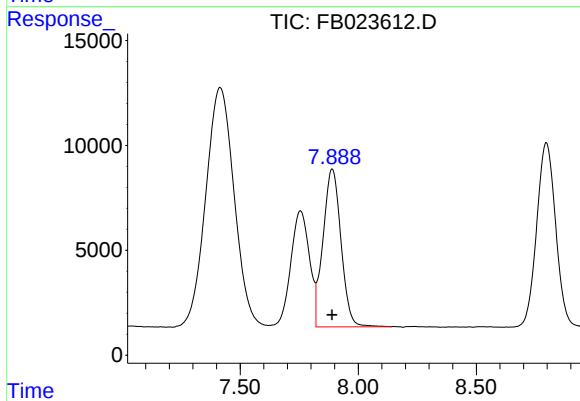


#4 Benzene

R.T.: 7.890 min
Delta R.T.: 0.000 min
Response: 398324
Conc: 9.75 ng/ml

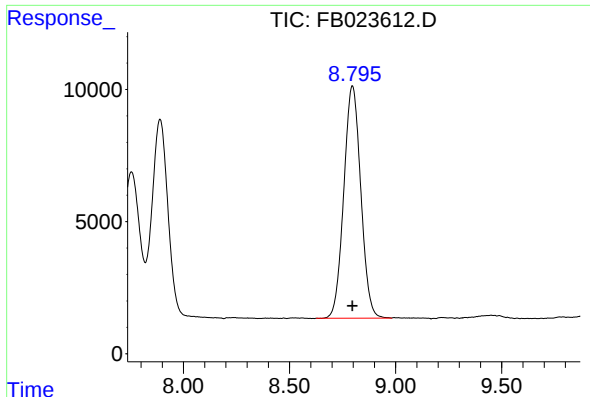


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: 0.000 min
Response: 489294
Conc: 20.60 ng/ml

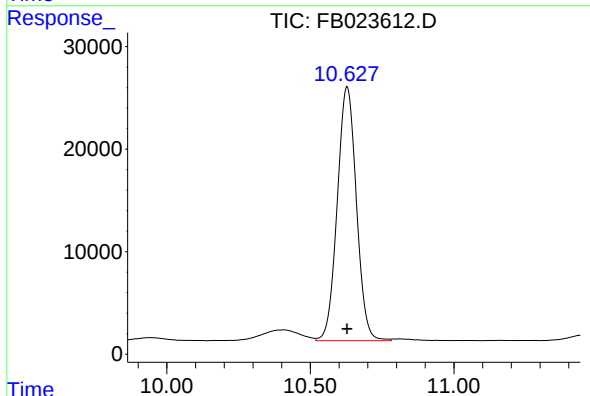


#6 Toluene

R.T.: 10.628 min
Delta R.T.: 0.000 min
Response: 1150436
Conc: 29.11 ng/ml

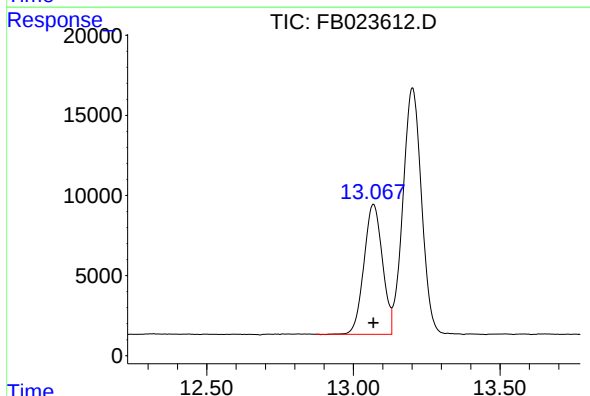


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: 0.000 min
Response: 355307
Conc: 9.51 ng/ml

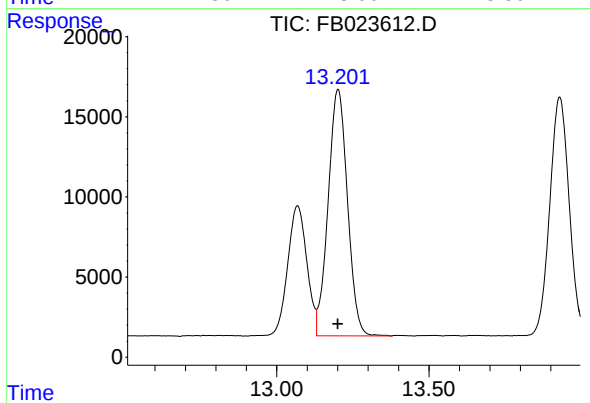


#8 m-Xylene

R.T.: 13.202 min
Delta R.T.: 0.001 min
Response: 680130
Conc: 19.13 ng/ml

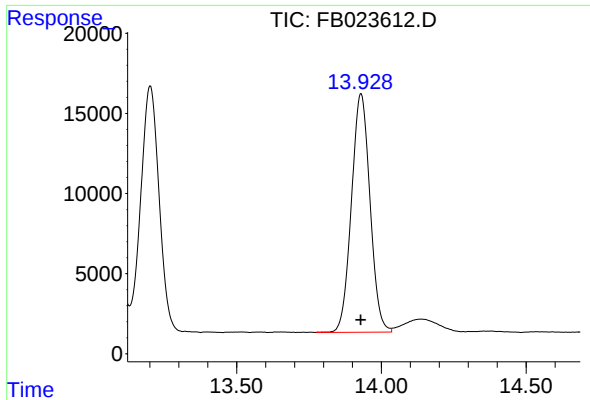

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: 0.000 min
Response: 663184
Conc: 19.19 ng/ml

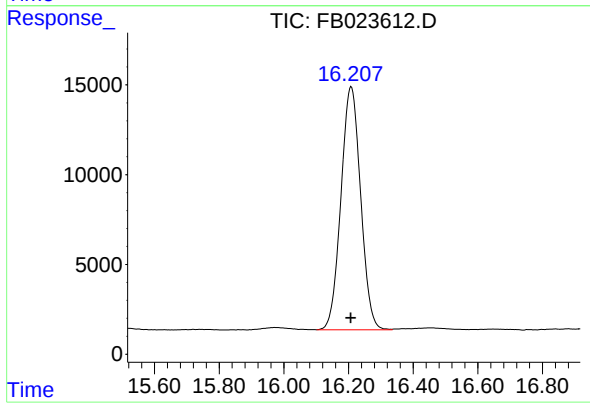

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: 0.001 min
Response: 572303
Conc: 19.57 ng/ml