

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020420\
 Data File : FB023623.D
 Signal(s) : FID2B.CH
 Acq On : 4 Feb 2020 15:30
 Operator : DD/AJ
 Sample : L1383-06MSD
 Misc : 5.05g/5.00ml DI WATER
 ALS Vial : 14 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 05 00:19:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
 Quant Title :
 QLast Update : Thu Jan 16 11:42:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	465533	19.598 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	704173	22.283 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	786294	23.158 ng/ml
3) t n-Heptane	7.759	248235	7.413 ng/ml
4) t Benzene	7.893	357905	8.764 ng/ml
6) t Toluene	10.631	1046296	26.476 ng/ml
7) t Ethylbenzene	13.072	322926	8.646 ng/ml
8) t m-Xylene	13.204	617226	17.357 ng/ml
9) t O-Xylene	13.932	614282	17.778 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	541054	18.503 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020420\
Data File : FB023623.D
Signal(s) : FID2B.CH
Acq On : 4 Feb 2020 15:30
Operator : DD/AJ
Sample : L1383-06MSD
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 14 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 05 00:19:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
Quant Title :
QLast Update : Thu Jan 16 11:42:55 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

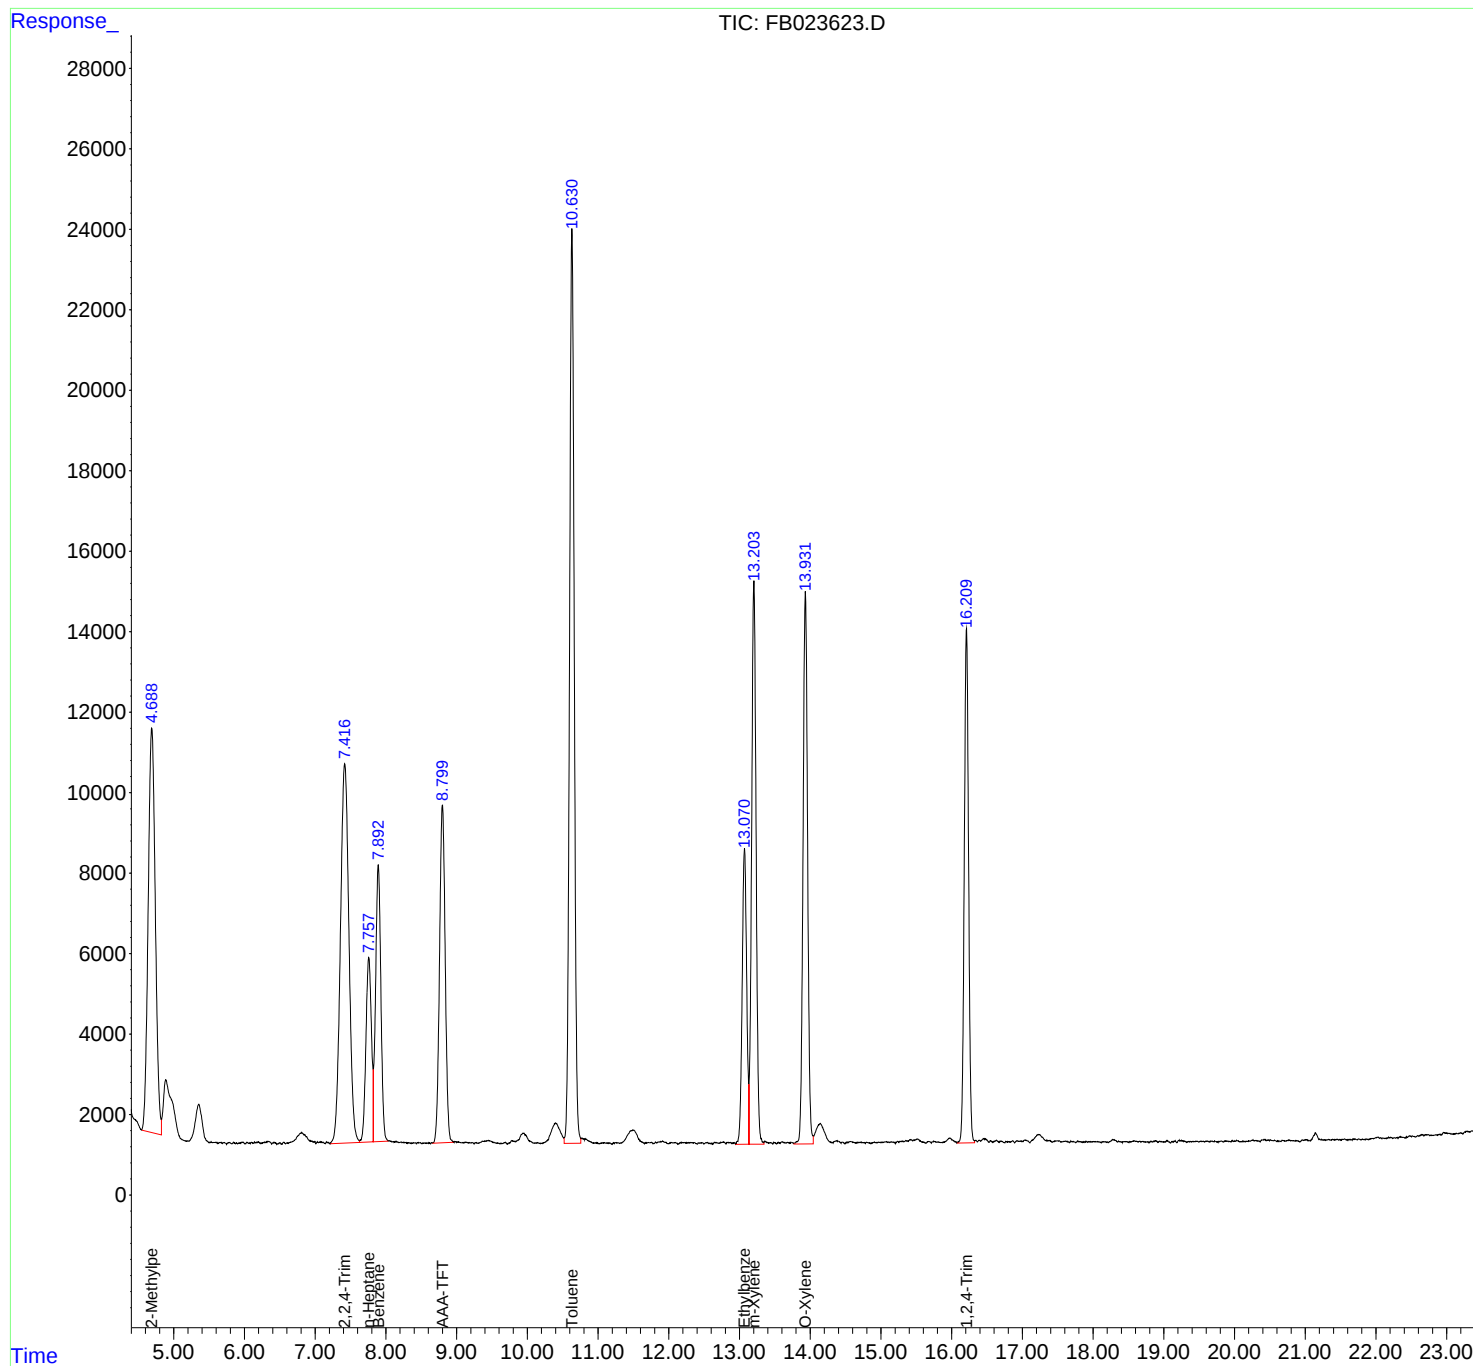

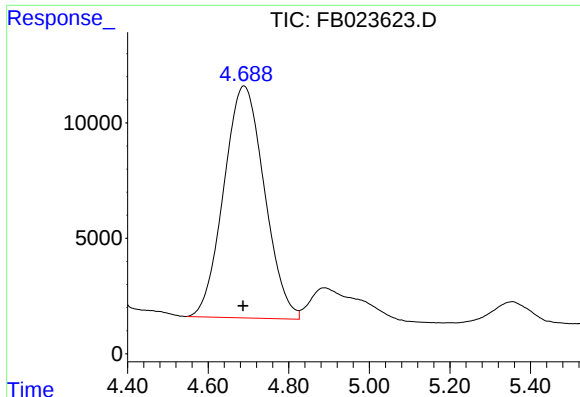


#1 2-Methylpentane

R.T.: 4.689 min
Delta R.T.: 0.002 min
Response: 704173
Conc: 22.28 ng/ml

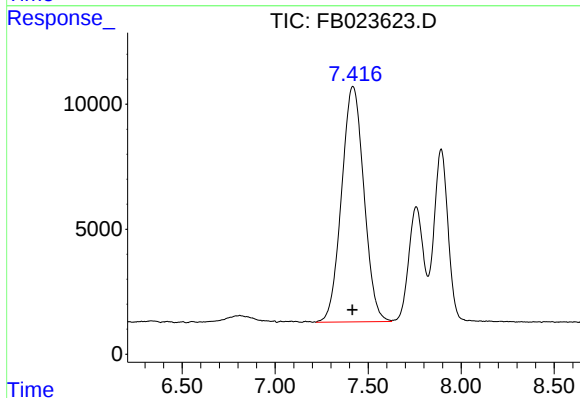


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.002 min
Response: 786294
Conc: 23.16 ng/ml

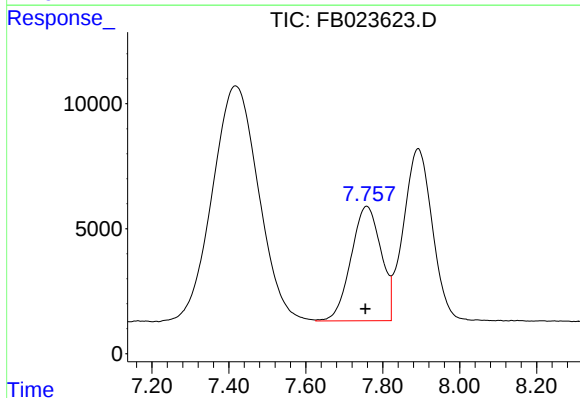


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.003 min
Response: 248235
Conc: 7.41 ng/ml

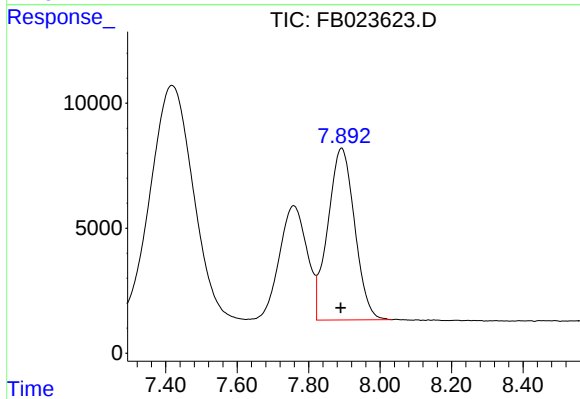


#4 Benzene

R.T.: 7.893 min
Delta R.T.: 0.003 min
Response: 357905
Conc: 8.76 ng/ml

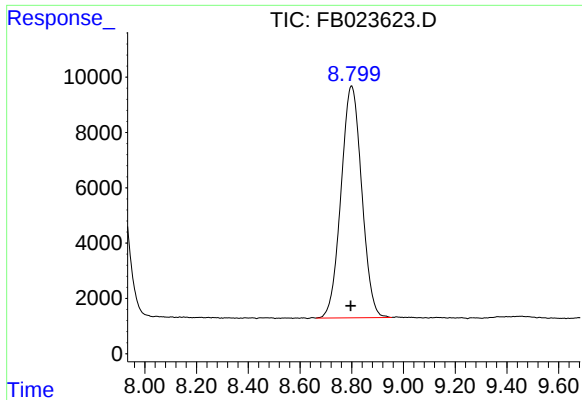


#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: 0.003 min
Response: 465533
Conc: 19.60 ng/ml

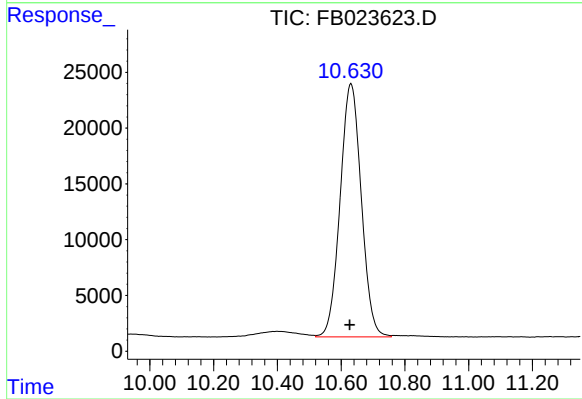


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.004 min
Response: 1046296
Conc: 26.48 ng/ml

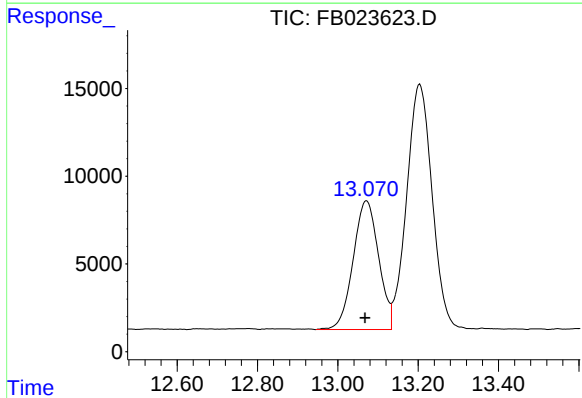


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.004 min
Response: 322926
Conc: 8.65 ng/ml

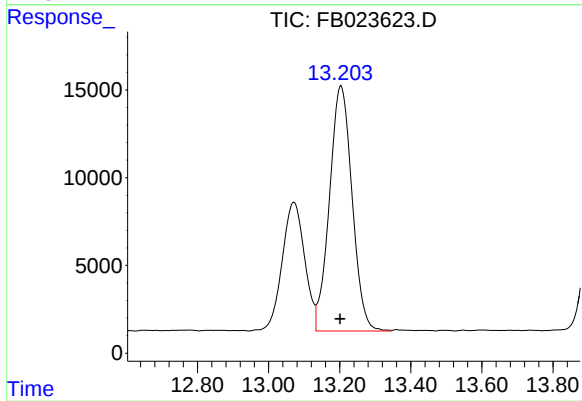

#8 m-Xylene

R.T.: 13.204 min
Delta R.T.: 0.003 min
Response: 617226
Conc: 17.36 ng/ml

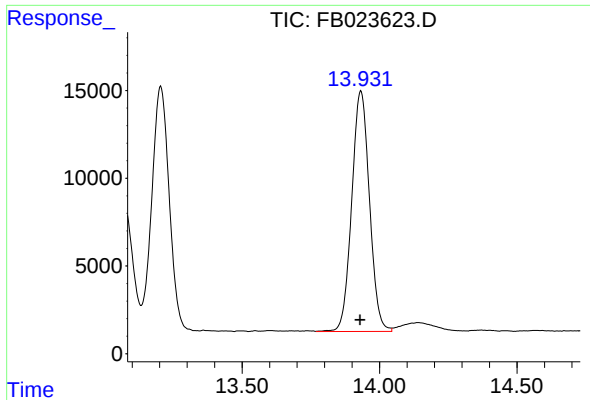


#9 O-Xylene

R.T.: 13.932 min

Delta R.T.: 0.003 min

Response: 614282

Conc: 17.78 ng/ml

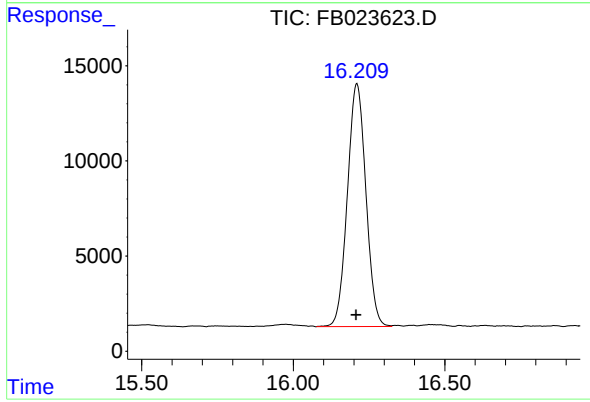

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min

Delta R.T.: 0.003 min

Response: 541054

Conc: 18.50 ng/ml