

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020519\
Data File : FB019618.D
Signal(s) : FID2B.CH
Acq On : 5 Feb 2019 9:10
Operator : MJ/SJ
Sample : BSF0205S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 06 03:59:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
Quant Title :
QLast Update : Tue Jan 29 12:07:12 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.043	221038	18.909 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.897	591855	34.185 ng/ml
2) t	2,2,4-Trimethylpentane	7.657	569926	34.367 ng/ml
3) t	n-Heptane	7.998	176539	10.955 ng/ml
4) t	Benzene	8.135	201075	10.661 ng/ml
6) t	Toluene	10.890	518346	29.633 ng/ml
7) t	Ethylbenzene	13.341	211196	9.624 ng/ml
8) t	m-Xylene	13.475	440290	19.237 ng/ml
9) t	O-Xylene	14.206	434253	19.443 ng/ml
10) t	1,2,4-Trimethylbenzene	16.493	439399	18.964 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020519\
Data File : FB019618.D
Signal(s) : FID2B.CH
Acq On : 5 Feb 2019 9:10
Operator : MJ/SJ
Sample : BSF0205S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 06 03:59:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
Quant Title :
QLast Update : Tue Jan 29 12:07:12 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

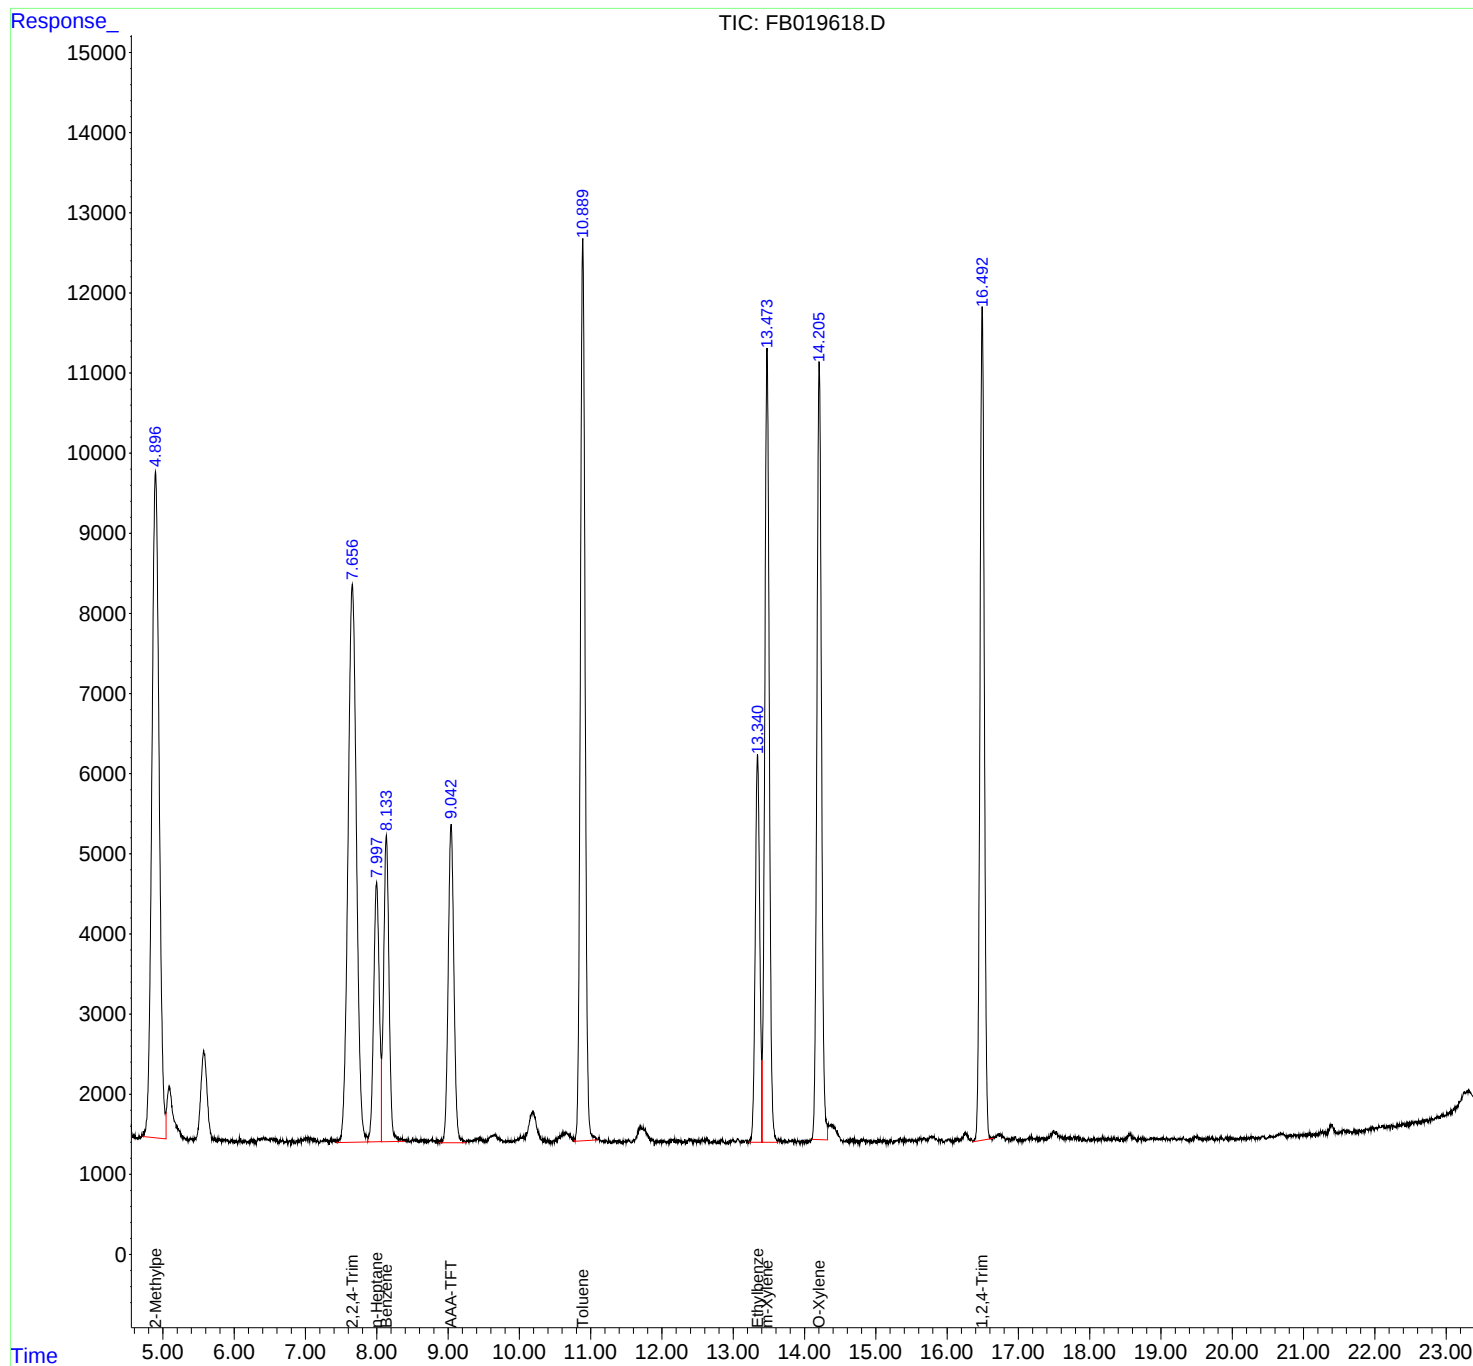

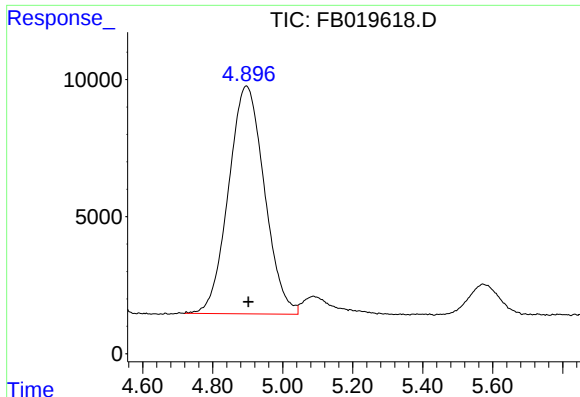


#1 2-Methylpentane

R.T.: 4.897 min
Delta R.T.: -0.005 min
Response: 591855
Conc: 34.19 ng/ml

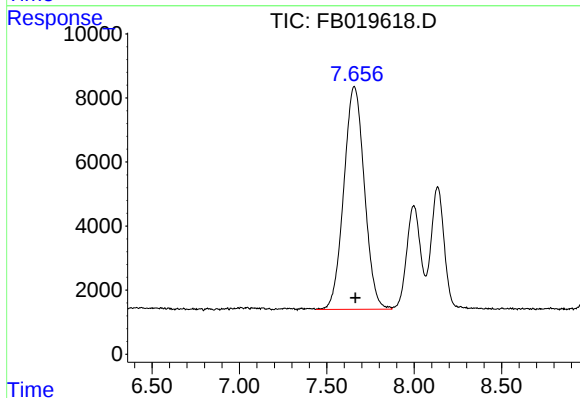


#2 2,2,4-Trimethylpentane

R.T.: 7.657 min
Delta R.T.: -0.007 min
Response: 569926
Conc: 34.37 ng/ml

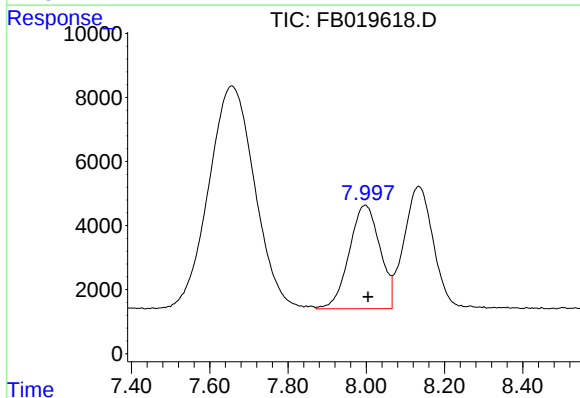


#3 n-Heptane

R.T.: 7.998 min
Delta R.T.: -0.007 min
Response: 176539
Conc: 10.96 ng/ml

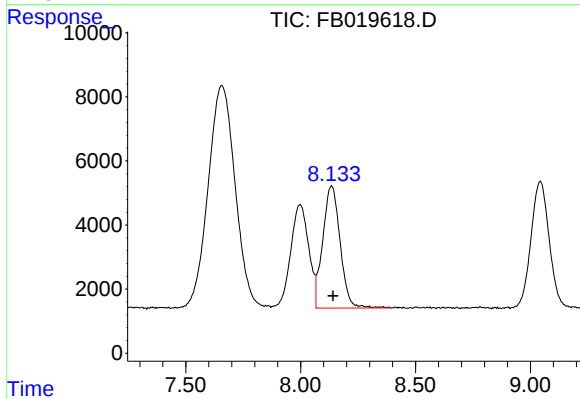


#4 Benzene

R.T.: 8.135 min
Delta R.T.: -0.007 min
Response: 201075
Conc: 10.66 ng/ml

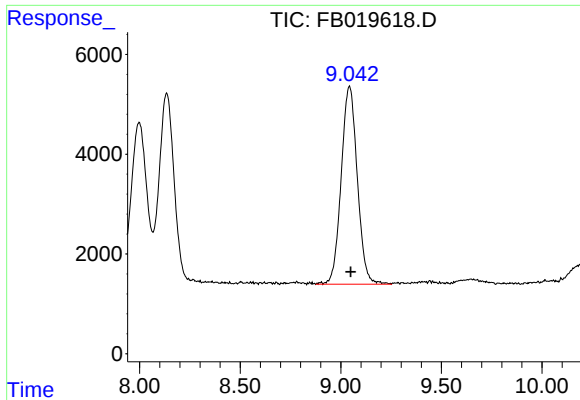


#5 AAA-TFT

R.T.: 9.043 min
Delta R.T.: -0.006 min
Response: 221038
Conc: 18.91 ng/ml

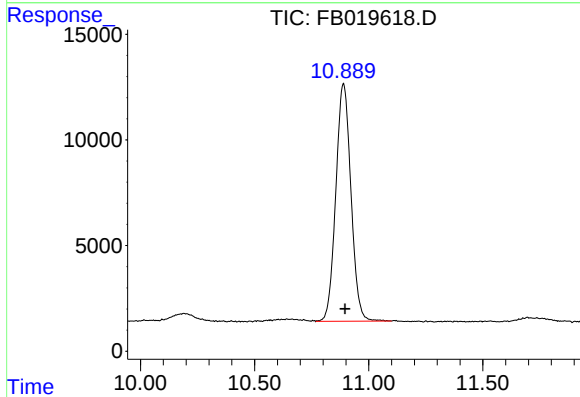


#6 Toluene

R.T.: 10.890 min
Delta R.T.: -0.007 min
Response: 518346
Conc: 29.63 ng/ml

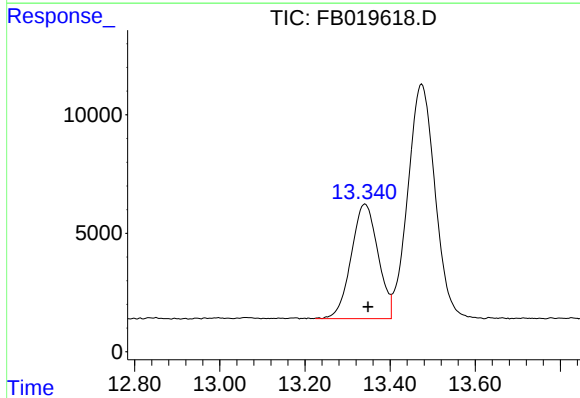


#7 Ethylbenzene

R.T.: 13.341 min
Delta R.T.: -0.007 min
Response: 211196
Conc: 9.62 ng/ml

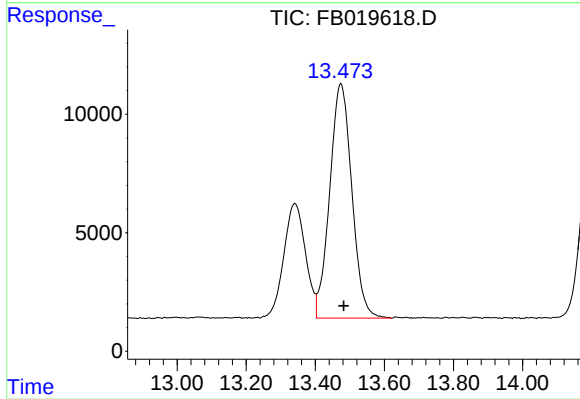


#8 m-Xylene

R.T.: 13.475 min
Delta R.T.: -0.007 min
Response: 440290
Conc: 19.24 ng/ml

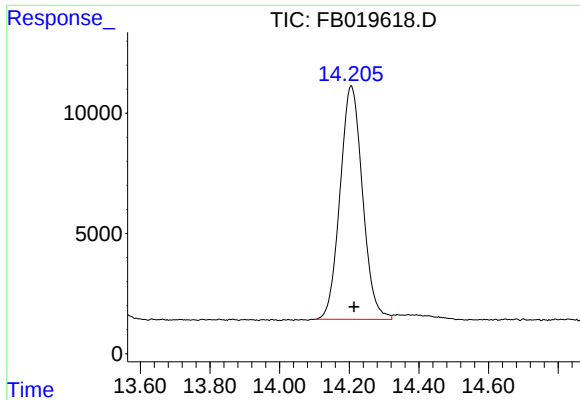

#9 O-Xylene

R.T.: 14.206 min
Delta R.T.: -0.008 min
Response: 434253
Conc: 19.44 ng/ml

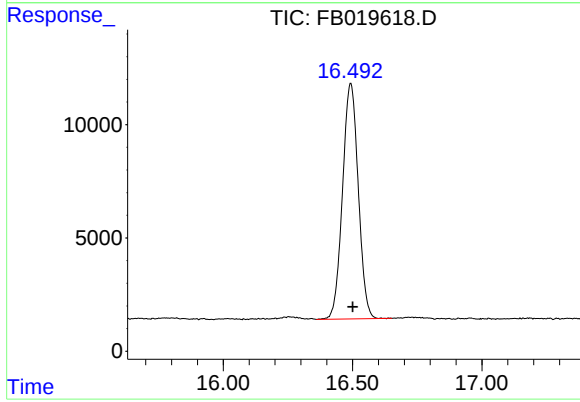

#10 1,2,4-Trimethylbenzene

R.T.: 16.493 min
Delta R.T.: -0.007 min
Response: 439399
Conc: 18.96 ng/ml