

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020619\
 Data File : FB019632.D
 Signal(s) : FID2B.CH
 Acq On : 6 Feb 2019 9:42
 Operator : MJ/SJ
 Sample : BSF0206S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 07 00:39:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
 Quant Title :
 QLast Update : Tue Jan 29 12:07:12 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.042	204993	17.536 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.896	602040	34.774 ng/ml
2) t	2,2,4-Trimethylpentane	7.655	579540	34.947 ng/ml
3) t	n-Heptane	7.995	180036	11.172 ng/ml
4) t	Benzene	8.133	197535	10.473 ng/ml
6) t	Toluene	10.888	521886	29.835 ng/ml
7) t	Ethylbenzene	13.339	211331	9.630 ng/ml
8) t	m-Xylene	13.473	441492	19.290 ng/ml
9) t	O-Xylene	14.205	425261	19.040 ng/ml
10) t	1,2,4-Trimethylbenzene	16.491	434871	18.769 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020619\
Data File : FB019632.D
Signal(s) : FID2B.CH
Acq On : 6 Feb 2019 9:42
Operator : MJ/SJ
Sample : BSF0206S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 07 00:39:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
Quant Title :
QLast Update : Tue Jan 29 12:07:12 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

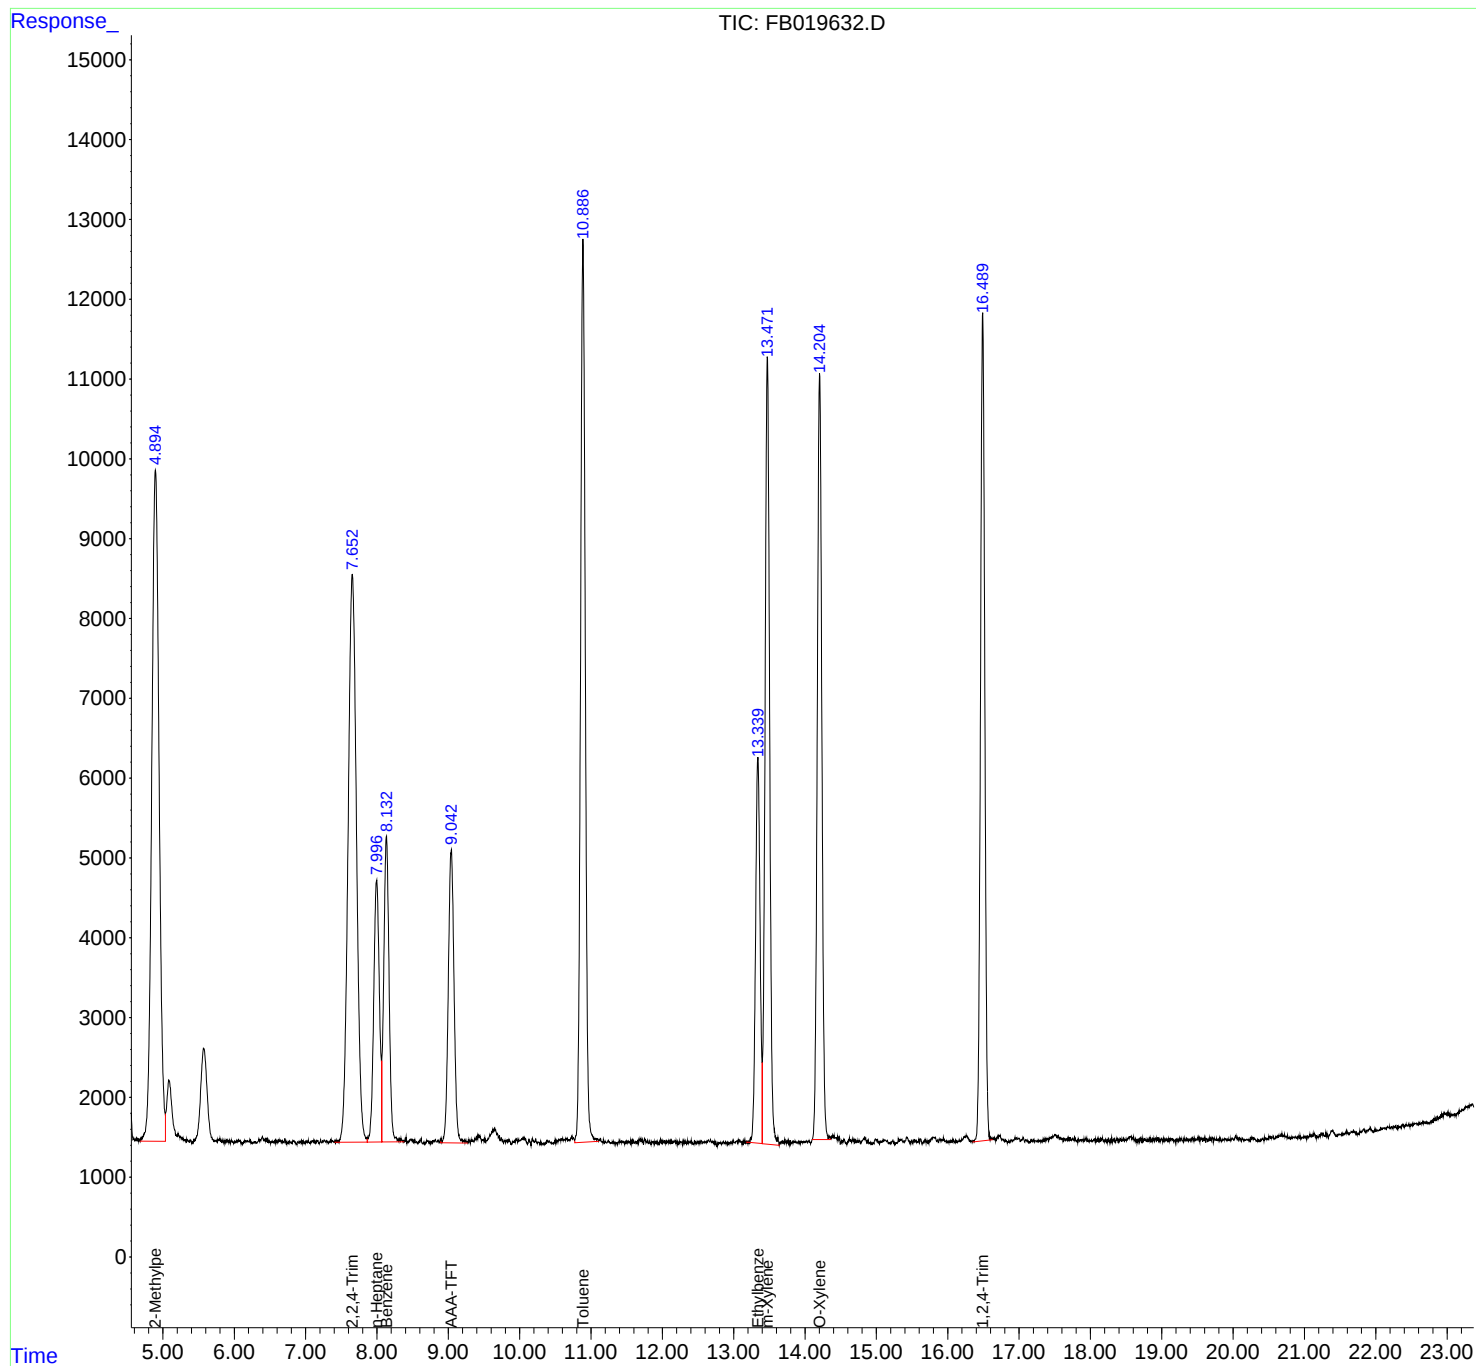

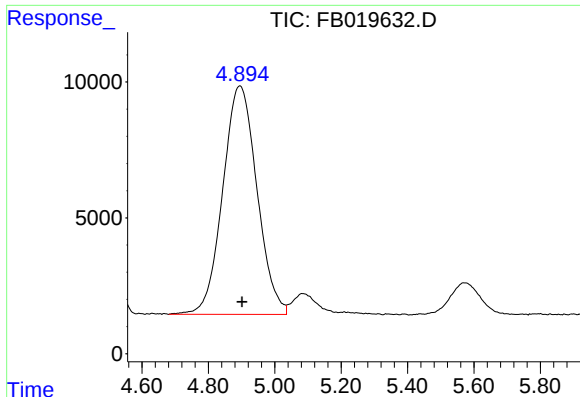


#1 2-Methylpentane

R.T.: 4.896 min
Delta R.T.: -0.006 min
Response: 602040
Conc: 34.77 ng/ml

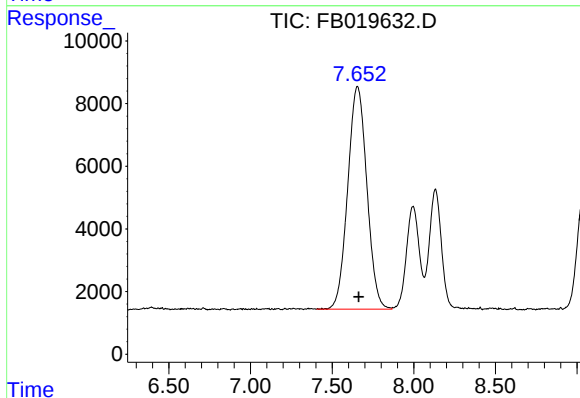


#2 2,2,4-Trimethylpentane

R.T.: 7.655 min
Delta R.T.: -0.010 min
Response: 579540
Conc: 34.95 ng/ml

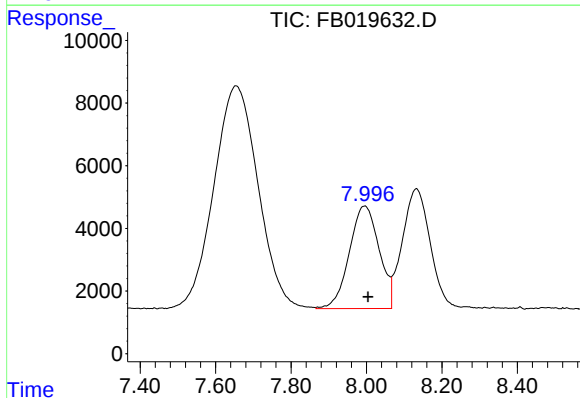


#3 n-Heptane

R.T.: 7.995 min
Delta R.T.: -0.009 min
Response: 180036
Conc: 11.17 ng/ml

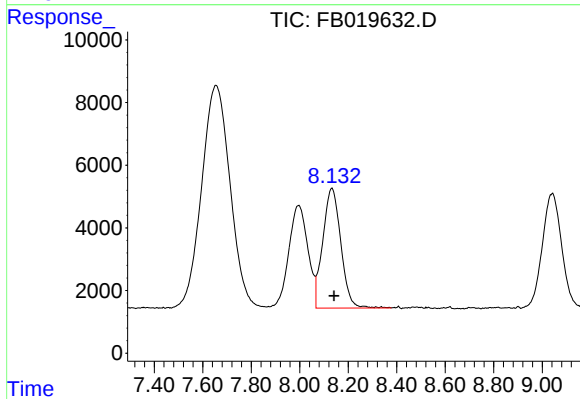


#4 Benzene

R.T.: 8.133 min
Delta R.T.: -0.008 min
Response: 197535
Conc: 10.47 ng/ml

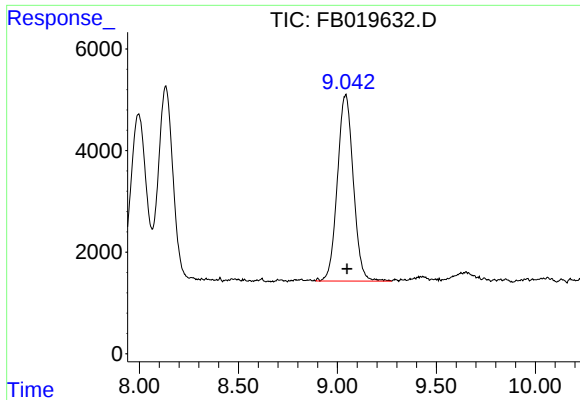


#5 AAA-TFT

R.T.: 9.042 min
Delta R.T.: -0.008 min
Response: 204993
Conc: 17.54 ng/ml

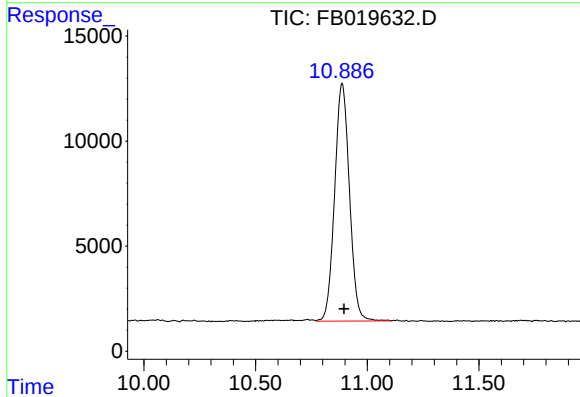


#6 Toluene

R.T.: 10.888 min
Delta R.T.: -0.009 min
Response: 521886
Conc: 29.83 ng/ml

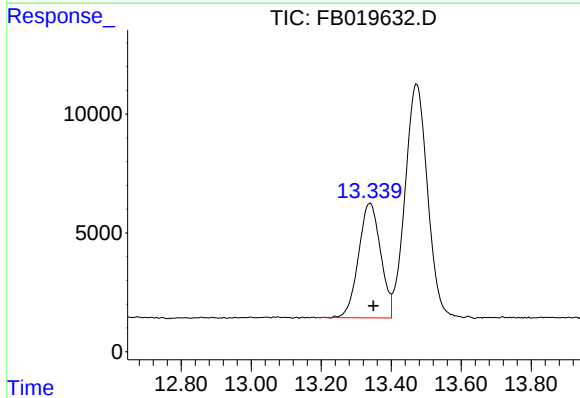


#7 Ethylbenzene

R.T.: 13.339 min
Delta R.T.: -0.009 min
Response: 211331
Conc: 9.63 ng/ml

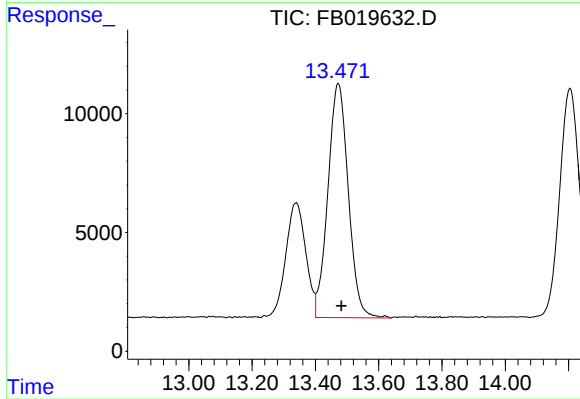

#8 m-Xylene

R.T.: 13.473 min
Delta R.T.: -0.009 min
Response: 441492
Conc: 19.29 ng/ml

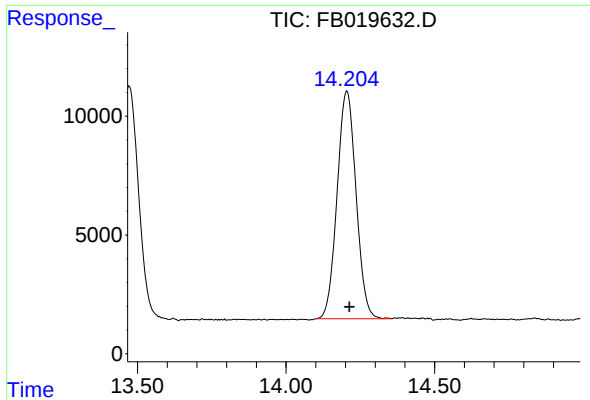


#9 O-Xylene

R.T.: 14.205 min

Delta R.T.: -0.009 min

Response: 425261

Conc: 19.04 ng/ml

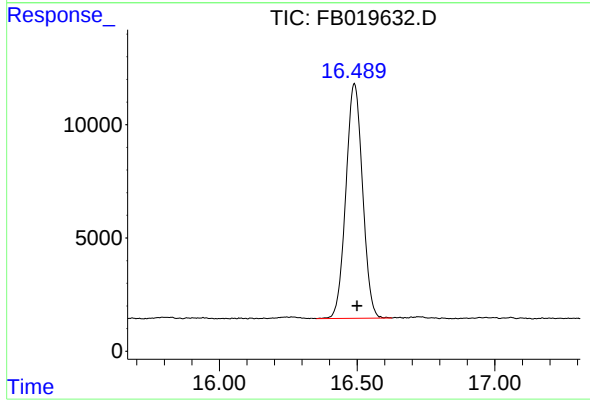

#10 1,2,4-Trimethylbenzene

R.T.: 16.491 min

Delta R.T.: -0.009 min

Response: 434871

Conc: 18.77 ng/ml