

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020620\
 Data File : FB023634.D
 Signal(s) : FID2B.CH
 Acq On : 6 Feb 2020 11:17
 Operator : DD/AJ
 Sample : FB020620GROICV
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 FB020620GROICV

Integration File: Calibration.e
 Quant Time: Feb 07 03:18:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
 Quant Title :
 QLast Update : Thu Feb 06 11:13:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	385365	18.928 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	922404	30.655 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	960337	29.430 ng/ml
3) t n-Heptane	7.757	319220	9.922 ng/ml
4) t Benzene	7.890	423366	10.351 ng/ml
6) t Toluene	10.629	1227097	30.913 ng/ml
7) t Ethylbenzene	13.069	364095	9.794 ng/ml
8) t m-Xylene	13.203	705919	19.767 ng/ml
9) t O-Xylene	13.931	685571	19.878 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	592231	20.228 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020620\
Data File : FB023634.D
Signal(s) : FID2B.CH
Acq On : 6 Feb 2020 11:17
Operator : DD/AJ
Sample : FB020620GROICV
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
FB020620GROICV

Integration File: Calibration.e
Quant Time: Feb 07 03:18:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
Quant Title :
QLast Update : Thu Feb 06 11:13:47 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

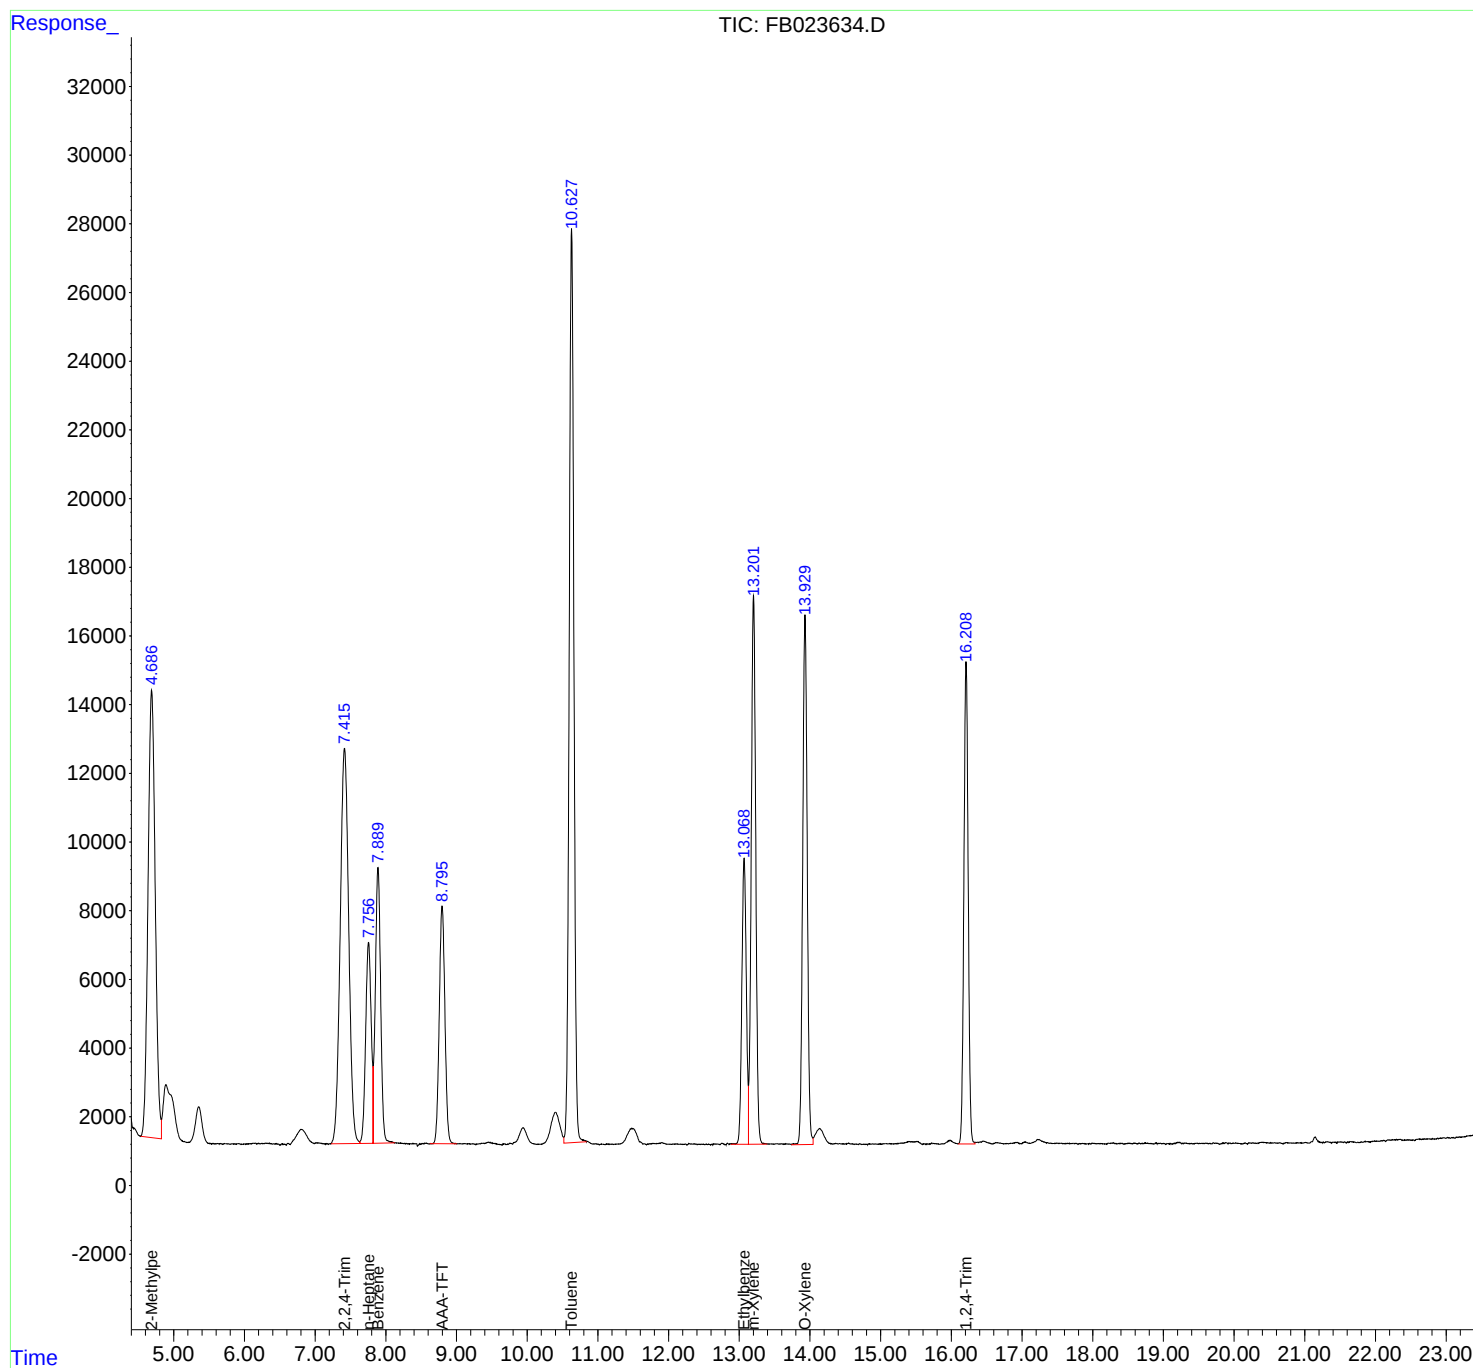


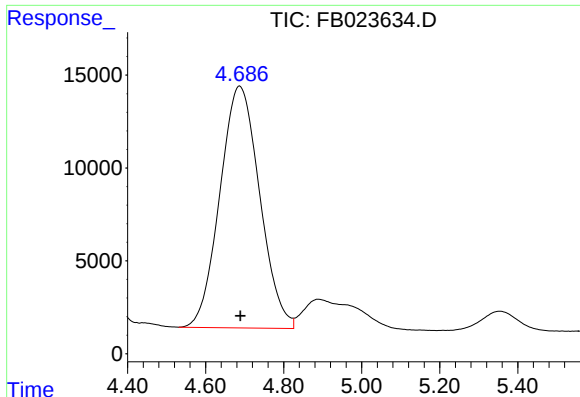

#1 2-Methylpentane


R.T.: 4.687 min
Delta R.T.: -0.002 min
Response: 922404
Conc: 30.65 ng/ml

Instrument :
FID_B
ClientSampleId :
FB020620GROICV

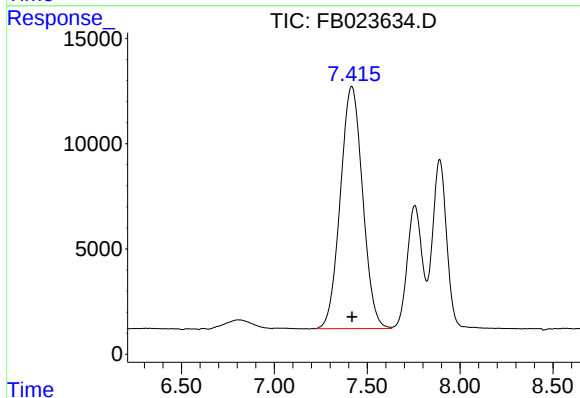


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: -0.001 min
Response: 960337
Conc: 29.43 ng/ml

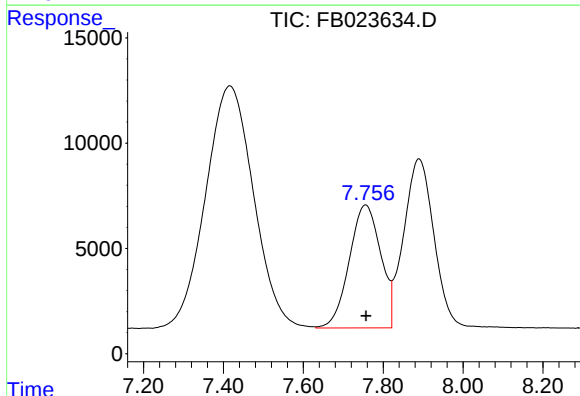


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.000 min
Response: 319220
Conc: 9.92 ng/ml

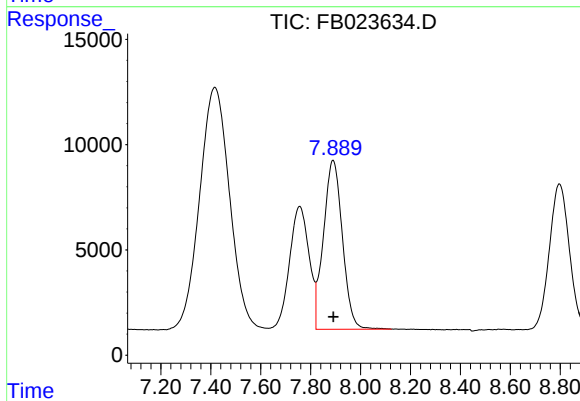

#4 Benzene


R.T.: 7.890 min
Delta R.T.: -0.001 min
Response: 423366
Conc: 10.35 ng/ml

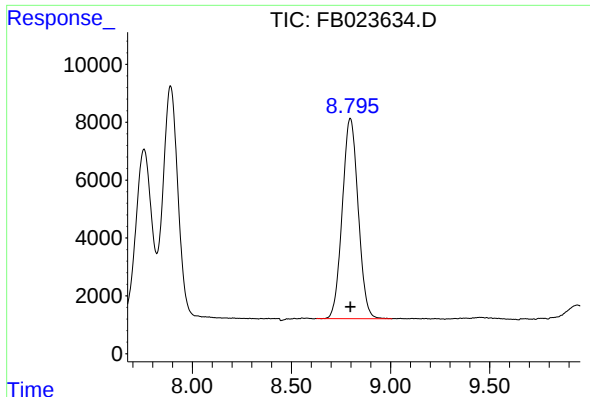

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: -0.001 min
Response: 385365
Conc: 18.93 ng/ml

Instrument :
FID_B
ClientSampleId :
FB020620GROICV

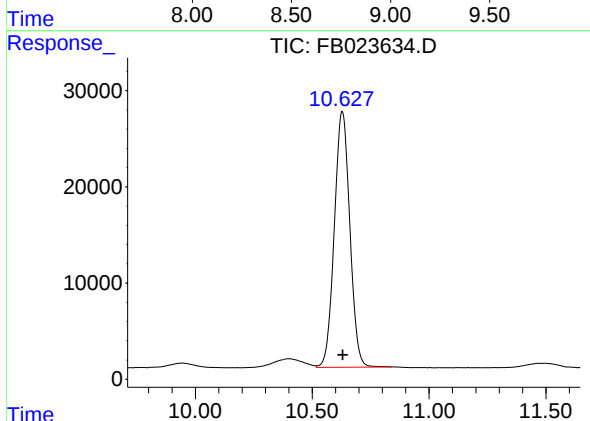


#6 Toluene

R.T.: 10.629 min
Delta R.T.: -0.001 min
Response: 1227097
Conc: 30.91 ng/ml

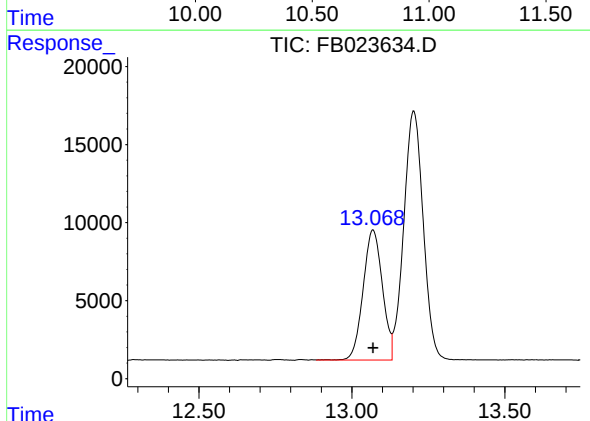


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: 0.000 min
Response: 364095
Conc: 9.79 ng/ml

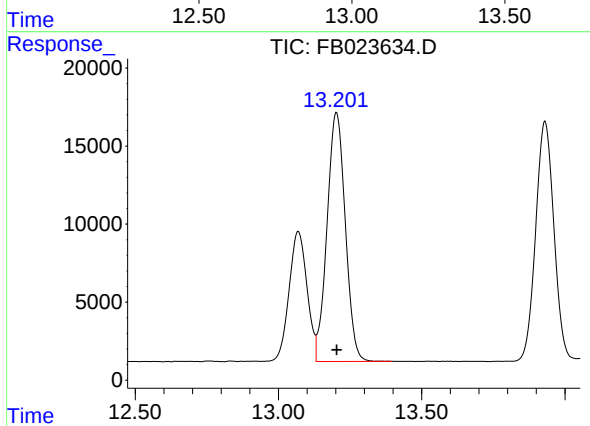

#8 m-Xylene


R.T.: 13.203 min
Delta R.T.: 0.000 min
Response: 705919
Conc: 19.77 ng/ml

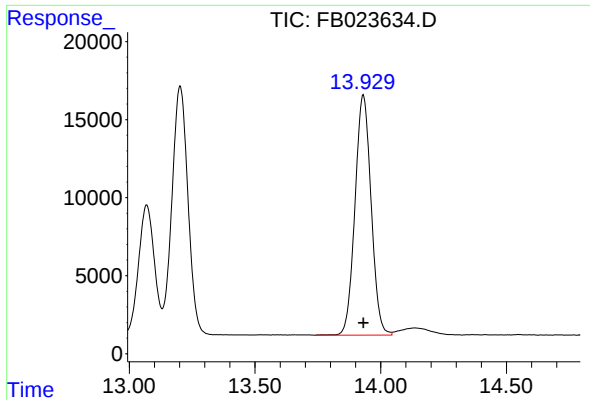

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.000 min
Response: 685571
Conc: 19.88 ng/ml

Instrument :
FID_B
ClientSampleId :
FB020620GROICV

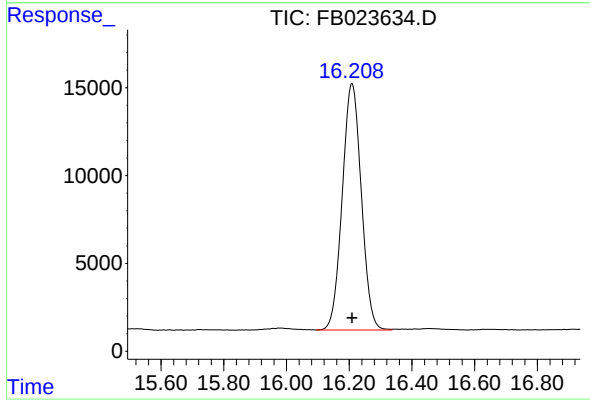

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.000 min
Response: 592231
Conc: 20.23 ng/ml