

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020620\
 Data File : FB023643.D
 Signal(s) : FID2B.CH
 Acq On : 6 Feb 2020 16:19
 Operator : DD/AJ
 Sample : L1365-02MS
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 CL-01-020520MS

Integration File: Calibration.e
 Quant Time: Feb 07 03:19:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
 Quant Title :
 QLast Update : Thu Feb 06 11:13:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	370951	18.220 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.694	642449	21.351 ng/ml
2) t 2,2,4-Trimethylpentane	7.421	527950	16.179 ng/ml
3) t n-Heptane	7.761	171960	5.345 ng/ml
4) t Benzene	7.895	353876	8.652 ng/ml
6) t Toluene	10.633	1015827	25.591 ng/ml
7) t Ethylbenzene	13.073	324740	8.735 ng/ml
8) t m-Xylene	13.206	571395	16.000 ng/ml
9) t O-Xylene	13.935	557776	16.172 ng/ml
10) t 1,2,4-Trimethylbenzene	16.213	504455	17.230 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020620\
Data File : FB023643.D
Signal(s) : FID2B.CH
Acq On : 6 Feb 2020 16:19
Operator : DD/AJ
Sample : L1365-02MS
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
CL-01-020520MS

Integration File: Calibration.e
Quant Time: Feb 07 03:19:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
Quant Title :
QLast Update : Thu Feb 06 11:13:47 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

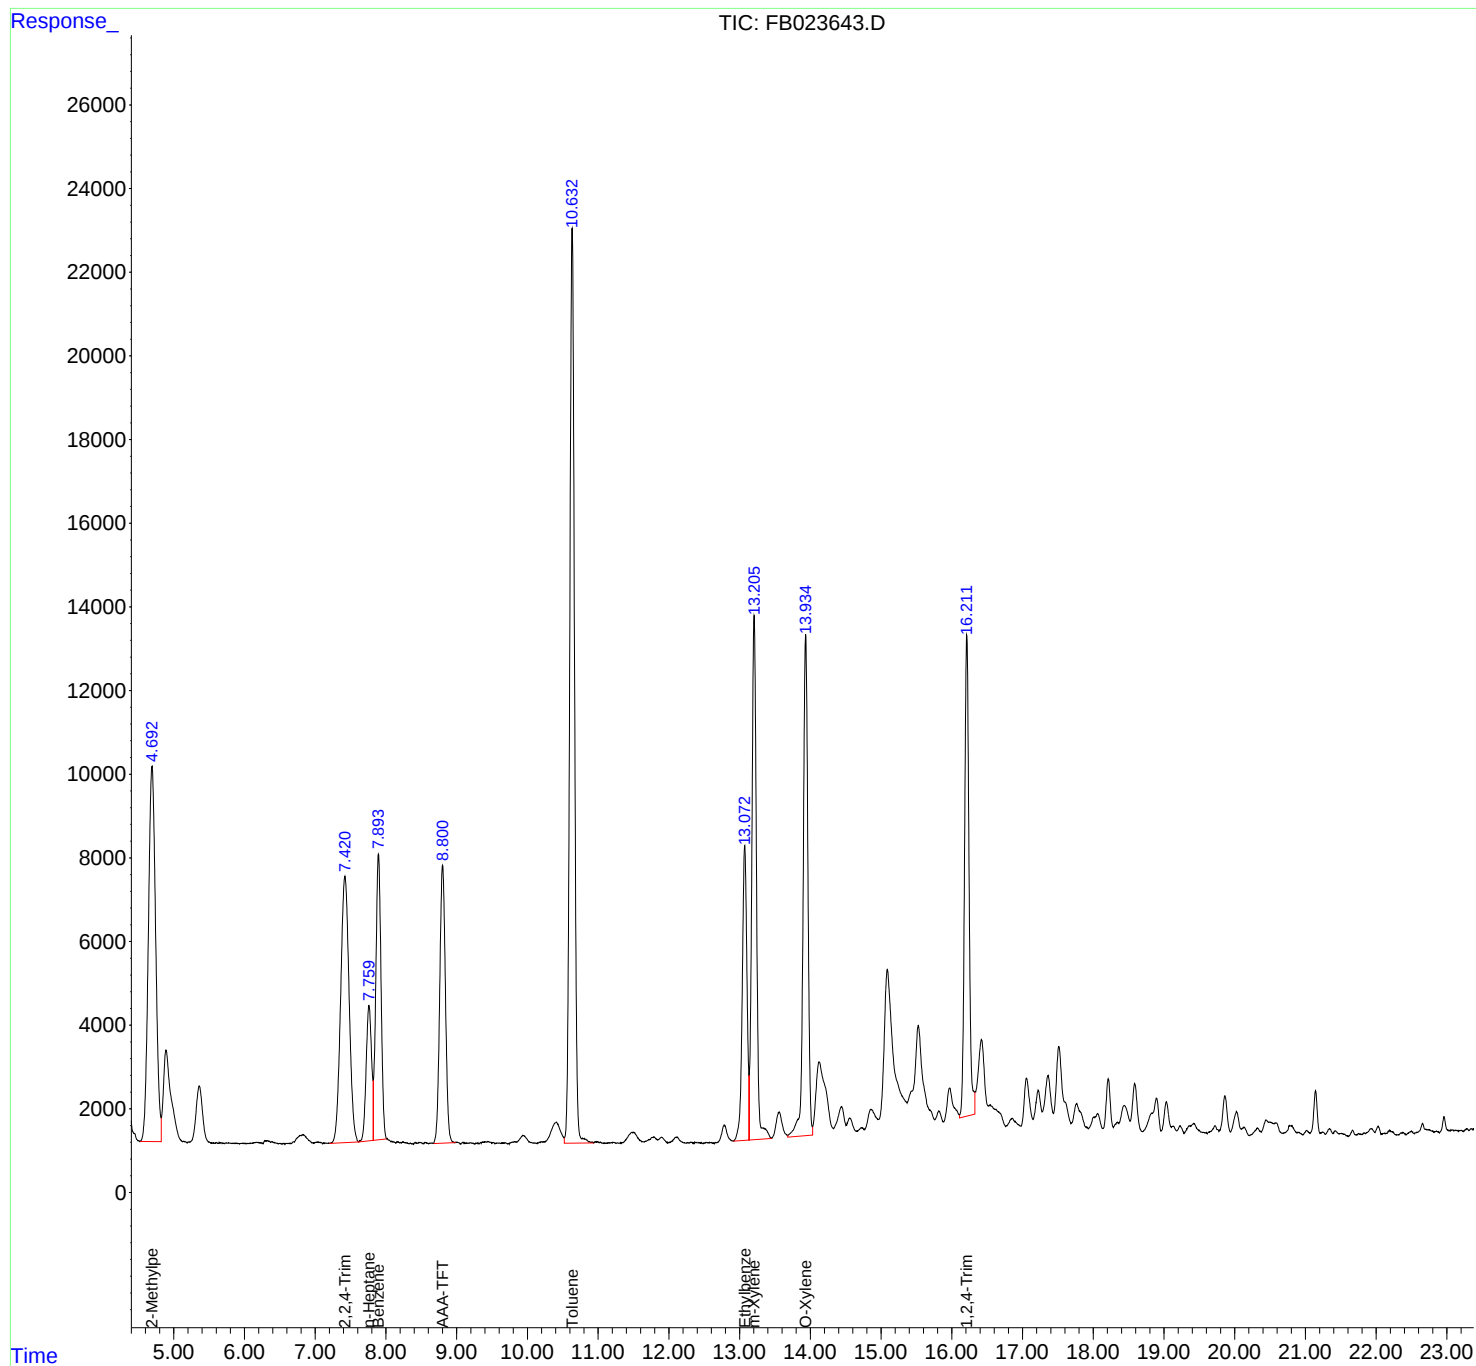


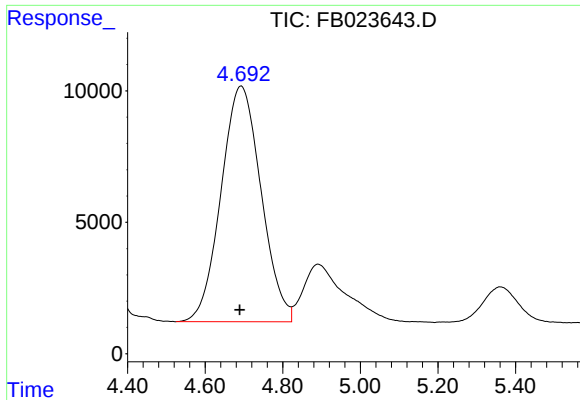

#1 2-Methylpentane


R.T.: 4.694 min
Delta R.T.: 0.005 min
Response: 642449
Conc: 21.35 ng/ml

Instrument :
FID_B
ClientSampleId :
CL-01-020520MS

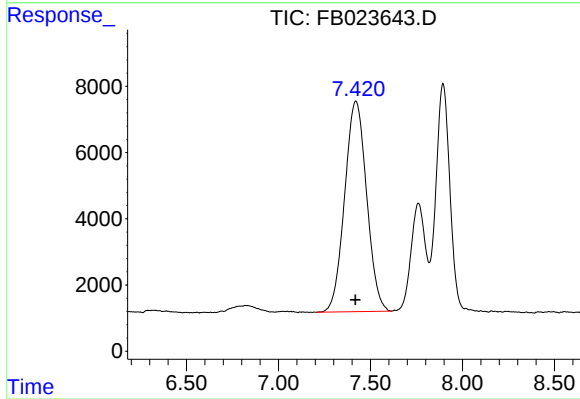


#2 2,2,4-Trimethylpentane

R.T.: 7.421 min
Delta R.T.: 0.003 min
Response: 527950
Conc: 16.18 ng/ml

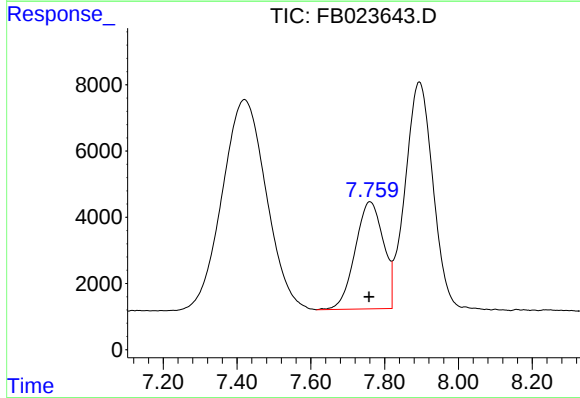


#3 n-Heptane

R.T.: 7.761 min
Delta R.T.: 0.003 min
Response: 171960
Conc: 5.34 ng/ml

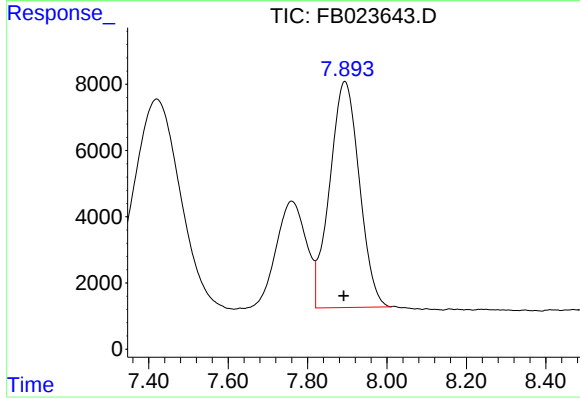

#4 Benzene


R.T.: 7.895 min
Delta R.T.: 0.003 min
Response: 353876
Conc: 8.65 ng/ml

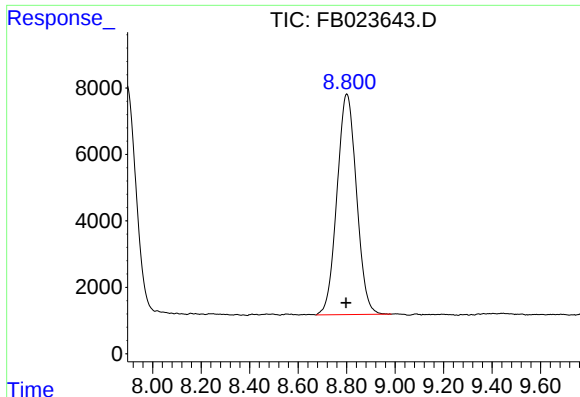

#5 AAA-TFT


R.T.: 8.801 min
Delta R.T.: 0.003 min
Response: 370951
Conc: 18.22 ng/ml

Instrument :
FID_B
ClientSampleId :
CL-01-020520MS

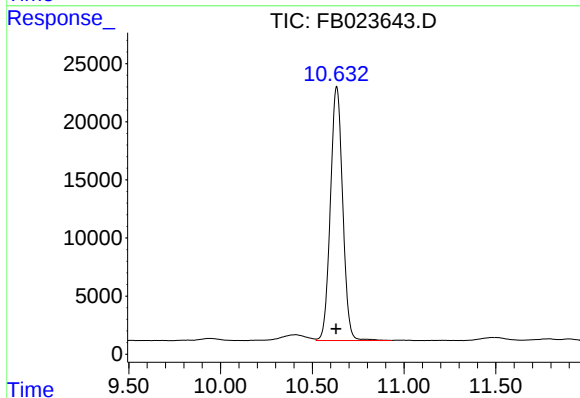


#6 Toluene

R.T.: 10.633 min
Delta R.T.: 0.003 min
Response: 1015827
Conc: 25.59 ng/ml

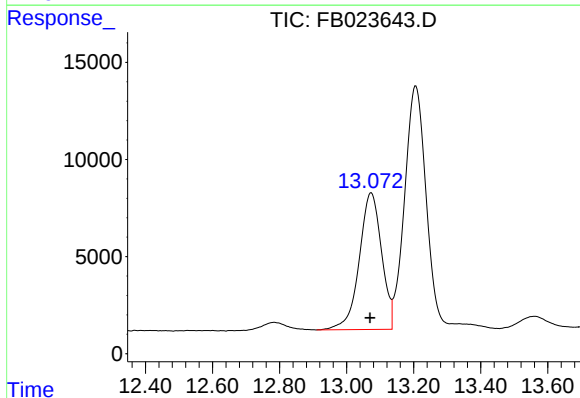


#7 Ethylbenzene

R.T.: 13.073 min
Delta R.T.: 0.003 min
Response: 324740
Conc: 8.74 ng/ml

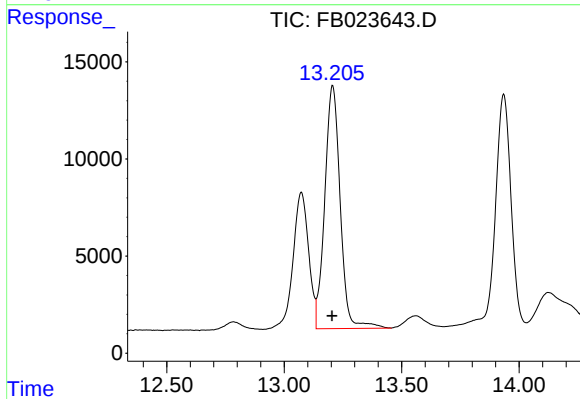

#8 m-Xylene


R.T.: 13.206 min
Delta R.T.: 0.003 min
Response: 571395
Conc: 16.00 ng/ml

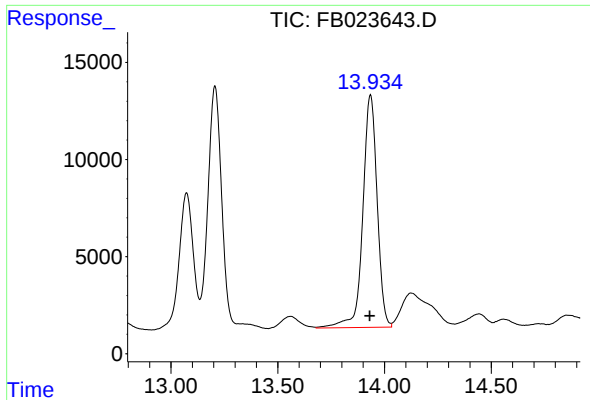

#9 O-Xylene

R.T.: 13.935 min
Delta R.T.: 0.003 min
Response: 557776
Conc: 16.17 ng/ml

Instrument :
FID_B
ClientSampleId :
CL-01-020520MS

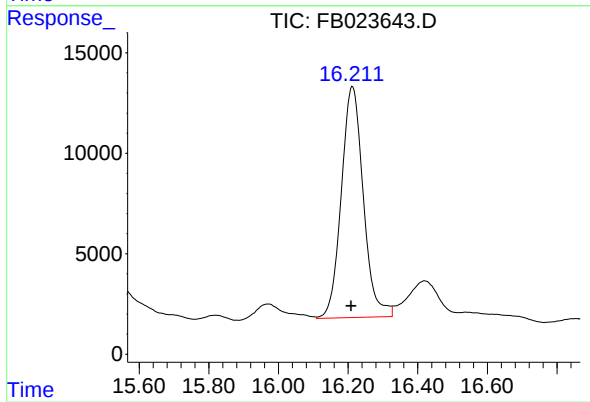

#10 1,2,4-Trimethylbenzene

R.T.: 16.213 min
Delta R.T.: 0.004 min
Response: 504455
Conc: 17.23 ng/ml