

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020620\
 Data File : FB023644.D
 Signal(s) : FID2B.CH
 Acq On : 6 Feb 2020 16:49
 Operator : DD/AJ
 Sample : L1365-02MSD
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 CL-01-020520MSD

Integration File: Calibration.e
 Quant Time: Feb 07 03:19:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
 Quant Title :
 QLast Update : Thu Feb 06 11:13:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.802	317569	15.598 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.691	539009	17.913 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	458641	14.055 ng/ml
3) t n-Heptane	7.760	149687	4.652 ng/ml
4) t Benzene	7.894	318086	7.777 ng/ml
6) t Toluene	10.633	868703	21.884 ng/ml
7) t Ethylbenzene	13.074	288211	7.753 ng/ml
8) t m-Xylene	13.206	503981	14.112 ng/ml
9) t O-Xylene	13.935	502506	14.570 ng/ml
10) t 1,2,4-Trimethylbenzene	16.213	470578	16.072 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020620\
Data File : FB023644.D
Signal(s) : FID2B.CH
Acq On : 6 Feb 2020 16:49
Operator : DD/AJ
Sample : L1365-02MSD
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
CL-01-020520MSD

Integration File: Calibration.e
Quant Time: Feb 07 03:19:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
Quant Title :
QLast Update : Thu Feb 06 11:13:47 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

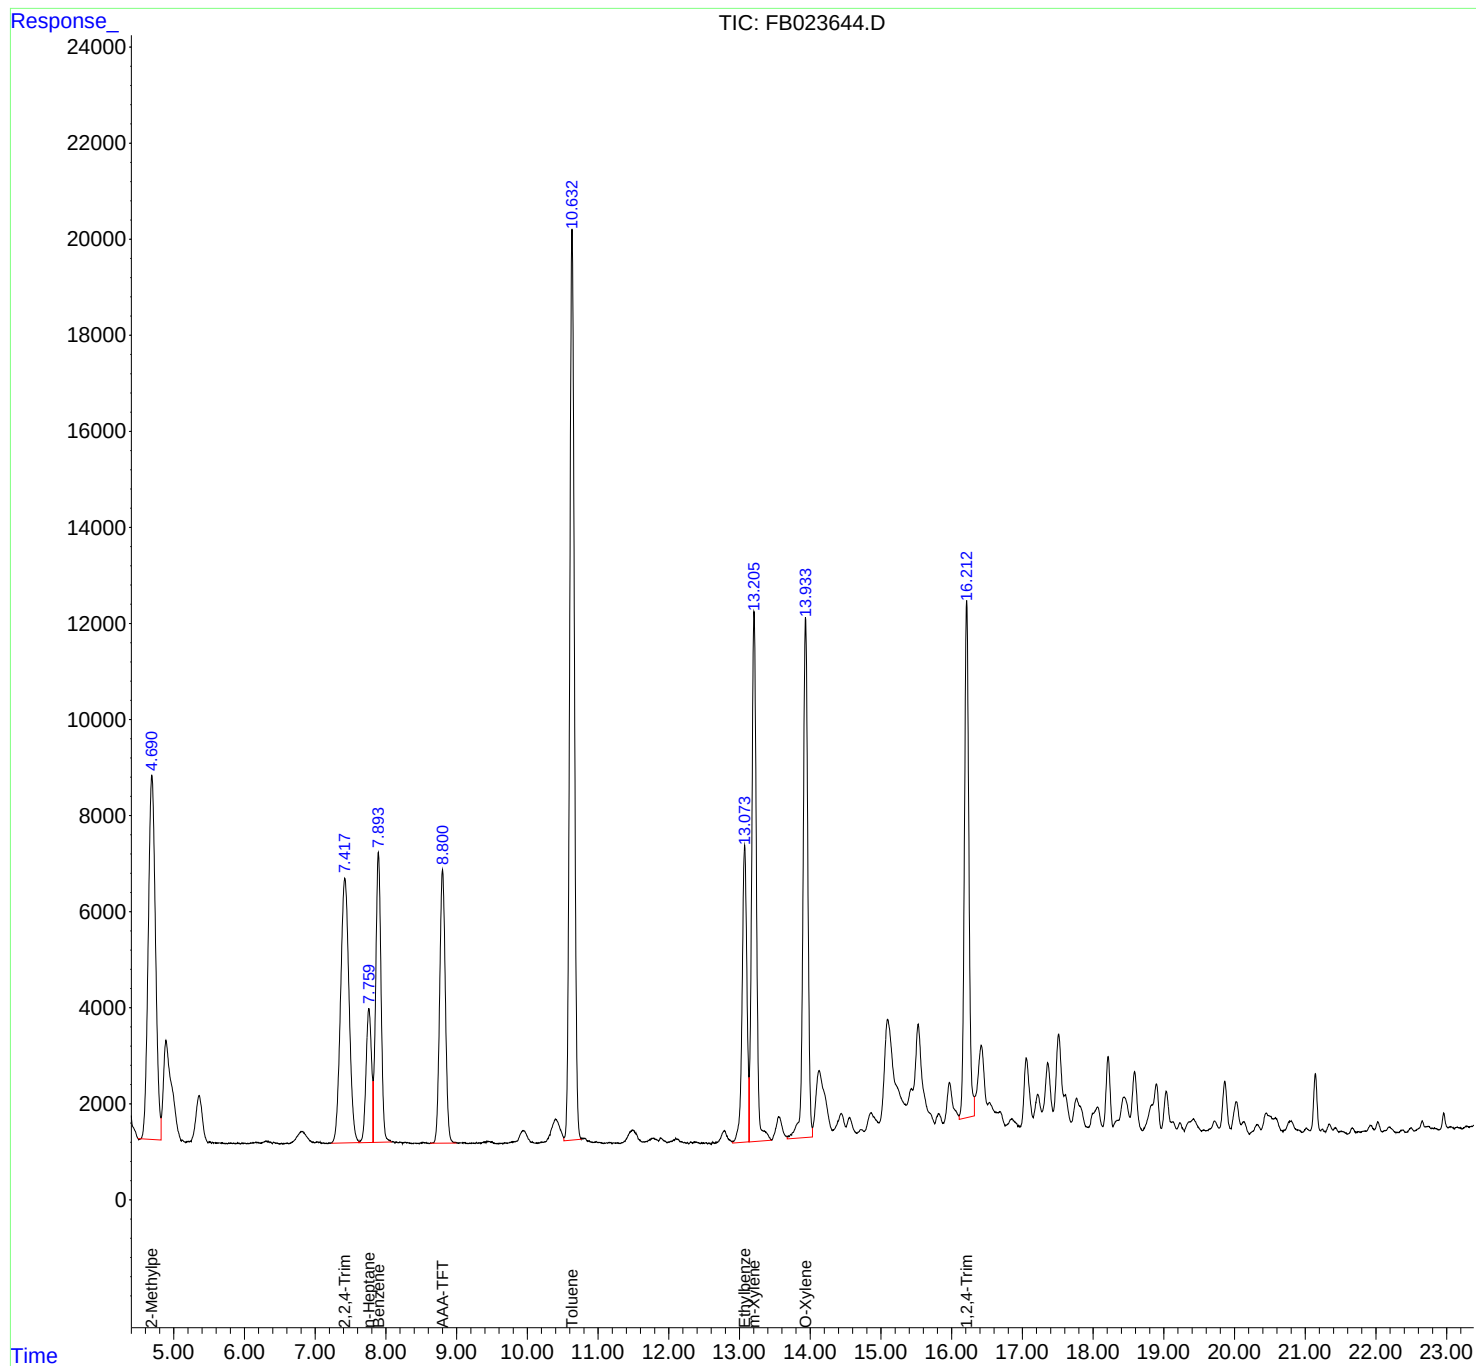


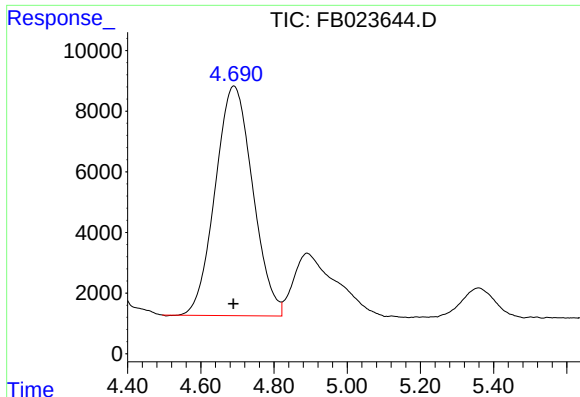

#1 2-Methylpentane


R.T.: 4.691 min
Delta R.T.: 0.002 min
Response: 539009
Conc: 17.91 ng/ml

Instrument :
FID_B
ClientSampleId :
CL-01-020520MSD

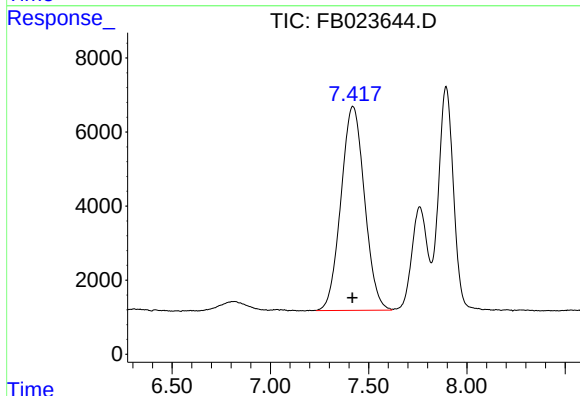


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.002 min
Response: 458641
Conc: 14.06 ng/ml

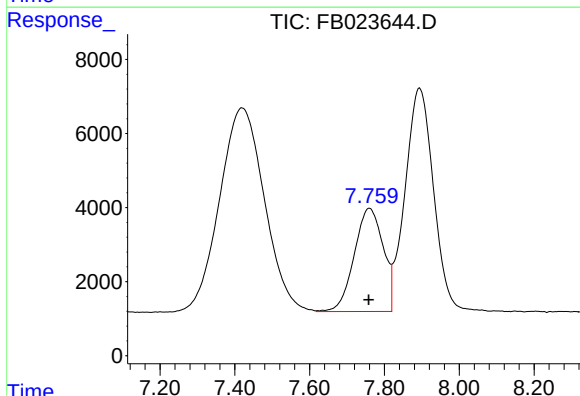


#3 n-Heptane

R.T.: 7.760 min
Delta R.T.: 0.002 min
Response: 149687
Conc: 4.65 ng/ml

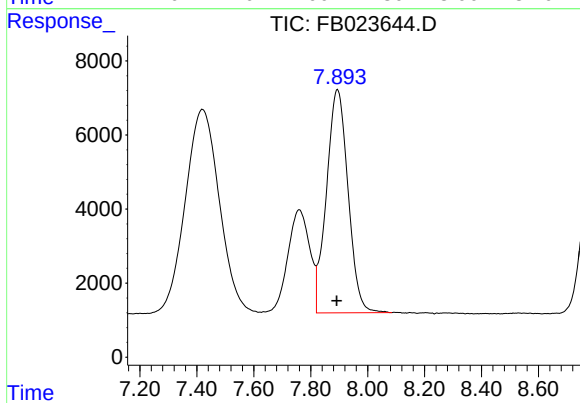

#4 Benzene


R.T.: 7.894 min
Delta R.T.: 0.003 min
Response: 318086
Conc: 7.78 ng/ml

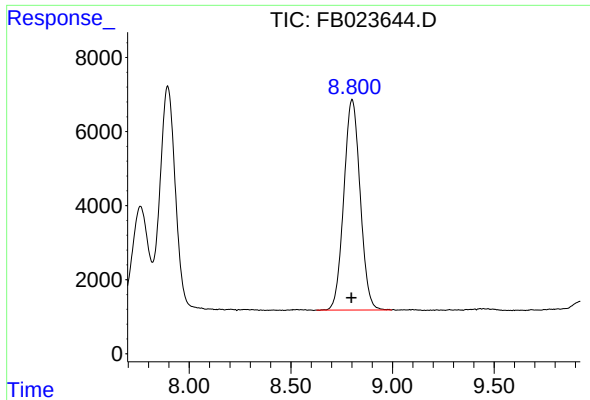

#5 AAA-TFT


R.T.: 8.802 min
Delta R.T.: 0.003 min
Response: 317569
Conc: 15.60 ng/ml

Instrument :
FID_B
ClientSampleId :
CL-01-020520MSD

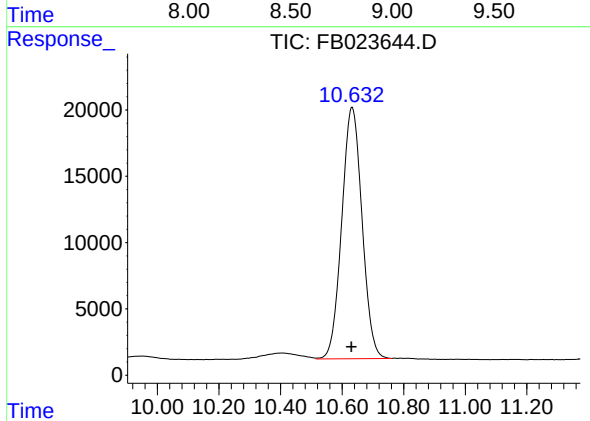


#6 Toluene

R.T.: 10.633 min
Delta R.T.: 0.003 min
Response: 868703
Conc: 21.88 ng/ml

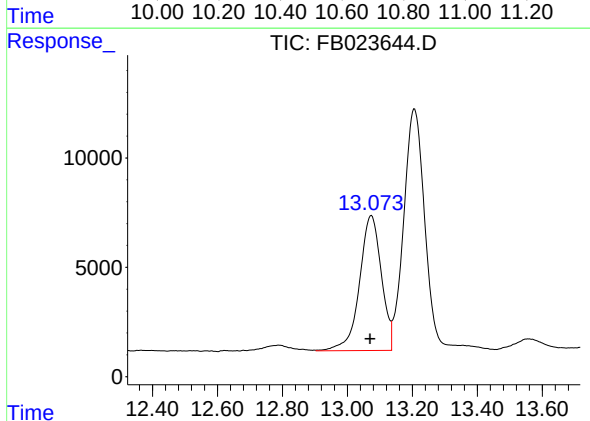


#7 Ethylbenzene

R.T.: 13.074 min
Delta R.T.: 0.004 min
Response: 288211
Conc: 7.75 ng/ml

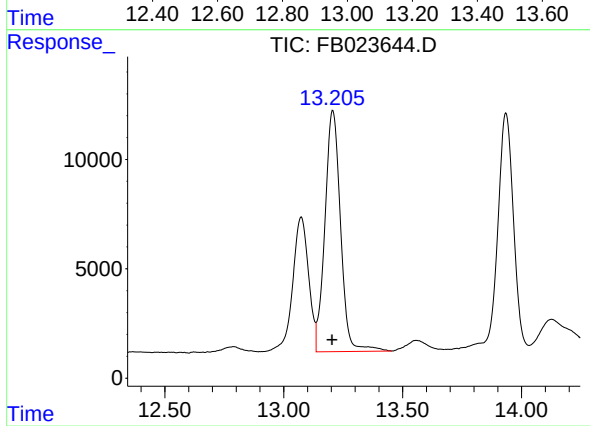

#8 m-Xylene


R.T.: 13.206 min
Delta R.T.: 0.003 min
Response: 503981
Conc: 14.11 ng/ml

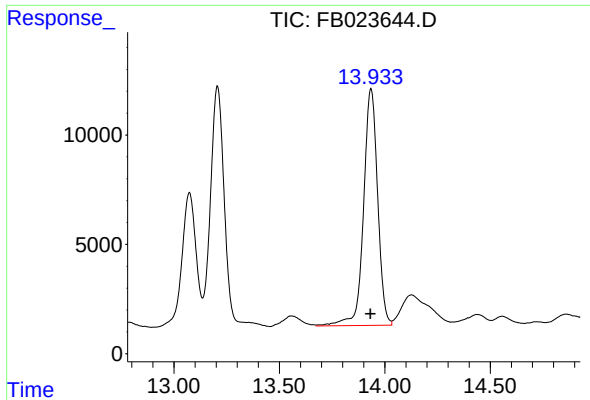

#9 O-Xylene

R.T.: 13.935 min
Delta R.T.: 0.003 min
Response: 502506
Conc: 14.57 ng/ml

Instrument :
FID_B
ClientSampleId :
CL-01-020520MSD

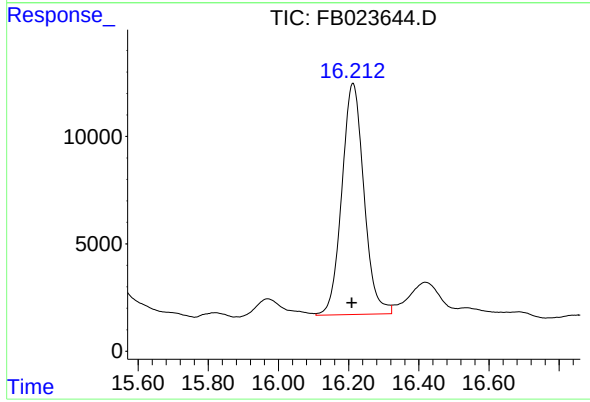

#10 1,2,4-Trimethylbenzene

R.T.: 16.213 min
Delta R.T.: 0.004 min
Response: 470578
Conc: 16.07 ng/ml