

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020623\
 Data File : FB029253.D
 Signal(s) : FID2B.CH
 Acq On : 6 Feb 2023 17:39
 Operator : YP/AJ
 Sample : BSF0206S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0206S1

Integration File: Calibration.e
 Quant Time: Feb 07 06:08:17 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
 Quant Title :
 QLast Update : Mon Feb 06 14:33:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.788	196204	20.399 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.706	454850	28.666 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	539432	31.320 ng/ml
3) t n-Heptane	7.748	166421	9.197 ng/ml
4) t Benzene	7.884	200615	9.631 ng/ml
6) t Toluene	10.617	593626	29.293 ng/ml
7) t Ethylbenzene	13.054	190822	9.998 ng/ml
8) t m-Xylene	13.186	381810	20.140 ng/ml
9) t O-Xylene	13.913	381458	20.907 ng/ml
10) t 1,2,4-Trimethylbenzene	16.188	390242	20.737 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020623\
Data File : FB029253.D
Signal(s) : FID2B.CH
Acq On : 6 Feb 2023 17:39
Operator : YP/AJ
Sample : BSF0206S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0206S1

Integration File: Calibration.e
Quant Time: Feb 07 06:08:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
Quant Title :
QLast Update : Mon Feb 06 14:33:16 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

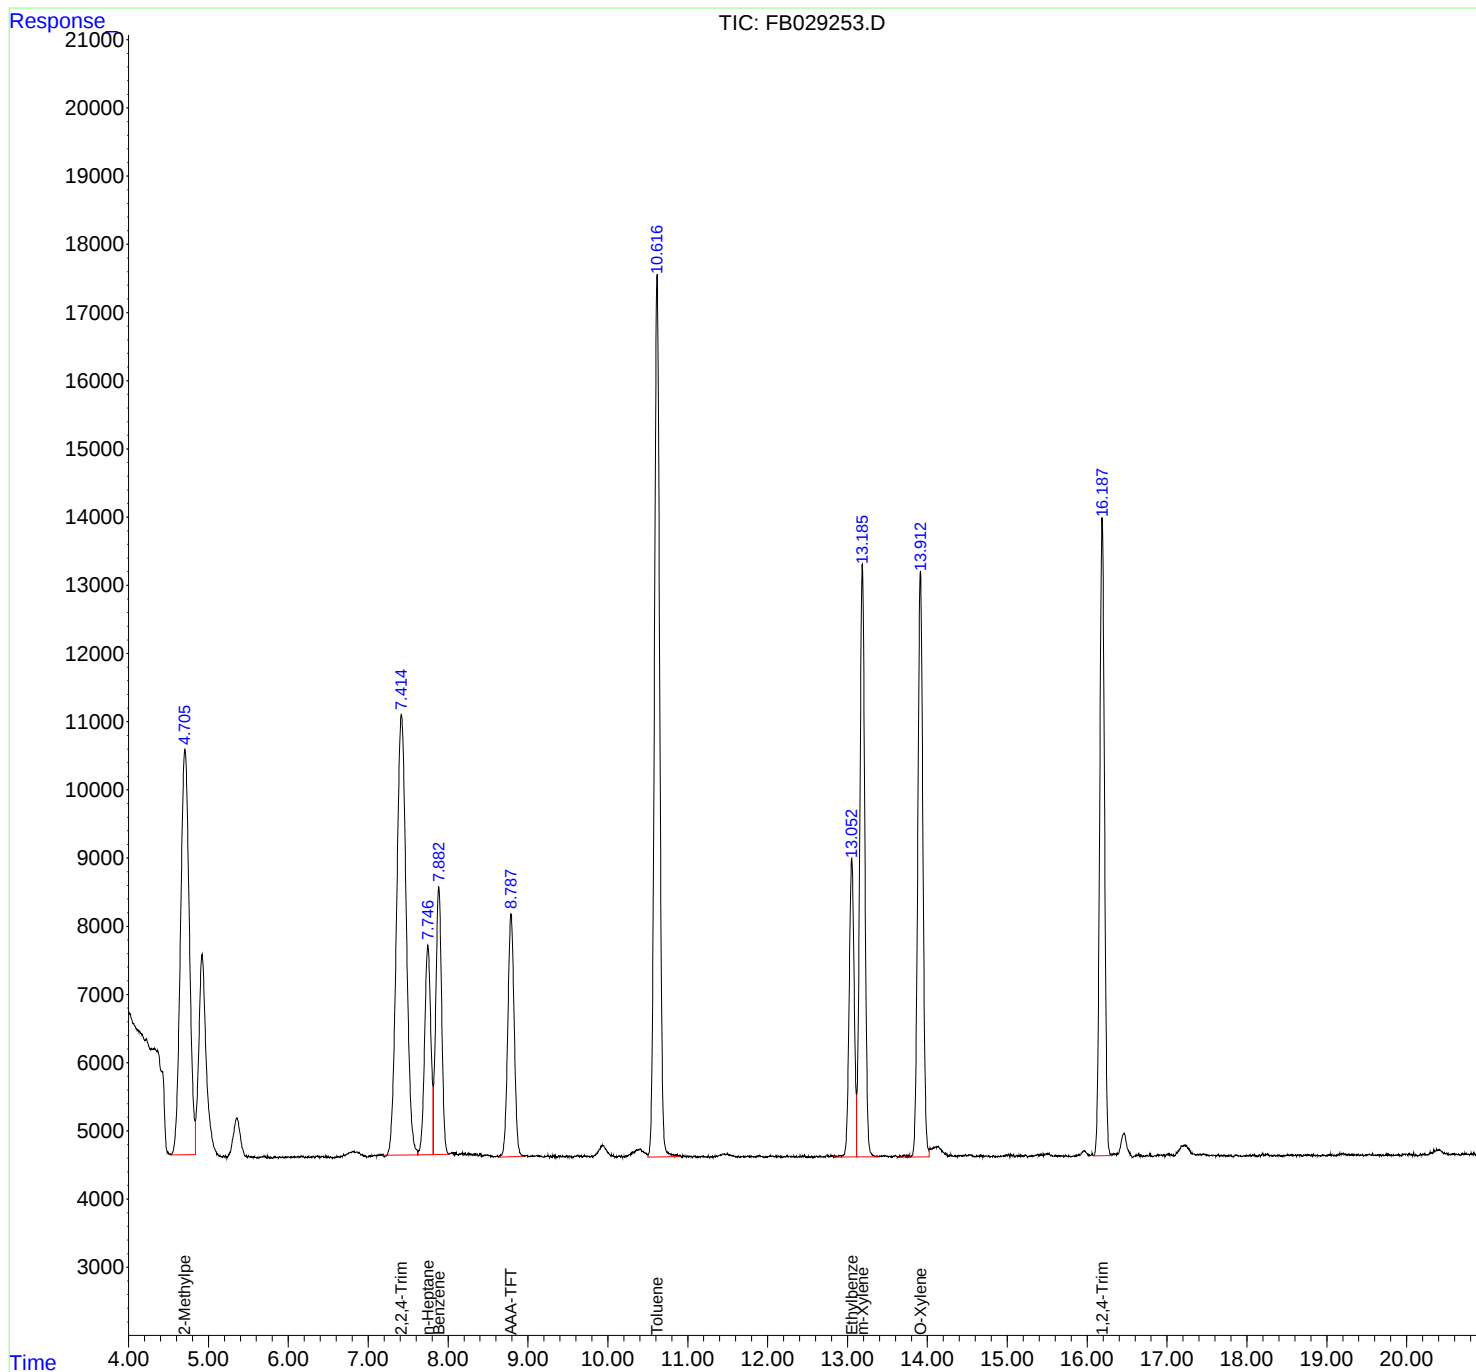


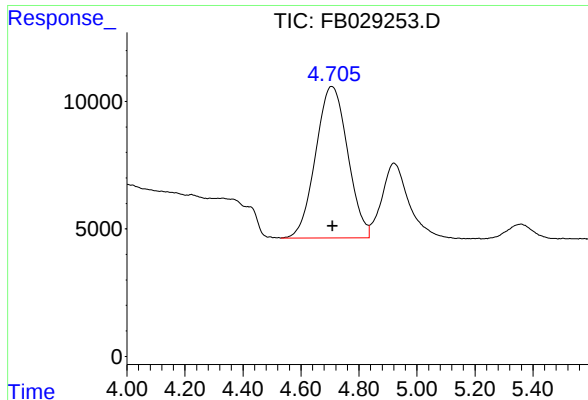

#1 2-Methylpentane


R.T.: 4.706 min
Delta R.T.: -0.003 min
Response: 454850
Conc: 28.67 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0206S1

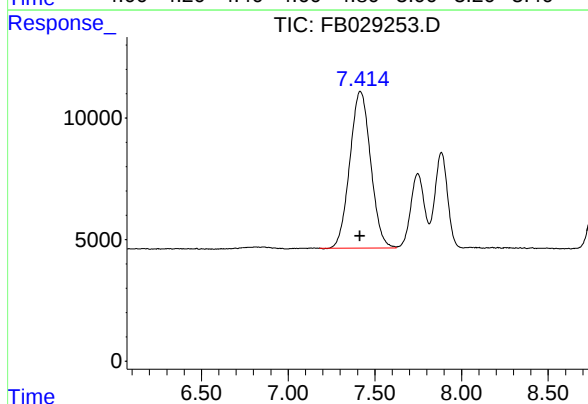


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: 0.000 min
Response: 539432
Conc: 31.32 ng/ml

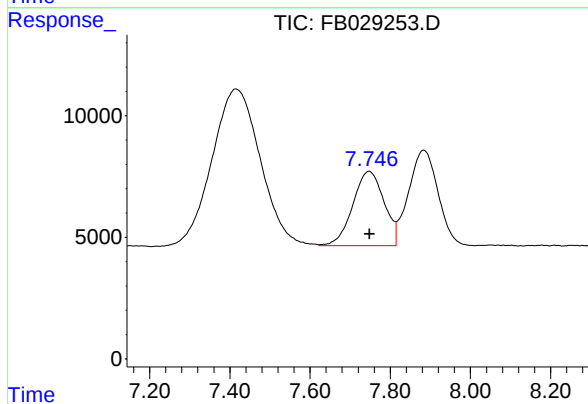


#3 n-Heptane

R.T.: 7.748 min
Delta R.T.: 0.000 min
Response: 166421
Conc: 9.20 ng/ml

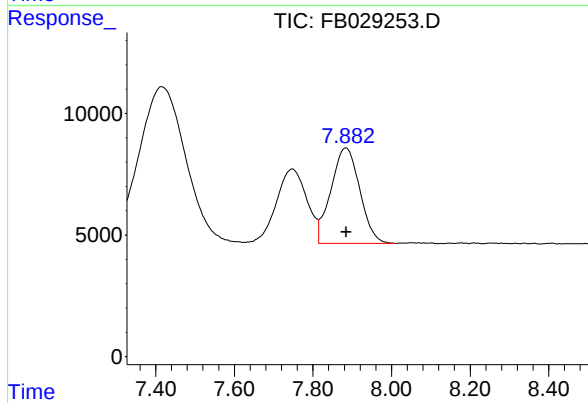

#4 Benzene


R.T.: 7.884 min
Delta R.T.: 0.000 min
Response: 200615
Conc: 9.63 ng/ml

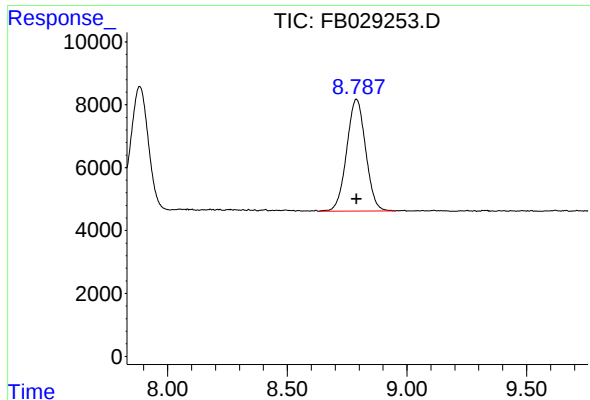

#5 AAA-TFT


R.T.: 8.788 min
Delta R.T.: 0.000 min
Response: 196204
Conc: 20.40 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0206S1

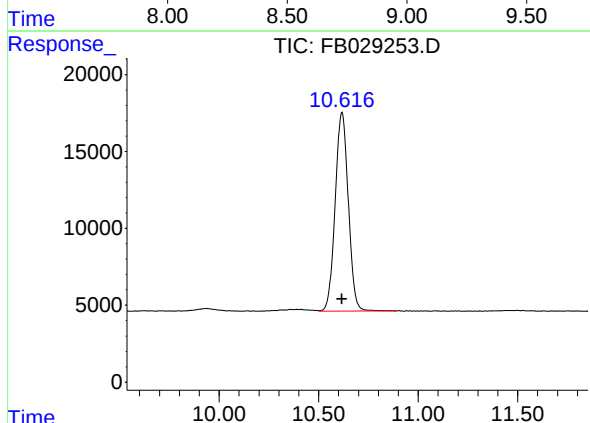


#6 Toluene

R.T.: 10.617 min
Delta R.T.: 0.000 min
Response: 593626
Conc: 29.29 ng/ml

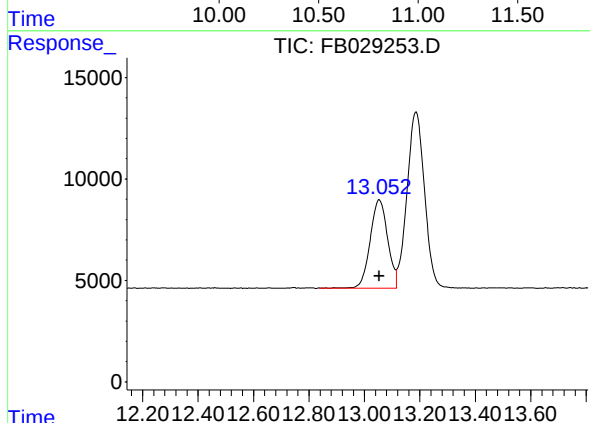


#7 Ethylbenzene

R.T.: 13.054 min
Delta R.T.: 0.000 min
Response: 190822
Conc: 10.00 ng/ml

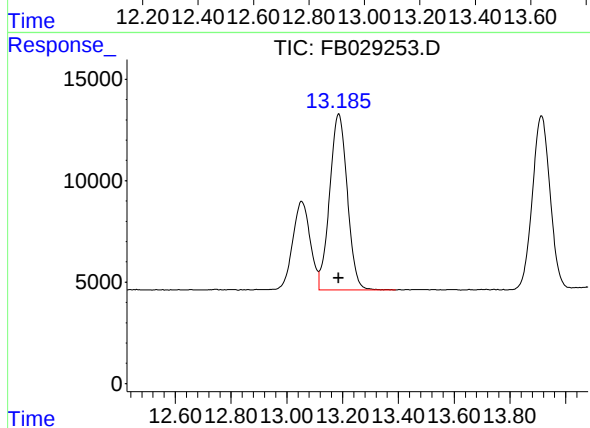

#8 m-Xylene


R.T.: 13.186 min
Delta R.T.: 0.000 min
Response: 381810
Conc: 20.14 ng/ml

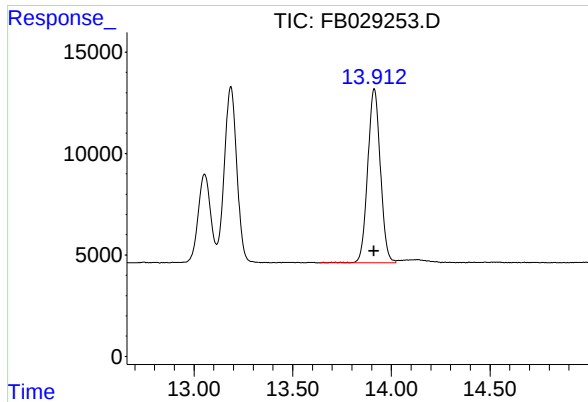

#9 O-Xylene

R.T.: 13.913 min
Delta R.T.: 0.000 min
Response: 381458
Conc: 20.91 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0206S1

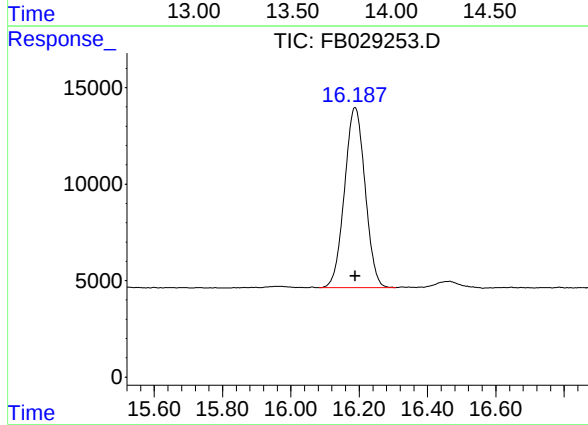

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: 0.000 min
Response: 390242
Conc: 20.74 ng/ml