

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB020623\  
Data File : FB029260.D  
Signal(s) : FID2B.CH  
Acq On : 6 Feb 2023 21:58  
Operator : YP/AJ  
Sample : 01445-07  
Misc : 5.40G/5.00 ML DI WATER  
ALS Vial : 19 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
JPP-29-020323

Integration File: Calibration.e  
Quant Time: Feb 07 06:08:49 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB020623.M  
Quant Title :  
QLast Update : Mon Feb 06 14:33:16 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

| Compound                    | R.T.   | Response | Conc Units   |
|-----------------------------|--------|----------|--------------|
| -----                       |        |          |              |
| System Monitoring Compounds |        |          |              |
| 5) s AAA-TFT                | 8.788  | 138678   | 14.418 ng/ml |
|                             |        |          |              |
| Target Compounds            |        |          |              |
| 6) t Toluene                | 10.613 | 7457     | 0.368 ng/ml  |
| -----                       |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB020623\  
Data File : FB029260.D  
Signal(s) : FID2B.CH  
Acq On : 6 Feb 2023 21:58  
Operator : YP/AJ  
Sample : 01445-07  
Misc : 5.40G/5.00 ML DI WATER  
ALS Vial : 19 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
JPP-29-020323

Integration File: Calibration.e  
Quant Time: Feb 07 06:08:49 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB020623.M  
Quant Title :  
QLast Update : Mon Feb 06 14:33:16 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

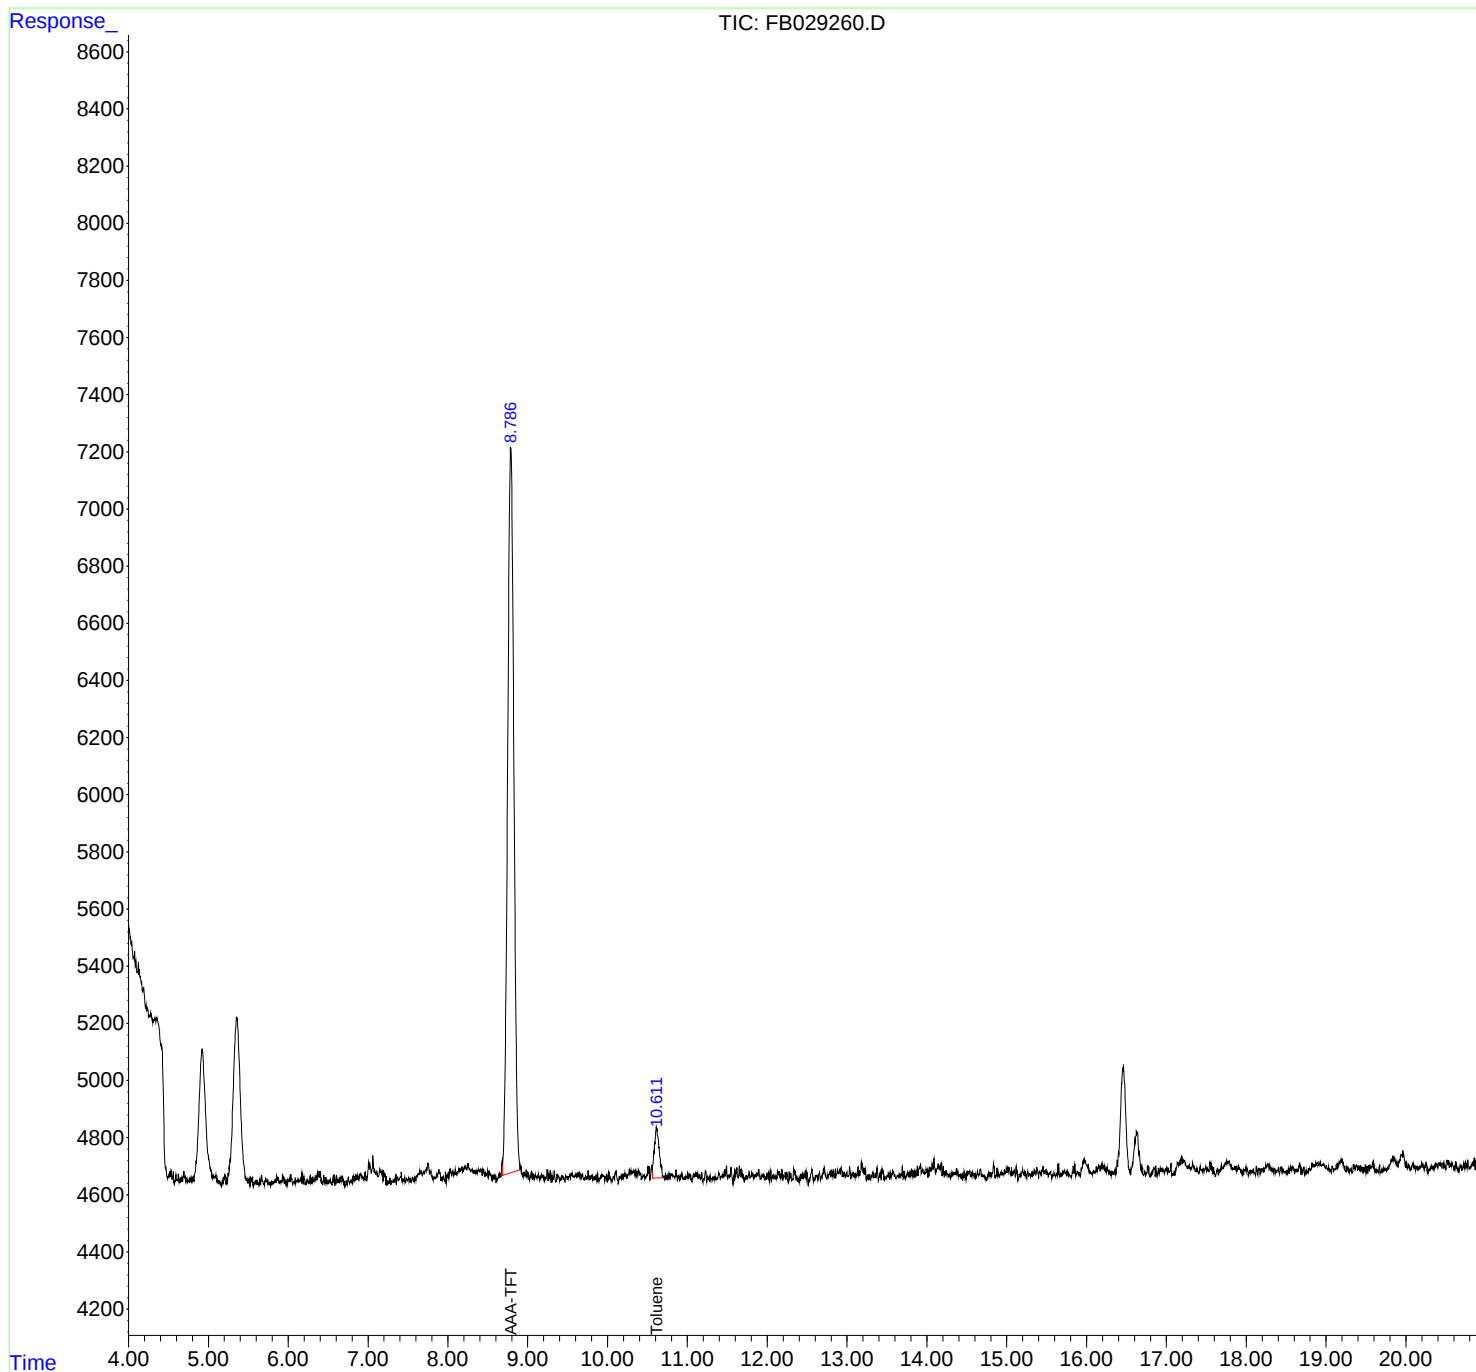


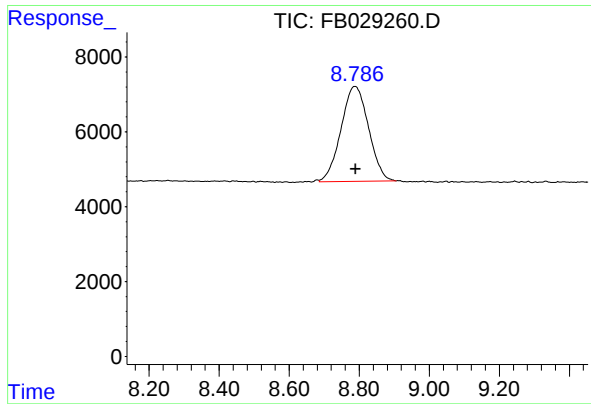

#5 AAA-TFT

R.T.: 8.788 min  
Delta R.T.: -0.001 min  
Response: 138678  
Conc: 14.42 ng/ml

Instrument :  
FID\_B  
ClientSampleId :  
JPP-29-020323

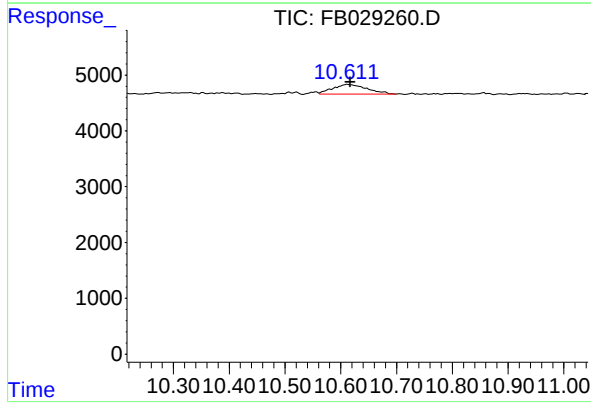

#6 Toluene

R.T.: 10.613 min  
Delta R.T.: -0.005 min  
Response: 7457  
Conc: 0.37 ng/ml