

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020623\
 Data File : FB029262.D
 Signal(s) : FID2B.CH
 Acq On : 6 Feb 2023 23:12
 Operator : YP/AJ
 Sample : BSF0206S2
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0206S2

Integration File: Calibration.e
 Quant Time: Feb 07 06:08:58 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
 Quant Title :
 QLast Update : Mon Feb 06 14:33:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.788	202538	21.058 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.703	479850	30.242 ng/ml
2) t	2,2,4-Trimethylpentane	7.413	512900	29.779 ng/ml
3) t	n-Heptane	7.747	181777	10.046 ng/ml
4) t	Benzene	7.883	214717	10.308 ng/ml
6) t	Toluene	10.616	617061	30.450 ng/ml
7) t	Ethylbenzene	13.052	193029	10.114 ng/ml
8) t	m-Xylene	13.185	383947	20.253 ng/ml
9) t	O-Xylene	13.911	373887	20.492 ng/ml
10) t	1,2,4-Trimethylbenzene	16.187	370902	19.709 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020623\
Data File : FB029262.D
Signal(s) : FID2B.CH
Acq On : 6 Feb 2023 23:12
Operator : YP/AJ
Sample : BSF0206S2
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0206S2

Integration File: Calibration.e
Quant Time: Feb 07 06:08:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
Quant Title :
QLast Update : Mon Feb 06 14:33:16 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

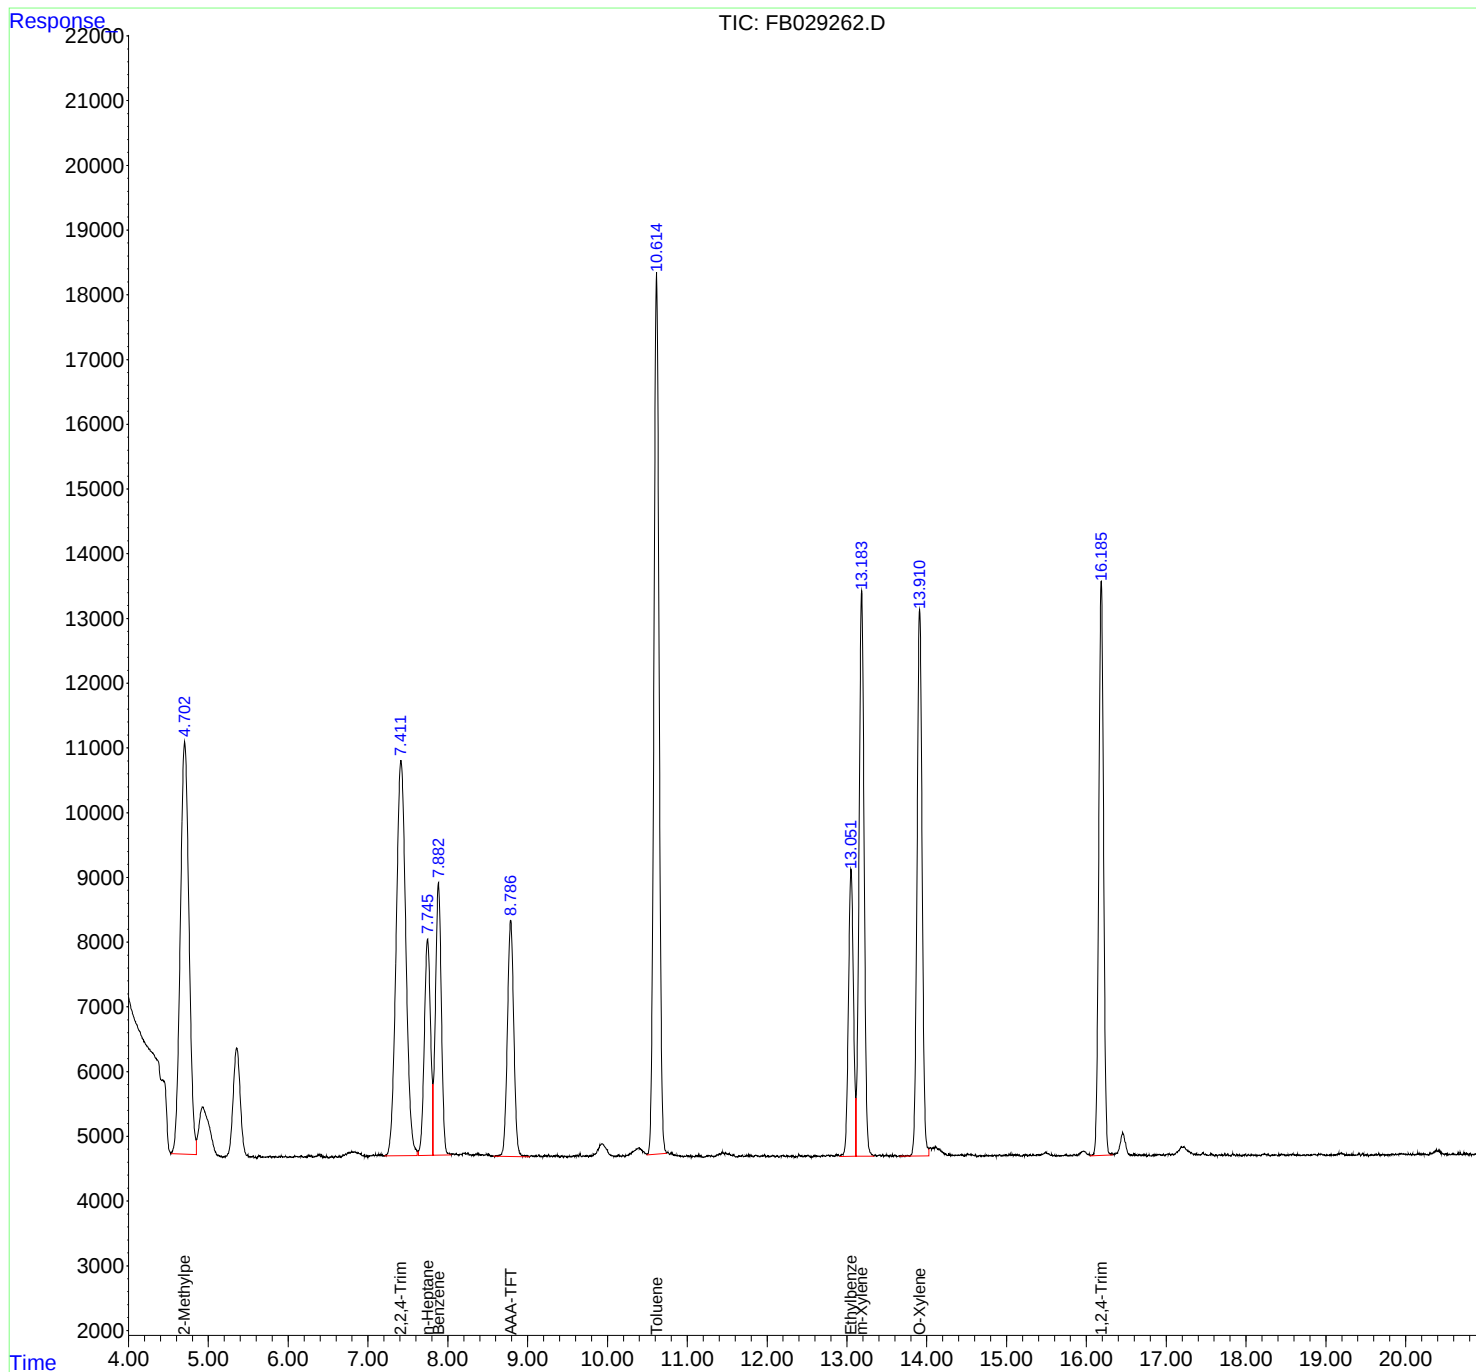


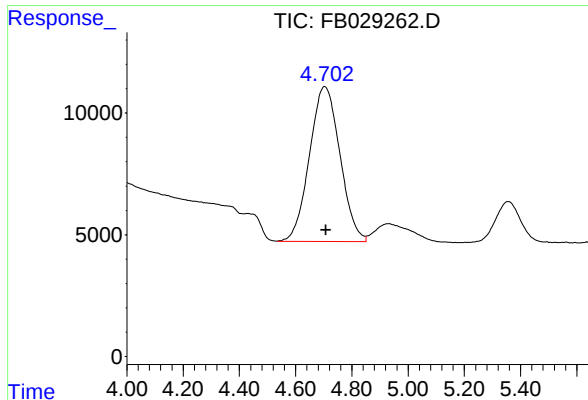

#1 2-Methylpentane


R.T.: 4.703 min
Delta R.T.: -0.006 min
Response: 479850
Conc: 30.24 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0206S2

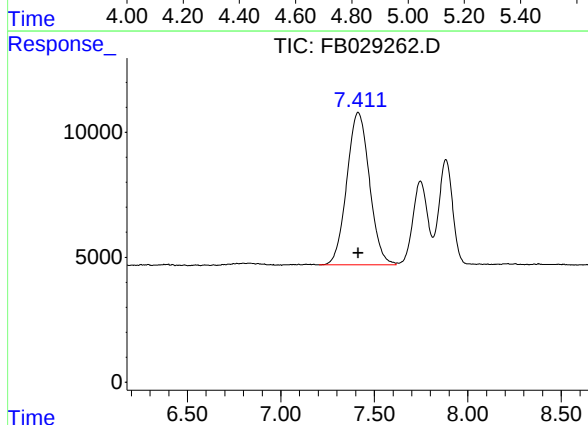


#2 2,2,4-Trimethylpentane

R.T.: 7.413 min
Delta R.T.: -0.001 min
Response: 512900
Conc: 29.78 ng/ml

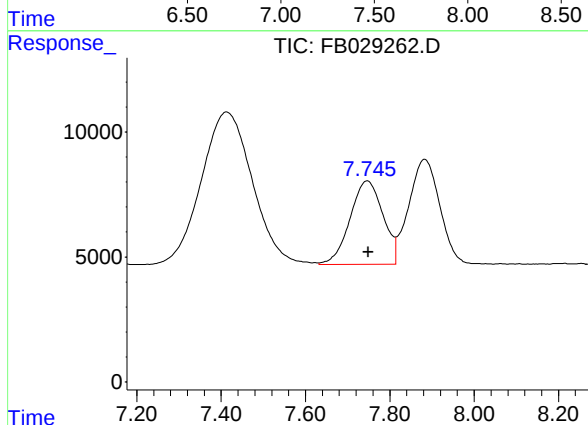


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: -0.002 min
Response: 181777
Conc: 10.05 ng/ml

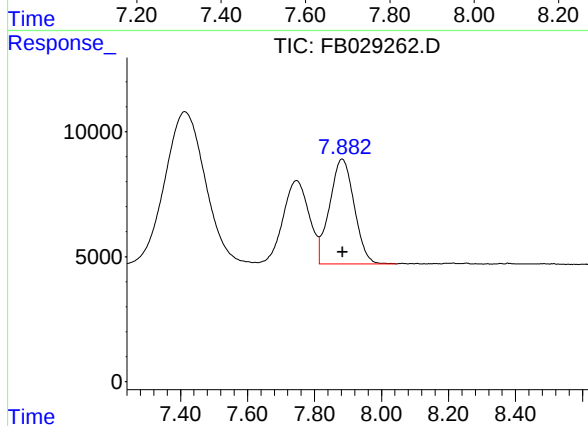

#4 Benzene


R.T.: 7.883 min
Delta R.T.: -0.002 min
Response: 214717
Conc: 10.31 ng/ml

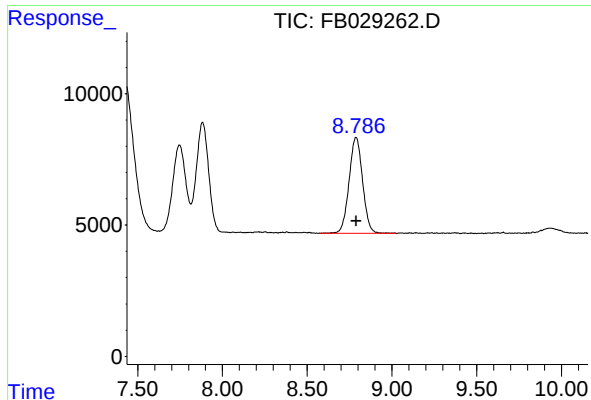

#5 AAA-TFT


R.T.: 8.788 min
Delta R.T.: -0.001 min
Response: 202538
Conc: 21.06 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0206S2

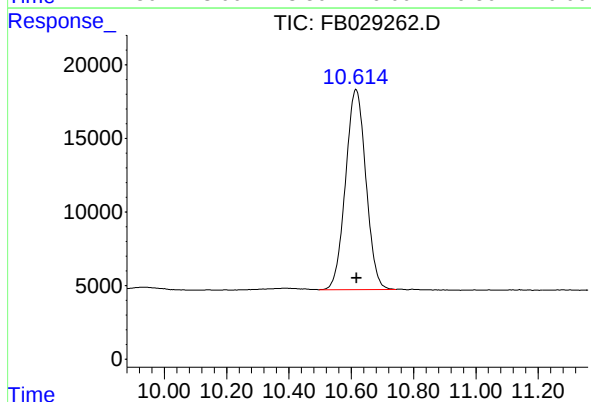


#6 Toluene

R.T.: 10.616 min
Delta R.T.: -0.001 min
Response: 617061
Conc: 30.45 ng/ml

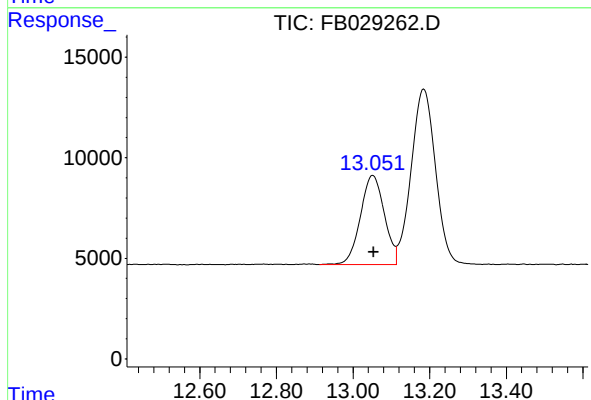


#7 Ethylbenzene

R.T.: 13.052 min
Delta R.T.: -0.002 min
Response: 193029
Conc: 10.11 ng/ml

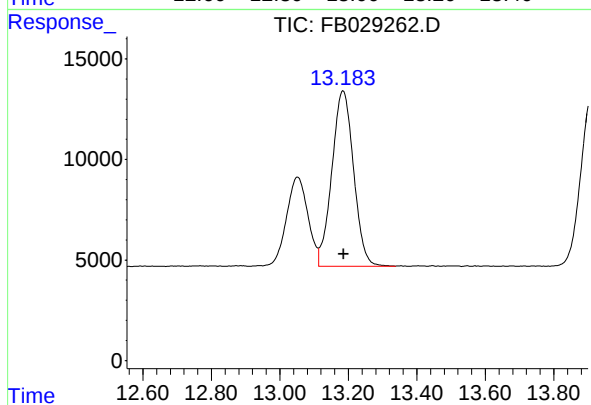

#8 m-Xylene


R.T.: 13.185 min
Delta R.T.: -0.001 min
Response: 383947
Conc: 20.25 ng/ml

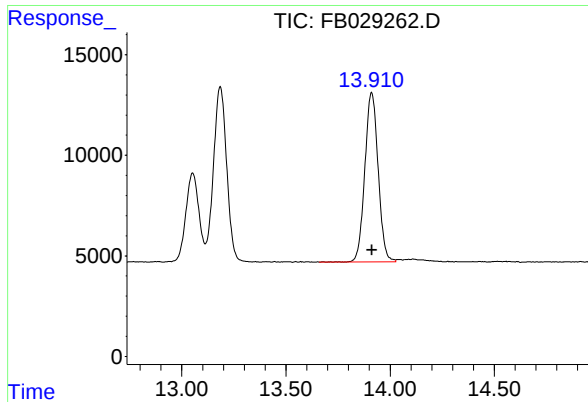

#9 O-Xylene

R.T.: 13.911 min
Delta R.T.: -0.001 min
Response: 373887
Conc: 20.49 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0206S2

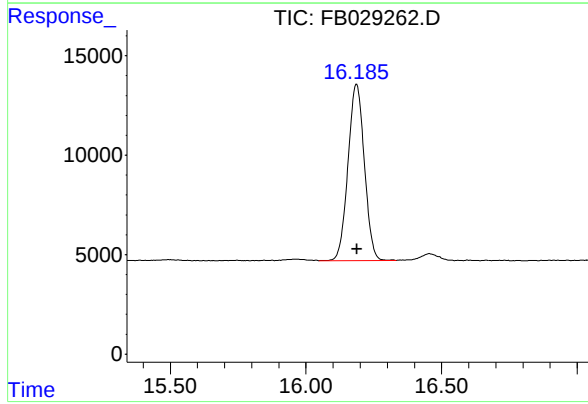

#10 1,2,4-Trimethylbenzene

R.T.: 16.187 min
Delta R.T.: -0.001 min
Response: 370902
Conc: 19.71 ng/ml