

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020623\
 Data File : FB029249.D
 Signal(s) : FID2B.CH
 Acq On : 6 Feb 2023 15:00
 Operator : YP/AJ
 Sample : FB020623GROICV
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 FB020623GROICV

Integration File: Calibration.e
 Quant Time: Feb 06 15:11:09 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
 Quant Title :
 QLast Update : Mon Feb 06 14:33:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	173300	18.018 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.702	389908	24.574 ng/ml
2) t 2,2,4-Trimethylpentane	7.413	400176	23.234 ng/ml
3) t n-Heptane	7.747	149567	8.266 ng/ml
4) t Benzene	7.884	169437	8.134 ng/ml
6) t Toluene	10.618	491897	24.273 ng/ml
7) t Ethylbenzene	13.055	154141	8.076 ng/ml
8) t m-Xylene	13.187	309450	16.323 ng/ml
9) t O-Xylene	13.914	300228	16.455 ng/ml
10) t 1,2,4-Trimethylbenzene	16.189	300345	15.960 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020623\
Data File : FB029249.D
Signal(s) : FID2B.CH
Acq On : 6 Feb 2023 15:00
Operator : YP/AJ
Sample : FB020623GROICV
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
FB020623GROICV

Integration File: Calibration.e
Quant Time: Feb 06 15:11:09 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
Quant Title :
QLast Update : Mon Feb 06 14:33:16 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

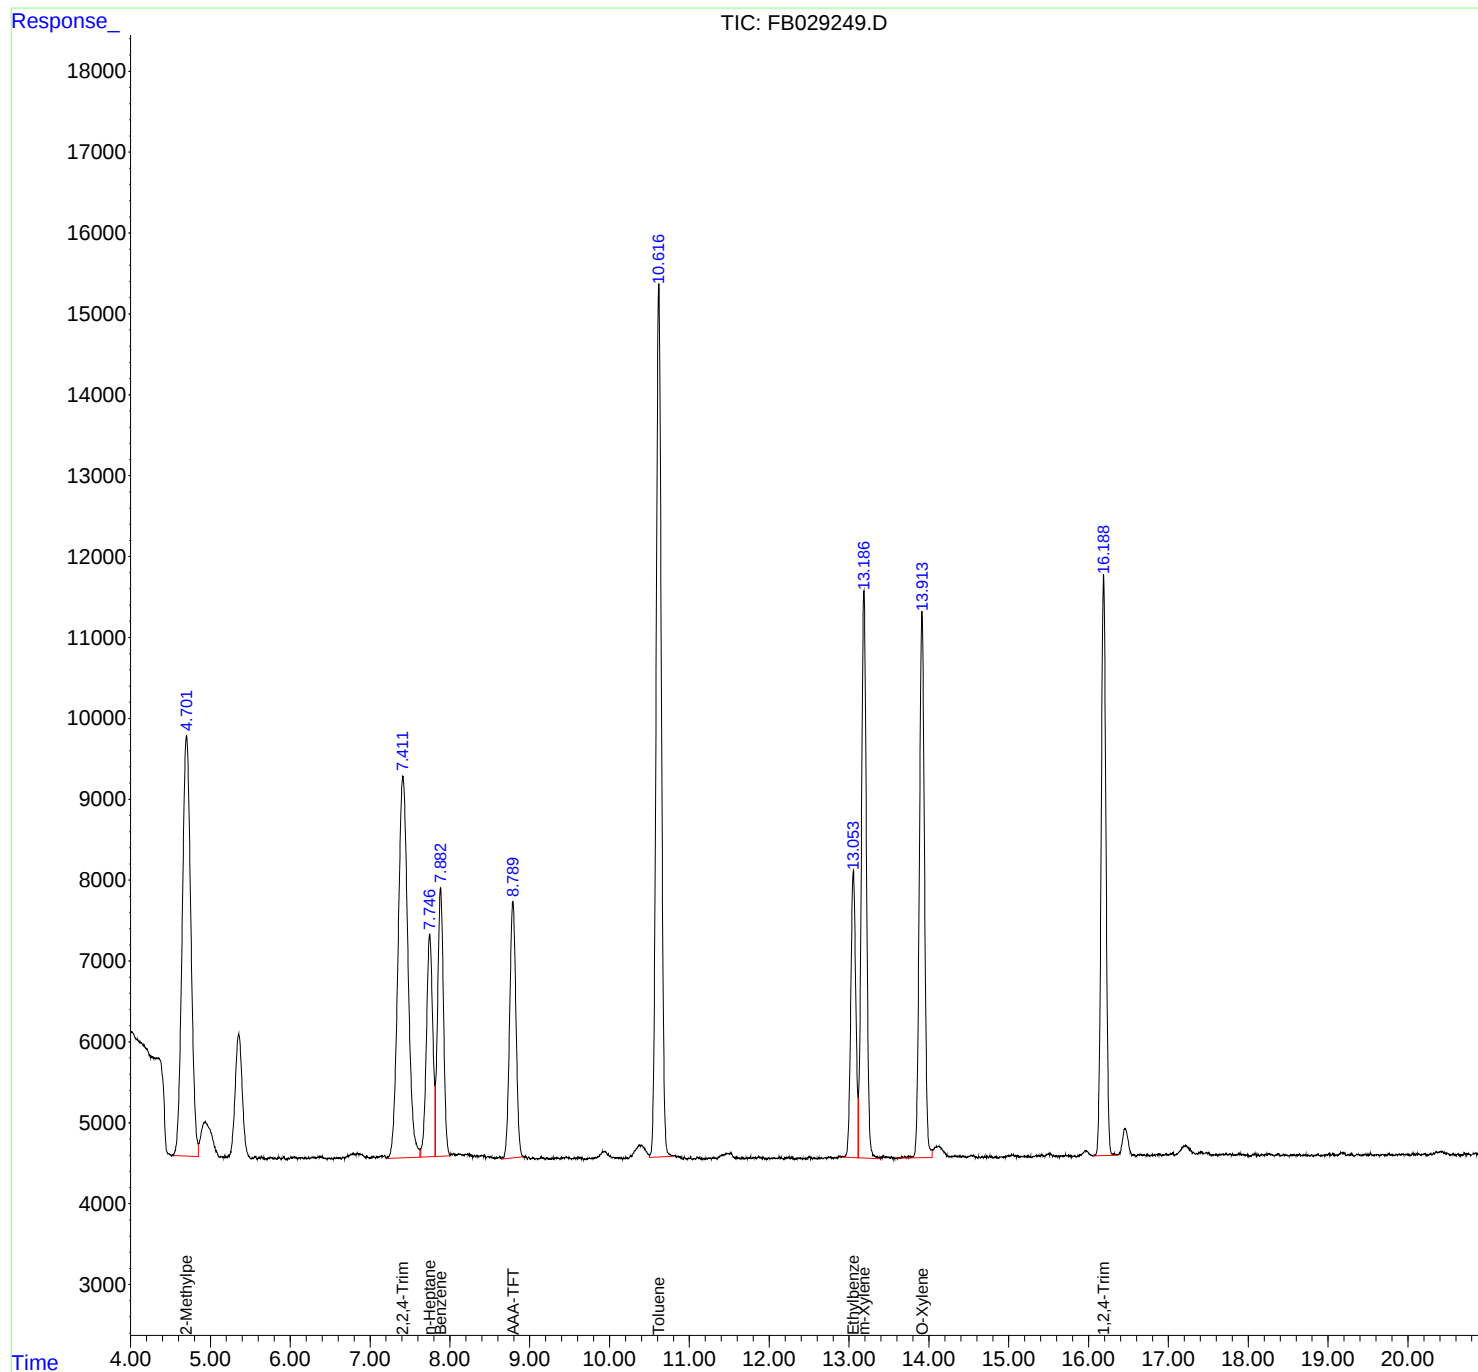


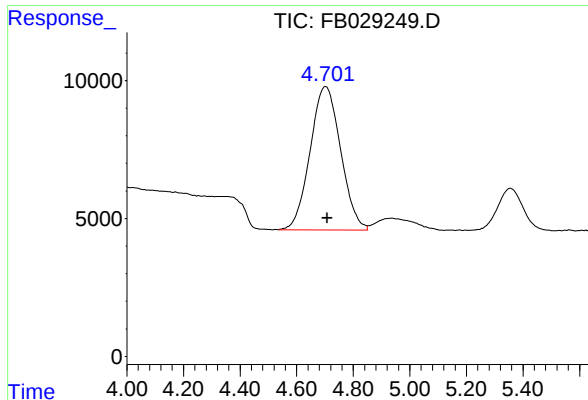

#1 2-Methylpentane


R.T.: 4.702 min
Delta R.T.: -0.007 min
Response: 389908
Conc: 24.57 ng/ml

Instrument :
FID_B
ClientSampleId :
FB020623GROICV

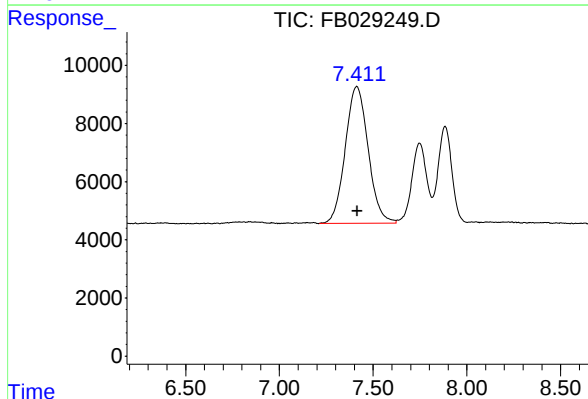


#2 2,2,4-Trimethylpentane

R.T.: 7.413 min
Delta R.T.: -0.002 min
Response: 400176
Conc: 23.23 ng/ml

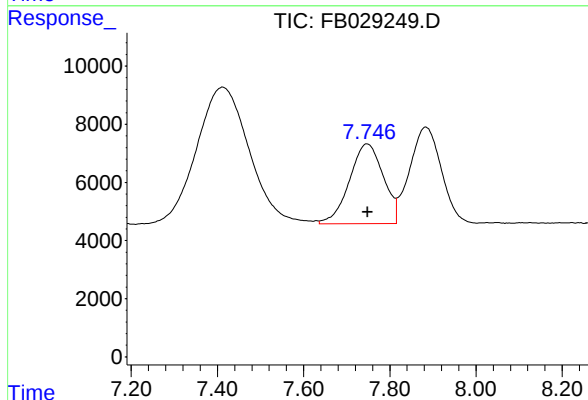


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: -0.002 min
Response: 149567
Conc: 8.27 ng/ml

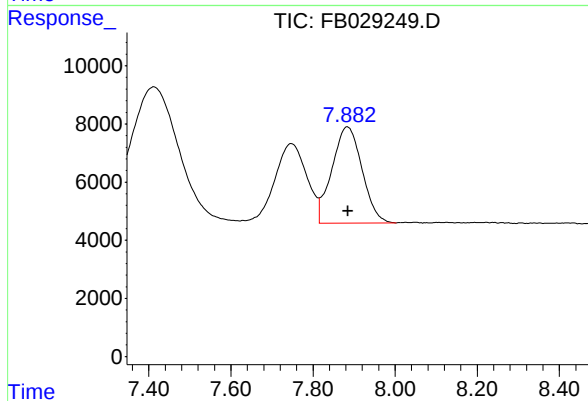

#4 Benzene


R.T.: 7.884 min
Delta R.T.: 0.000 min
Response: 169437
Conc: 8.13 ng/ml

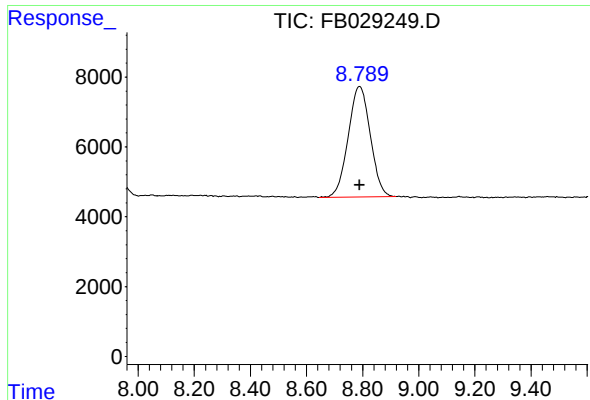

#5 AAA-TFT


R.T.: 8.789 min
Delta R.T.: 0.000 min
Response: 173300
Conc: 18.02 ng/ml

Instrument :
FID_B
ClientSampleId :
FB020623GROICV

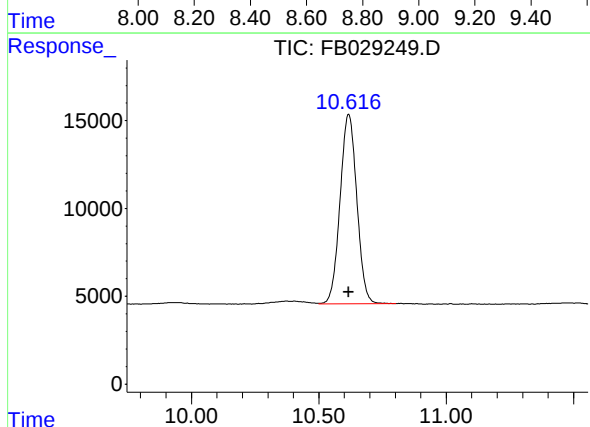


#6 Toluene

R.T.: 10.618 min
Delta R.T.: 0.000 min
Response: 491897
Conc: 24.27 ng/ml

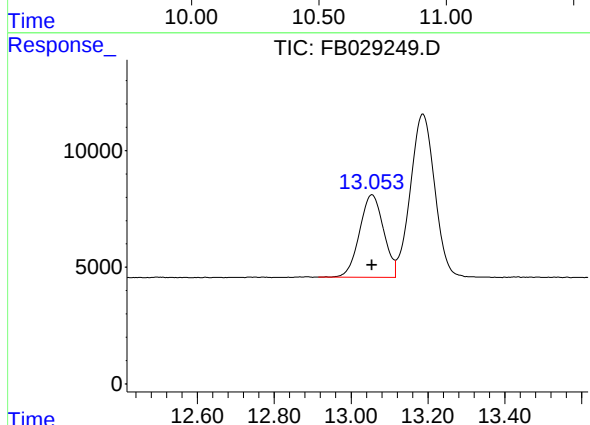


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: 0.000 min
Response: 154141
Conc: 8.08 ng/ml

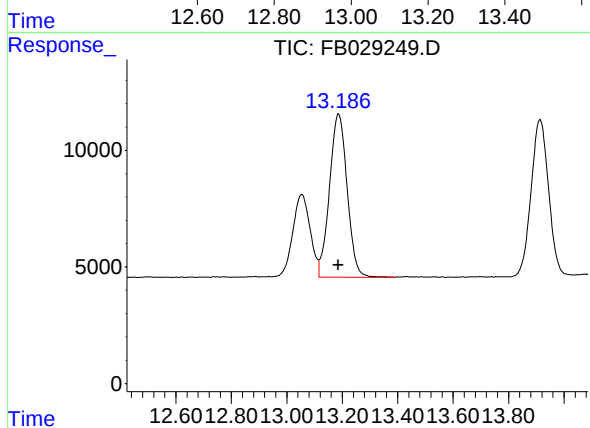

#8 m-Xylene


R.T.: 13.187 min
Delta R.T.: 0.000 min
Response: 309450
Conc: 16.32 ng/ml

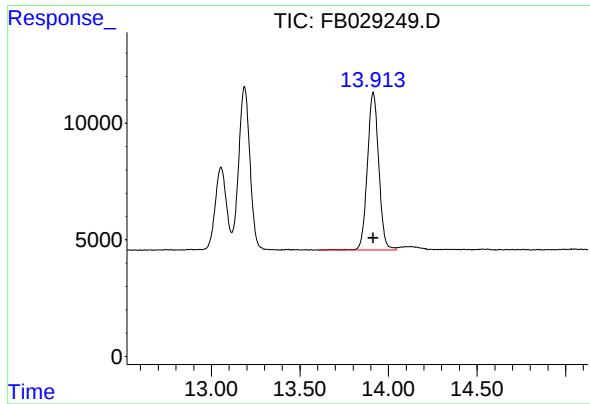

#9 O-Xylene

R.T.: 13.914 min
Delta R.T.: 0.000 min
Response: 300228
Conc: 16.45 ng/ml

Instrument :
FID_B
ClientSampleId :
FB020623GROICV

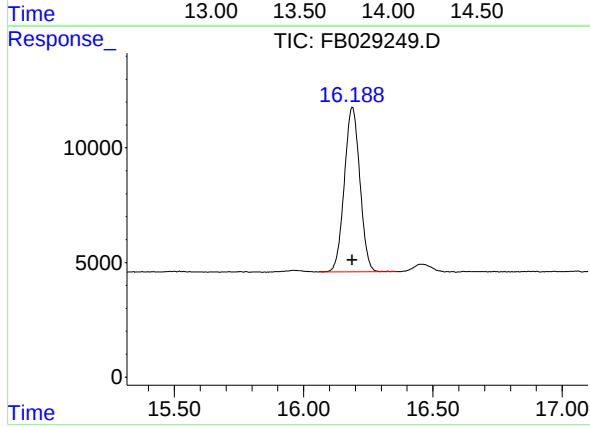

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min
Delta R.T.: 0.000 min
Response: 300345
Conc: 15.96 ng/ml