

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020625\
 Data File : FB031459.D
 Signal(s) : FID2B.CH
 Acq On : 6 Feb 2025 14:39
 Operator : YP/AJ
 Sample : BSF0206S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0206S2

Integration File: Calibration.e
 Quant Time: Feb 07 01:44:03 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011525.M
 Quant Title :
 QLast Update : Wed Jan 15 12:01:08 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	495709	20.782 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.722	1089103	32.858 ng/ml
2) t 2,2,4-Trimethylpentane	7.426	1235530	32.853 ng/ml
3) t n-Heptane	7.755	413966	11.467 ng/ml
4) t Benzene	7.894	472090	11.085 ng/ml
6) t Toluene	10.623	1293630	33.130 ng/ml
7) t Ethylbenzene	13.060	367683	10.618 ng/ml
8) t m-Xylene	13.193	791080	21.164 ng/ml
9) t O-Xylene	13.921	739916	20.776 ng/ml
10) t 1,2,4-Trimethylbenzene	16.197	629101	22.213 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020625\
Data File : FB031459.D
Signal(s) : FID2B.CH
Acq On : 6 Feb 2025 14:39
Operator : YP/AJ
Sample : BSF0206S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0206S2

Integration File: Calibration.e
Quant Time: Feb 07 01:44:03 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011525.M
Quant Title :
QLast Update : Wed Jan 15 12:01:08 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

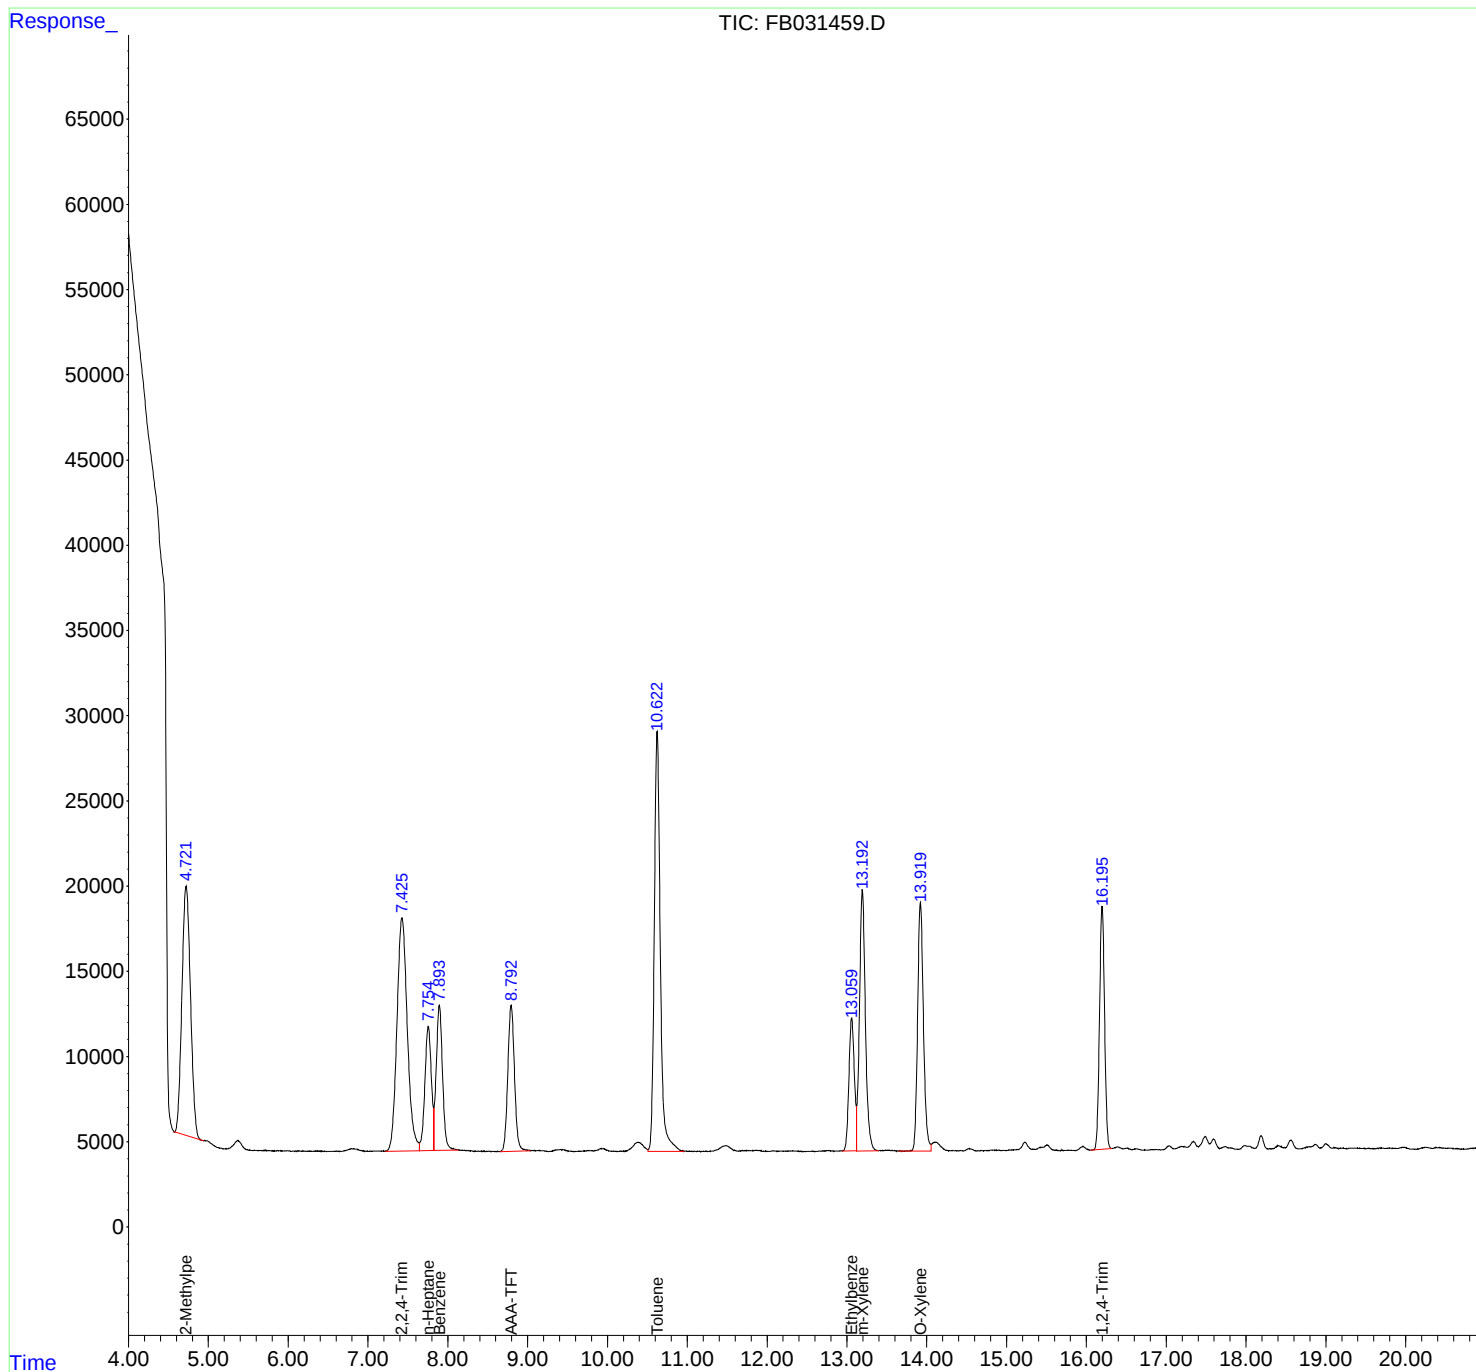


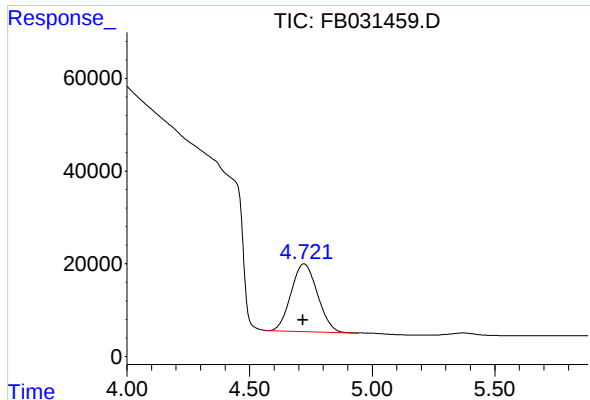

#1 2-Methylpentane


R.T.: 4.722 min
Delta R.T.: 0.004 min
Response: 1089103
Conc: 32.86 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0206S2

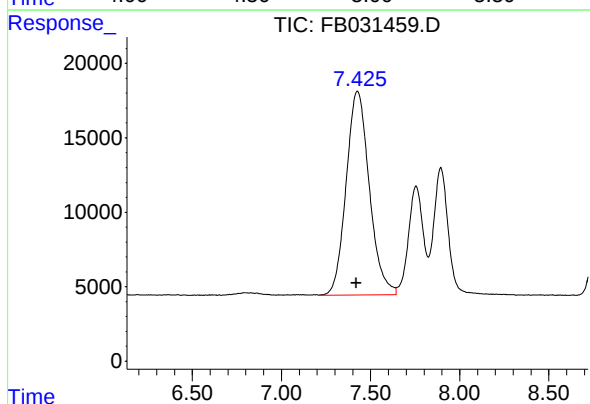


#2 2,2,4-Trimethylpentane

R.T.: 7.426 min
Delta R.T.: 0.006 min
Response: 1235530
Conc: 32.85 ng/ml

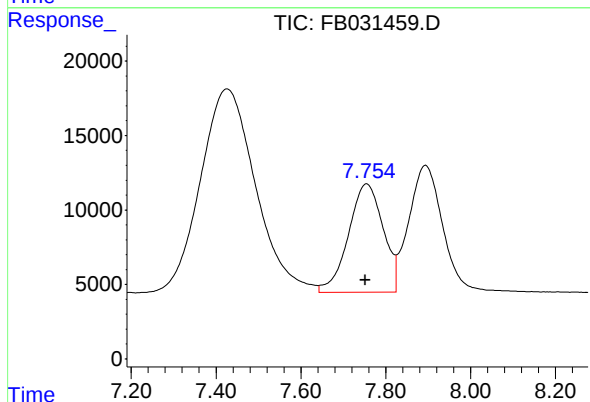


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.004 min
Response: 413966
Conc: 11.47 ng/ml

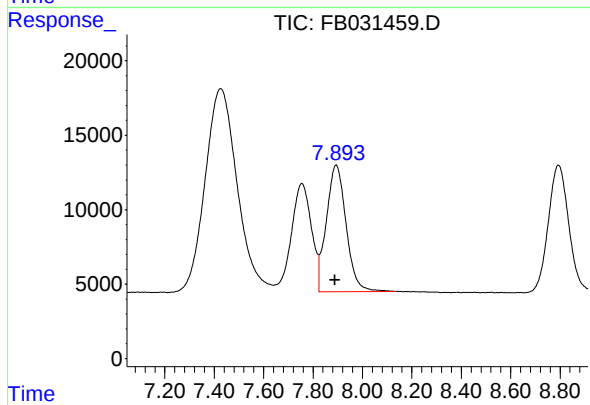

#4 Benzene


R.T.: 7.894 min
Delta R.T.: 0.004 min
Response: 472090
Conc: 11.08 ng/ml

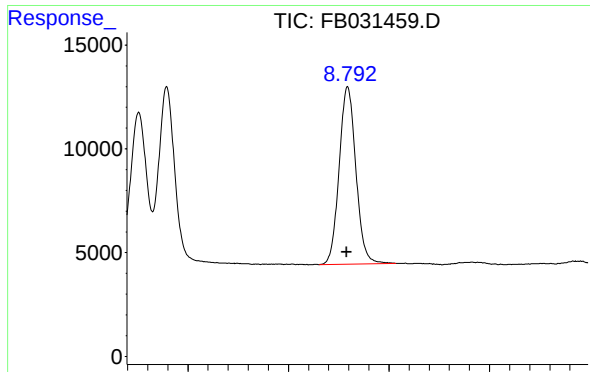

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: 0.004 min
Response: 495709
Conc: 20.78 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0206S2

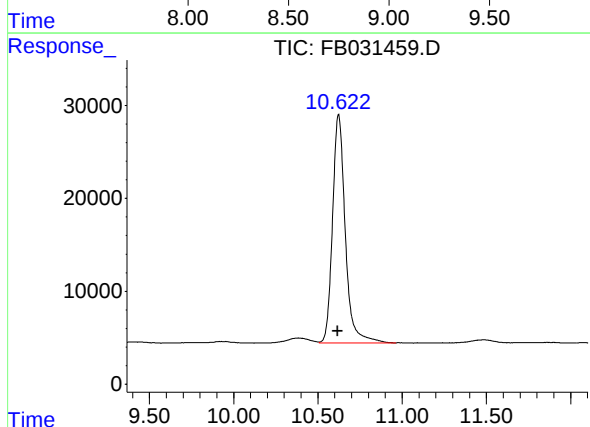


#6 Toluene

R.T.: 10.623 min
Delta R.T.: 0.005 min
Response: 1293630
Conc: 33.13 ng/ml

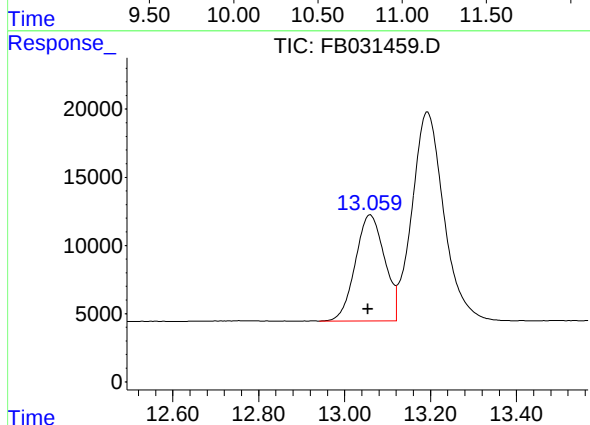


#7 Ethylbenzene

R.T.: 13.060 min
Delta R.T.: 0.005 min
Response: 367683
Conc: 10.62 ng/ml

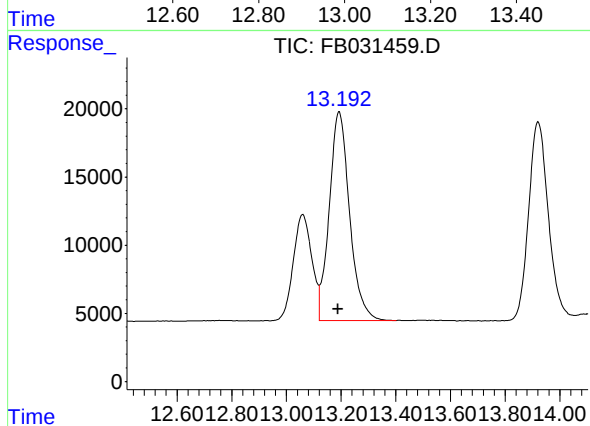

#8 m-Xylene


R.T.: 13.193 min
Delta R.T.: 0.005 min
Response: 791080
Conc: 21.16 ng/ml

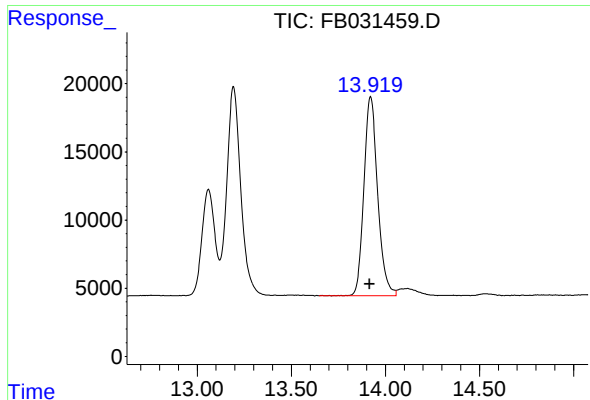

#9 O-Xylene

R.T.: 13.921 min
Delta R.T.: 0.005 min
Response: 739916
Conc: 20.78 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0206S2

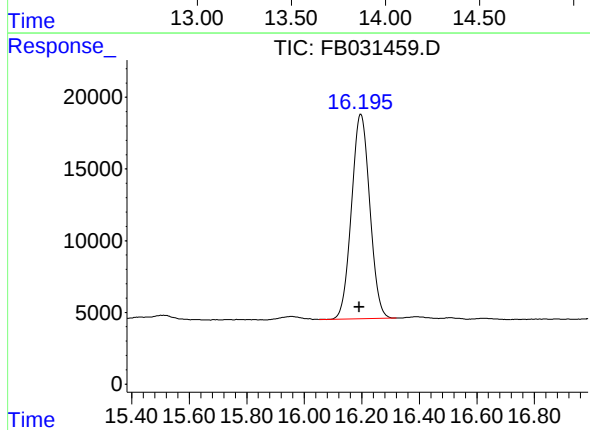

#10 1,2,4-Trimethylbenzene

R.T.: 16.197 min
Delta R.T.: 0.005 min
Response: 629101
Conc: 22.21 ng/ml