

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_B\Data\FB020719\
Data File : FB019662.D
Signal(s) : FID2B.CH
Acq On : 7 Feb 2019 13:26
Operator : MJ/SJ
Sample : K1401-07MS
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 08 07:54:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
Quant Title :
QLast Update : Tue Jan 29 12:07:12 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.042	197356	17.646 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.896	478922	26.138 ng/ml
2) t	2,2,4-Trimethylpentane	7.658	409250	23.429 ng/ml
3) t	n-Heptane	7.997	127775	7.675 ng/ml
4) t	Benzene	8.135	179873	9.341 ng/ml
6) t	Toluene	10.889	448570	25.773 ng/ml
7) t	Ethylbenzene	13.342	173346	8.006 ng/ml
8) t	m-Xylene	13.474	361486	16.005 ng/ml
9) t	O-Xylene	14.206	362427	16.389 ng/ml
10) t	1,2,4-Trimethylbenzene	16.492	330455	14.519 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_B\Data\FB020719\
Data File : FB019662.D
Signal(s) : FID2B.CH
Acq On : 7 Feb 2019 13:26
Operator : MJ/SJ
Sample : K1401-07MS
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 08 07:54:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
Quant Title :
QLast Update : Tue Jan 29 12:07:12 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

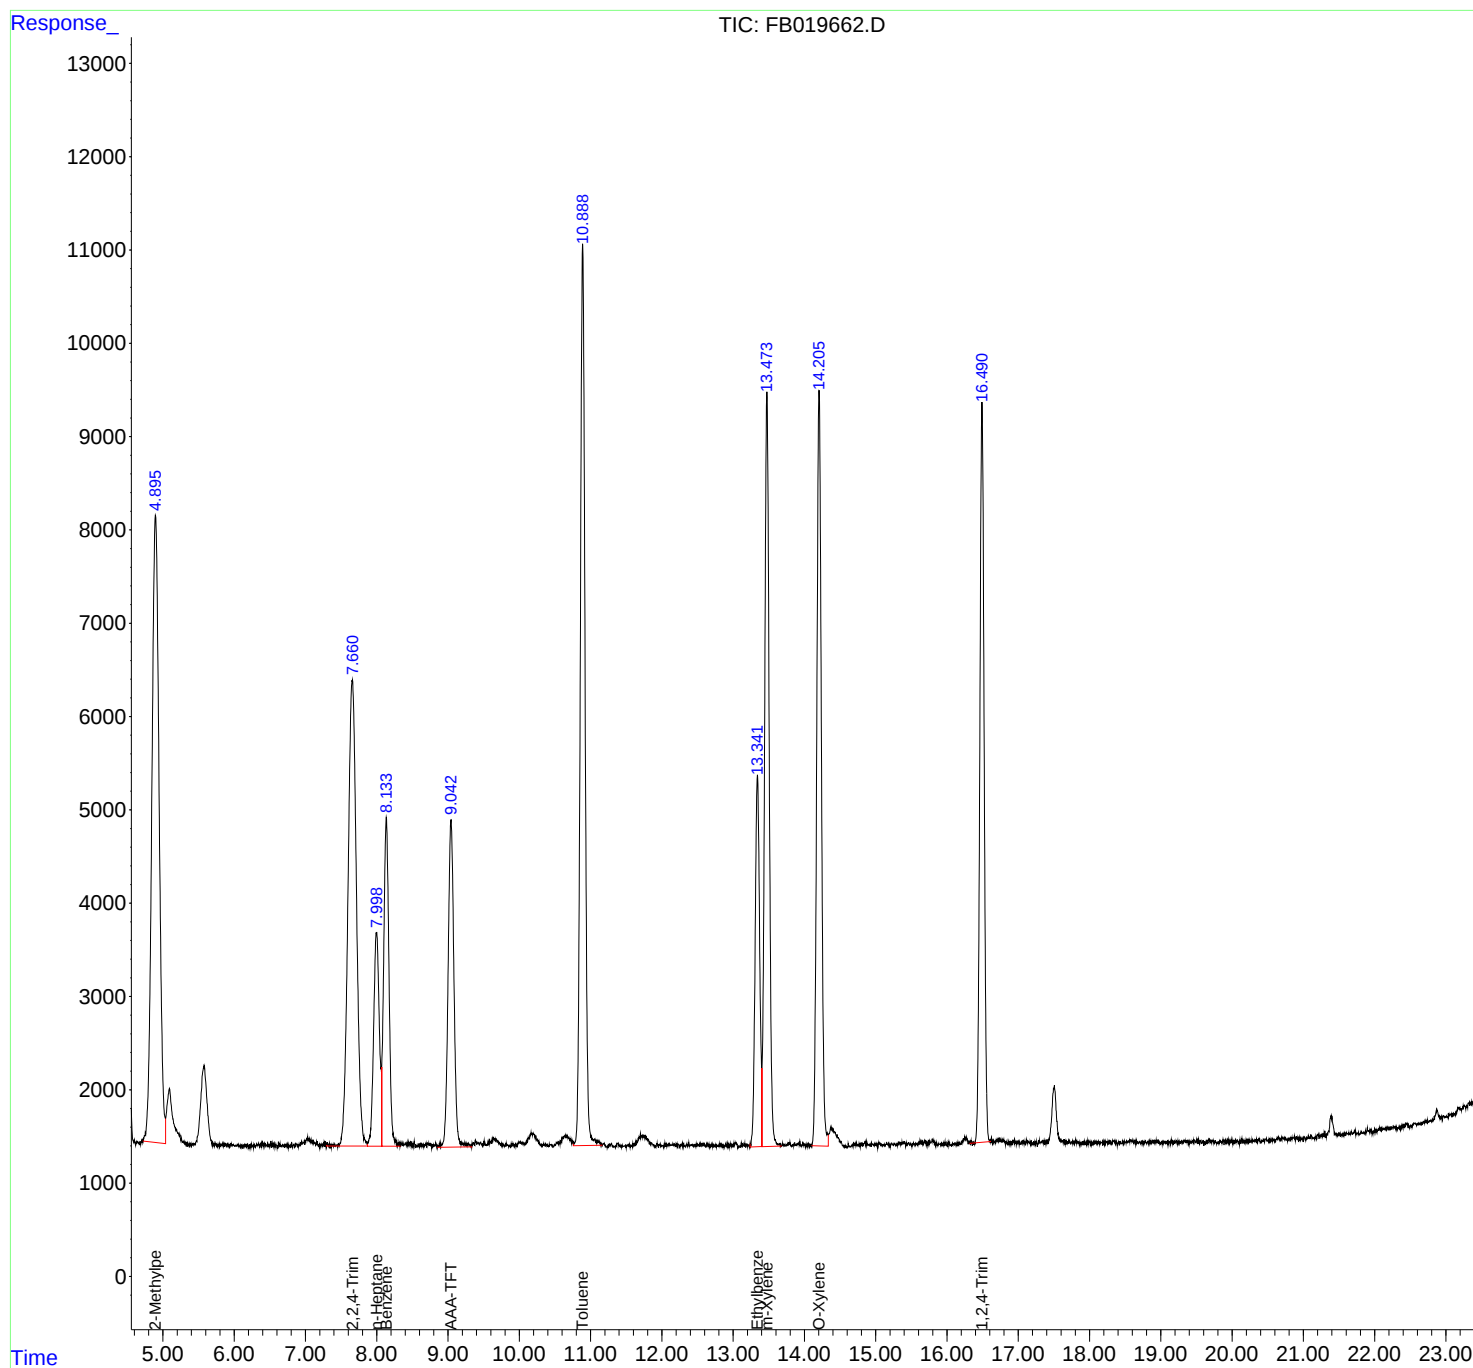

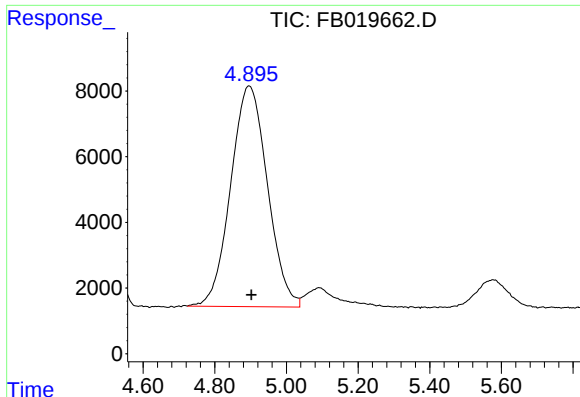


#1 2-Methylpentane

R.T.: 4.896 min
Delta R.T.: -0.006 min
Response: 478922
Conc: 26.14 ng/ml

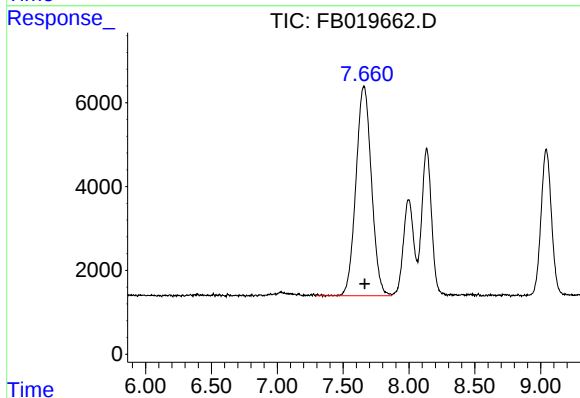


#2 2,2,4-Trimethylpentane

R.T.: 7.658 min
Delta R.T.: -0.007 min
Response: 409250
Conc: 23.43 ng/ml

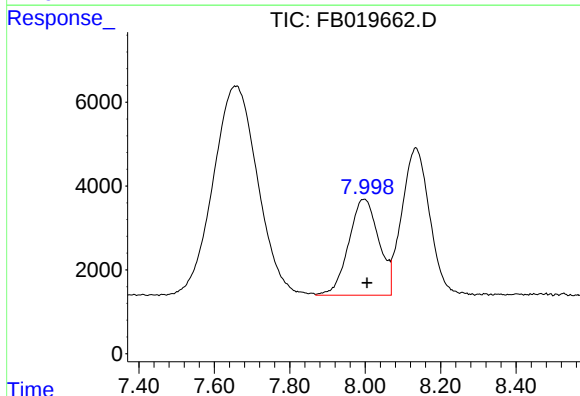


#3 n-Heptane

R.T.: 7.997 min
Delta R.T.: -0.007 min
Response: 127775
Conc: 7.67 ng/ml

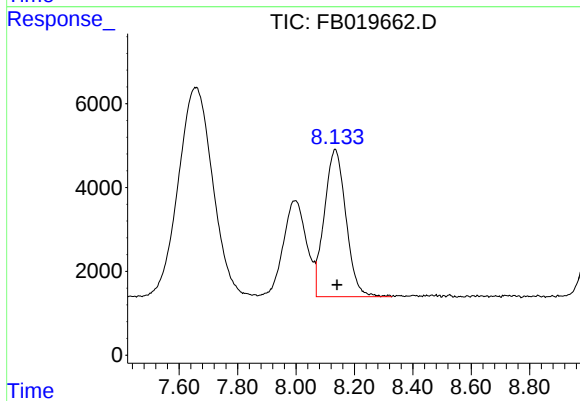


#4 Benzene

R.T.: 8.135 min
Delta R.T.: -0.006 min
Response: 179873
Conc: 9.34 ng/ml

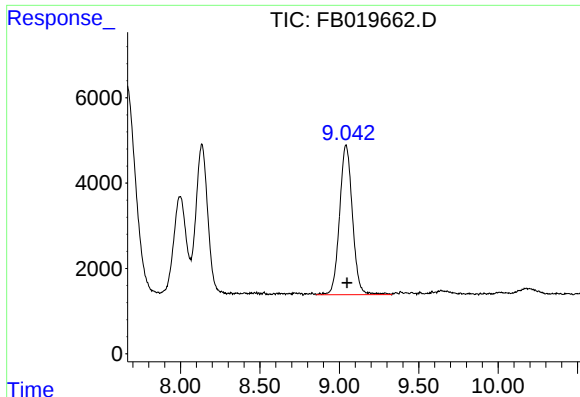


#5 AAA-TFT

R.T.: 9.042 min
Delta R.T.: -0.008 min
Response: 197356
Conc: 17.65 ng/ml

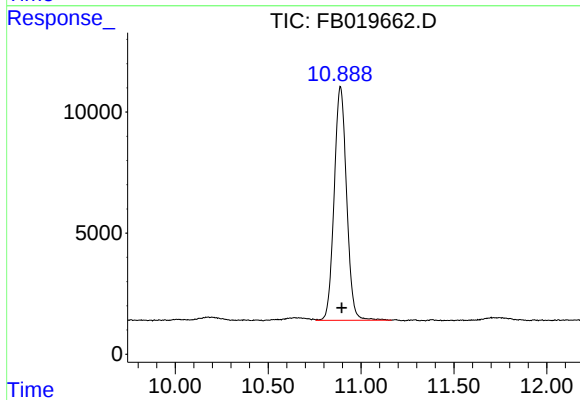


#6 Toluene

R.T.: 10.889 min
Delta R.T.: -0.007 min
Response: 448570
Conc: 25.77 ng/ml

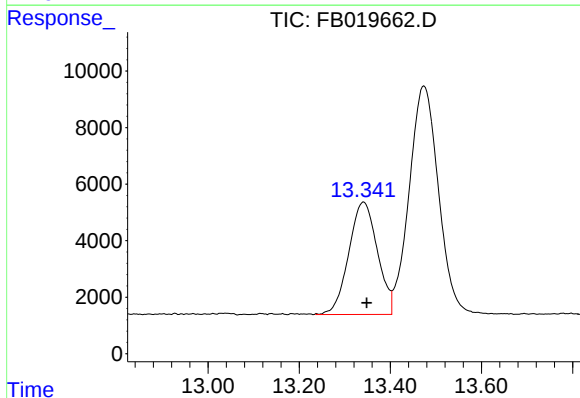


#7 Ethylbenzene

R.T.: 13.342 min
Delta R.T.: -0.007 min
Response: 173346
Conc: 8.01 ng/ml

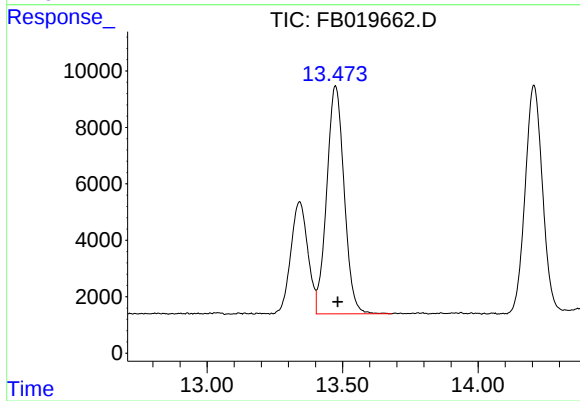


#8 m-Xylene

R.T.: 13.474 min
Delta R.T.: -0.008 min
Response: 361486
Conc: 16.01 ng/ml

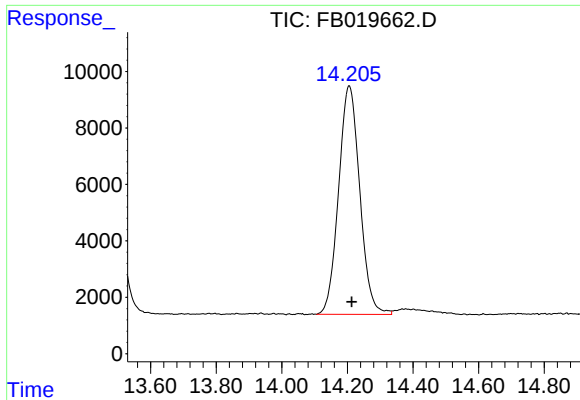

#9 O-Xylene

R.T.: 14.206 min
Delta R.T.: -0.008 min
Response: 362427
Conc: 16.39 ng/ml

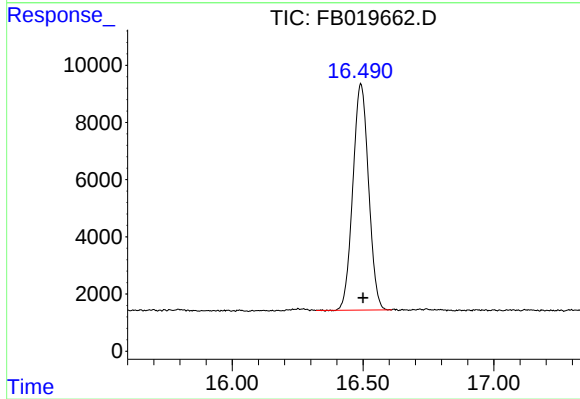

#10 1,2,4-Trimethylbenzene

R.T.: 16.492 min
Delta R.T.: -0.008 min
Response: 330455
Conc: 14.52 ng/ml