

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_B\Data\FB020719\
Data File : FB019663.D
Signal(s) : FID2B.CH
Acq On : 7 Feb 2019 13:56
Operator : MJ/SJ
Sample : K1401-07MSD
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 08 07:54:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
Quant Title :
QLast Update : Tue Jan 29 12:07:12 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.043	203061	18.156 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.897	472611	25.793 ng/ml
2) t	2,2,4-Trimethylpentane	7.658	400173	22.909 ng/ml
3) t	n-Heptane	7.998	121661	7.308 ng/ml
4) t	Benzene	8.135	177636	9.225 ng/ml
6) t	Toluene	10.890	448625	25.776 ng/ml
7) t	Ethylbenzene	13.342	179515	8.291 ng/ml
8) t	m-Xylene	13.475	374434	16.578 ng/ml
9) t	O-Xylene	14.207	374981	16.957 ng/ml
10) t	1,2,4-Trimethylbenzene	16.493	349210	15.343 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_B\Data\FB020719\
Data File : FB019663.D
Signal(s) : FID2B.CH
Acq On : 7 Feb 2019 13:56
Operator : MJ/SJ
Sample : K1401-07MSD
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 08 07:54:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
Quant Title :
QLast Update : Tue Jan 29 12:07:12 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

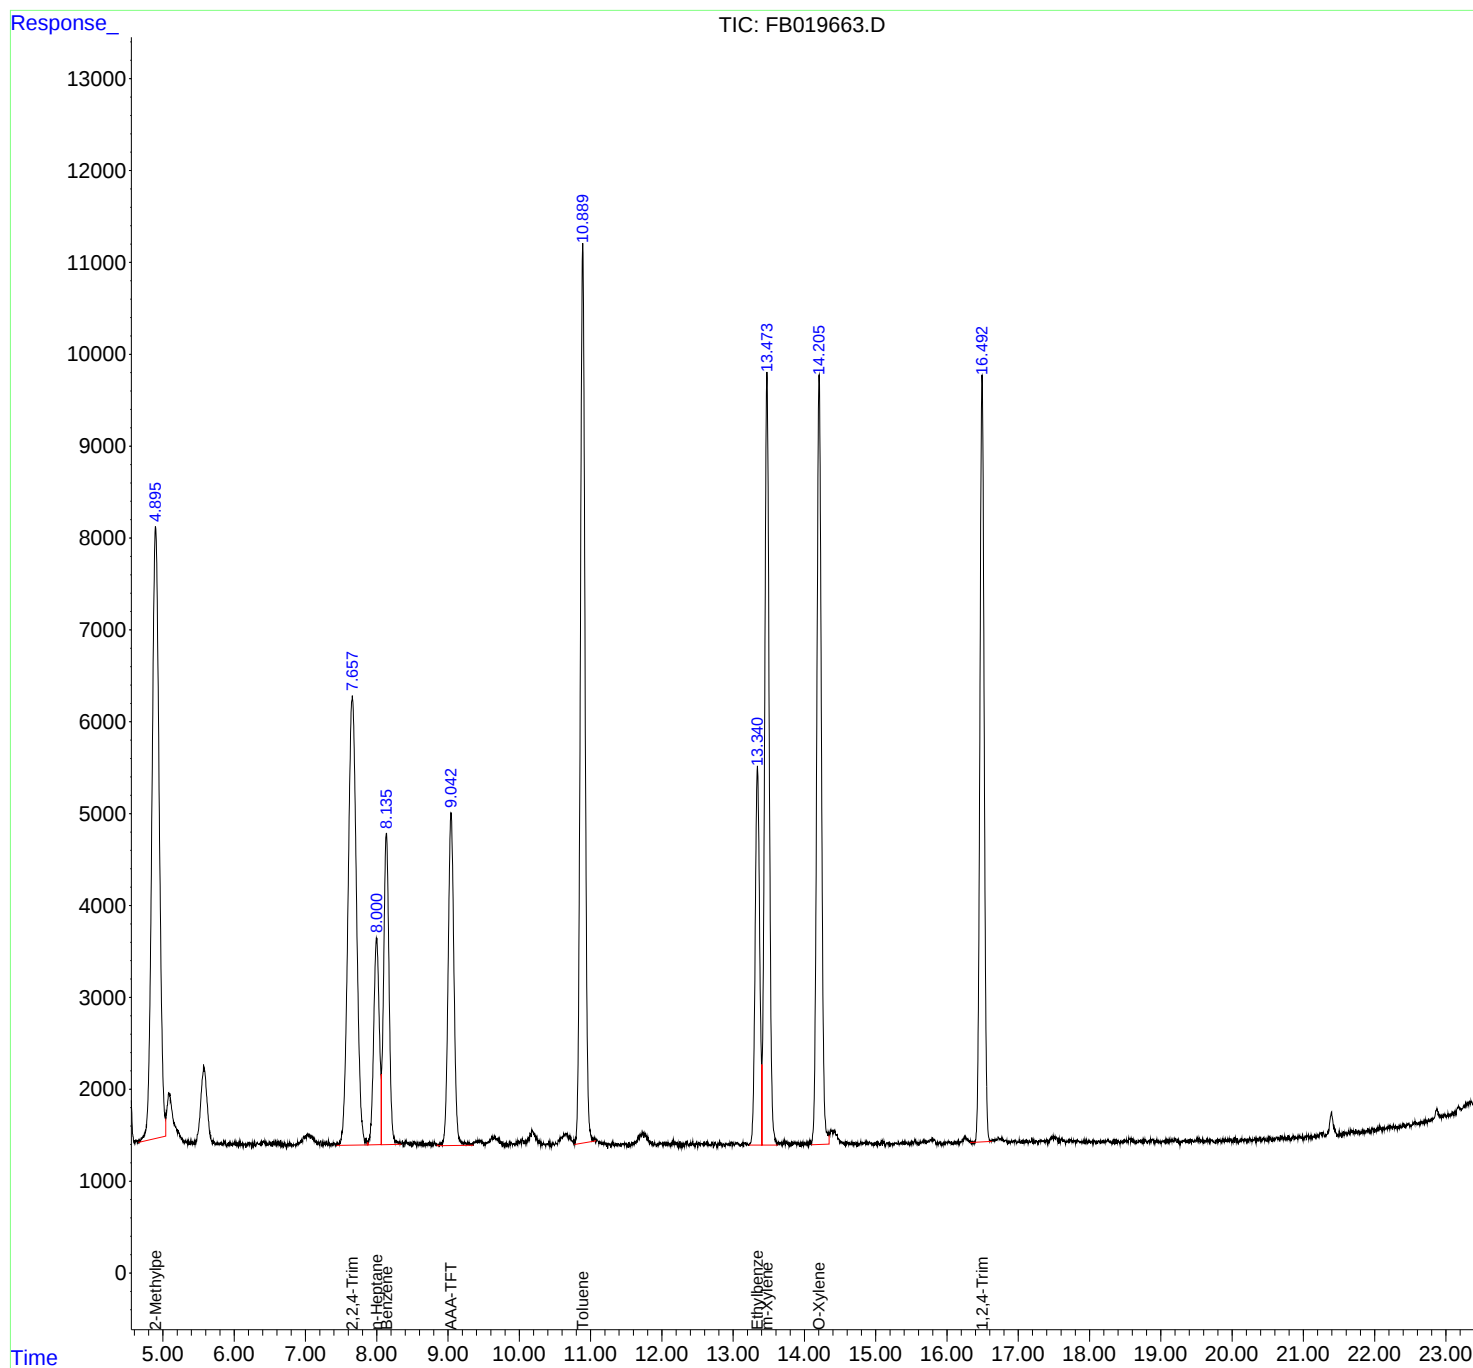

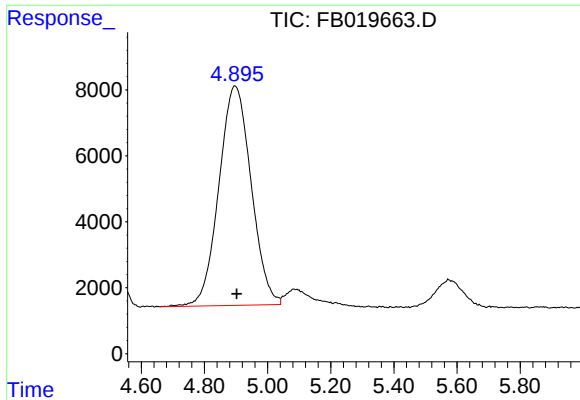


#1 2-Methylpentane

R.T.: 4.897 min
Delta R.T.: -0.005 min
Response: 472611
Conc: 25.79 ng/ml

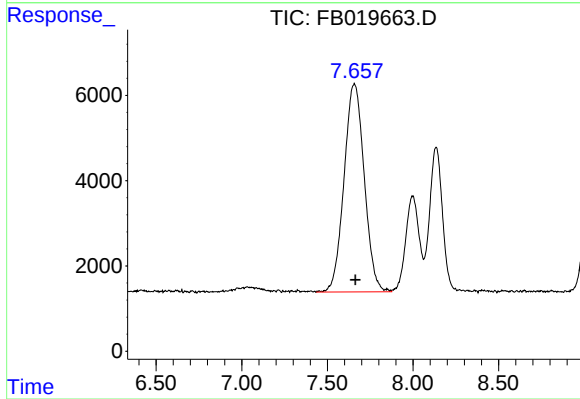


#2 2,2,4-Trimethylpentane

R.T.: 7.658 min
Delta R.T.: -0.006 min
Response: 400173
Conc: 22.91 ng/ml

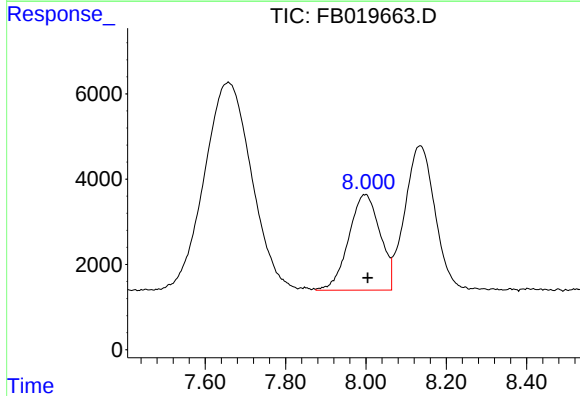


#3 n-Heptane

R.T.: 7.998 min
Delta R.T.: -0.006 min
Response: 121661
Conc: 7.31 ng/ml

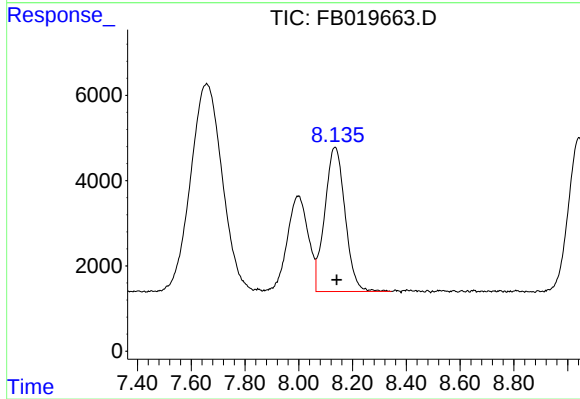


#4 Benzene

R.T.: 8.135 min
Delta R.T.: -0.006 min
Response: 177636
Conc: 9.23 ng/ml

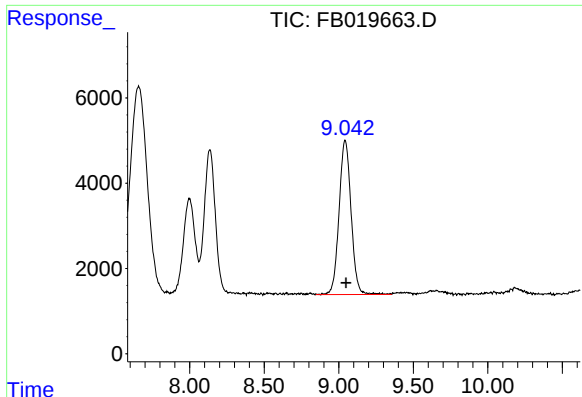


#5 AAA-TFT

R.T.: 9.043 min
Delta R.T.: -0.007 min
Response: 203061
Conc: 18.16 ng/ml

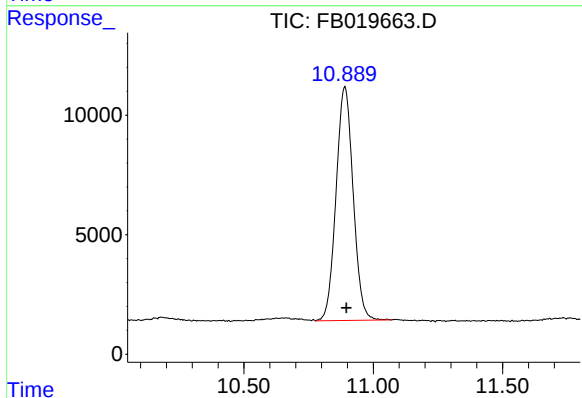


#6 Toluene

R.T.: 10.890 min
Delta R.T.: -0.006 min
Response: 448625
Conc: 25.78 ng/ml

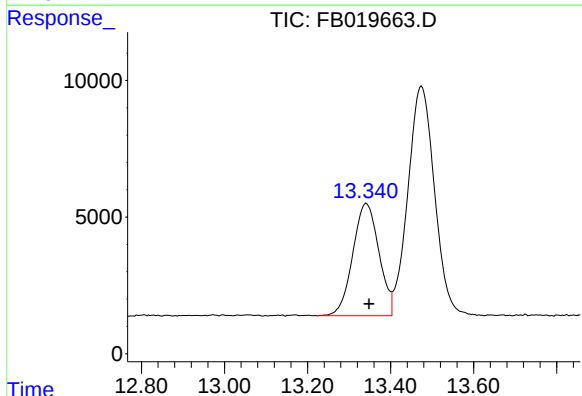


#7 Ethylbenzene

R.T.: 13.342 min
Delta R.T.: -0.007 min
Response: 179515
Conc: 8.29 ng/ml

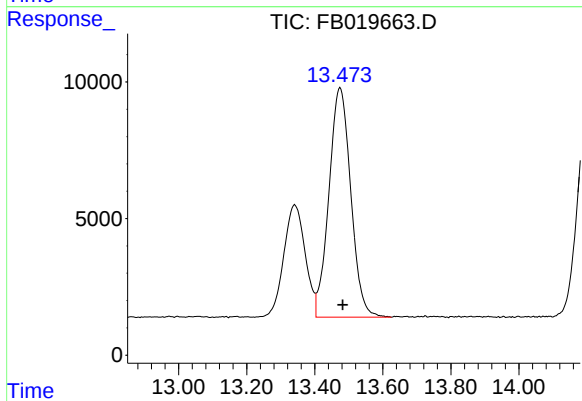


#8 m-Xylene

R.T.: 13.475 min
Delta R.T.: -0.007 min
Response: 374434
Conc: 16.58 ng/ml

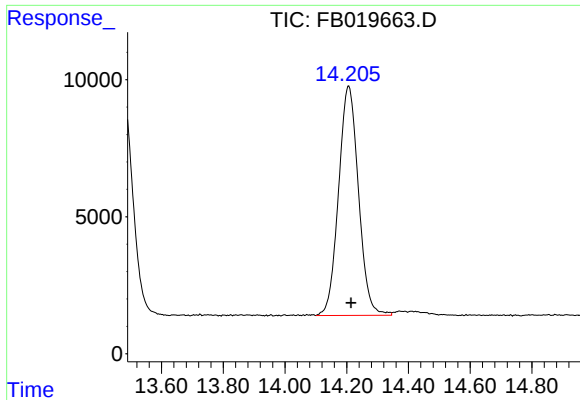

#9 O-Xylene

R.T.: 14.207 min
Delta R.T.: -0.007 min
Response: 374981
Conc: 16.96 ng/ml

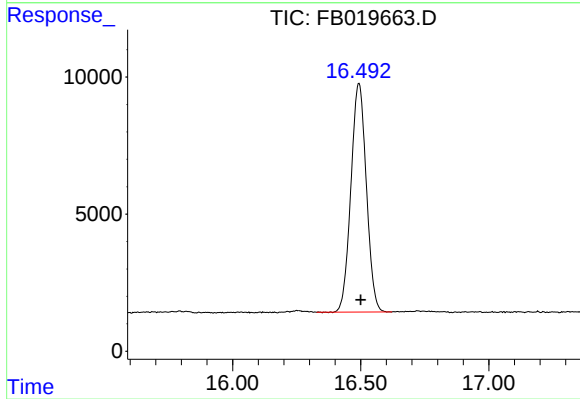

#10 1,2,4-Trimethylbenzene

R.T.: 16.493 min
Delta R.T.: -0.007 min
Response: 349210
Conc: 15.34 ng/ml