

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020725\
 Data File : FB031482.D
 Signal(s) : FID2B.CH
 Acq On : 7 Feb 2025 10:18
 Operator : YP/AJ
 Sample : VBF0207S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Feb 08 00:59:02 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011525.M
 Quant Title :
 QLast Update : Wed Jan 15 12:01:08 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	488539	20.481 ng/ml
Target Compounds			
8) t m-Xylene	13.183	4539	0.121 ng/ml
9) t O-Xylene	13.918	2973	0.083 ng/ml
10) t 1,2,4-Trimethylbenzene	16.197	13229	0.467 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020725\
Data File : FB031482.D
Signal(s) : FID2B.CH
Acq On : 7 Feb 2025 10:18
Operator : YP/AJ
Sample : VBF0207S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Feb 08 00:59:02 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011525.M
Quant Title :
QLast Update : Wed Jan 15 12:01:08 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

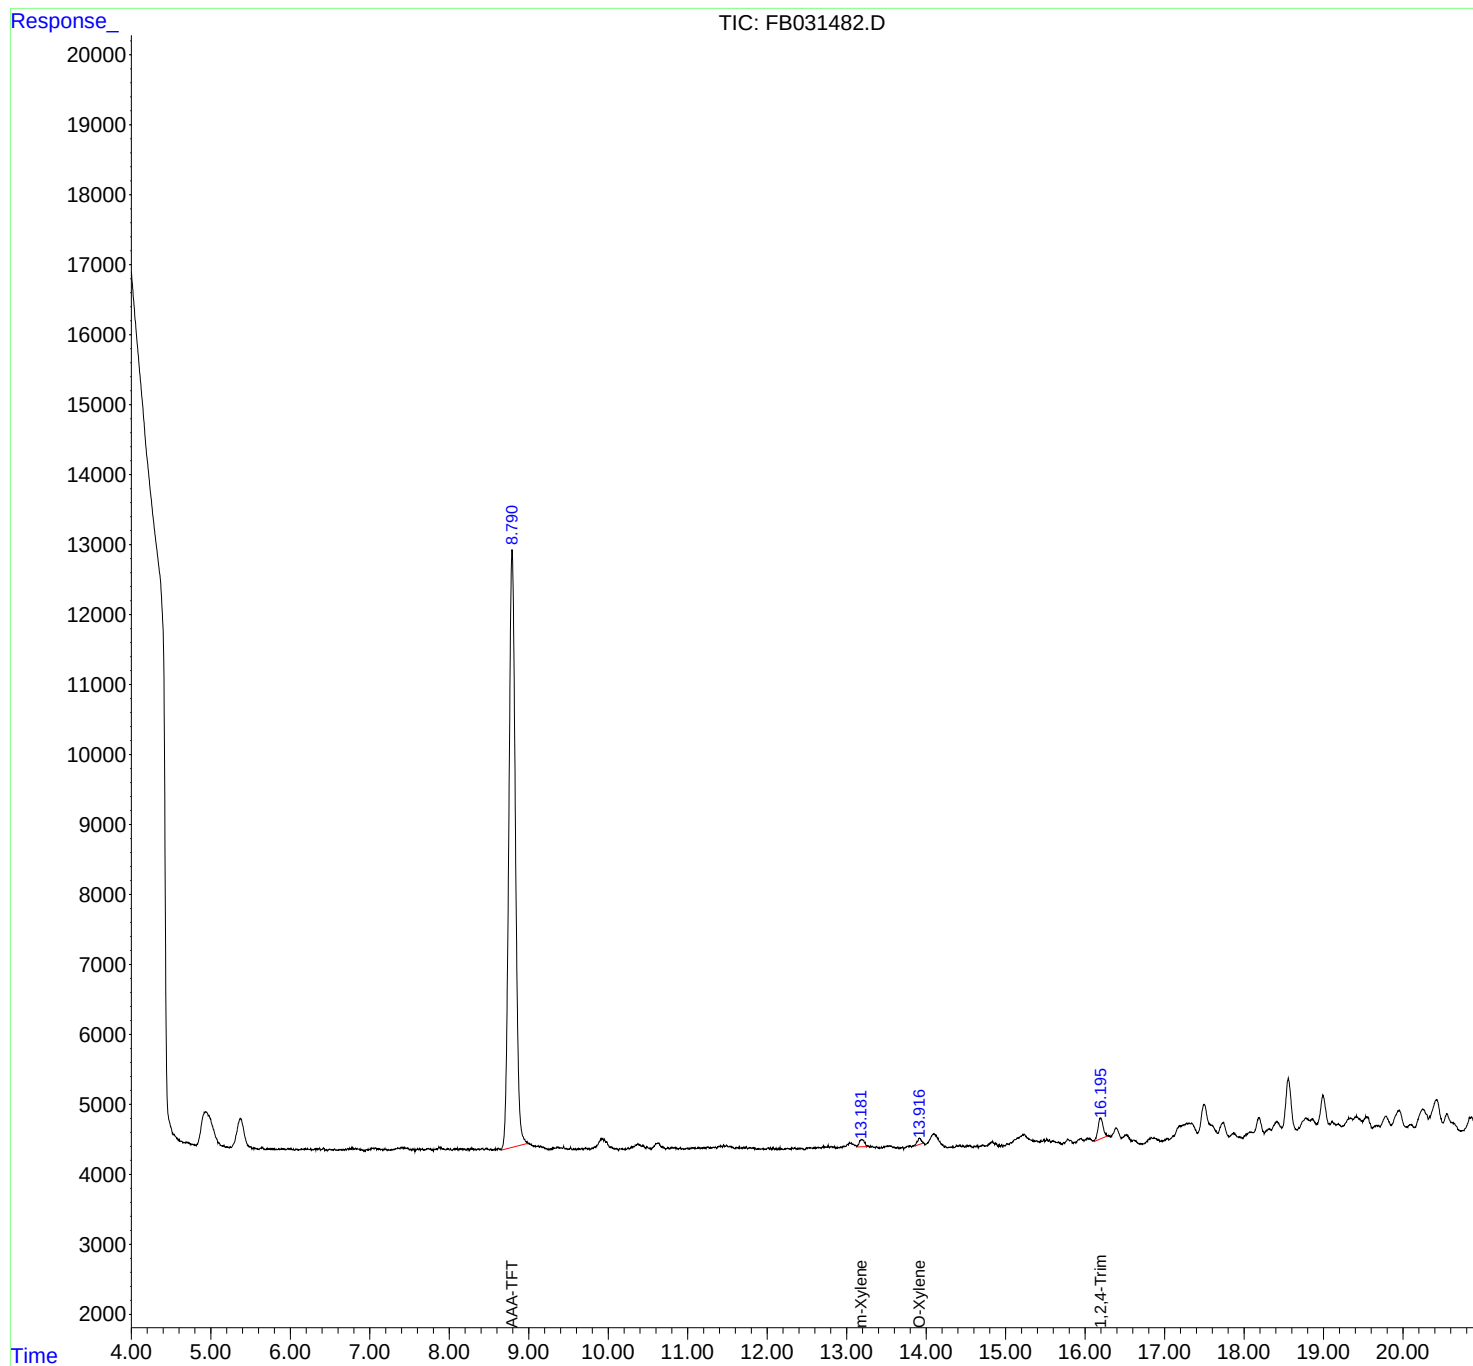


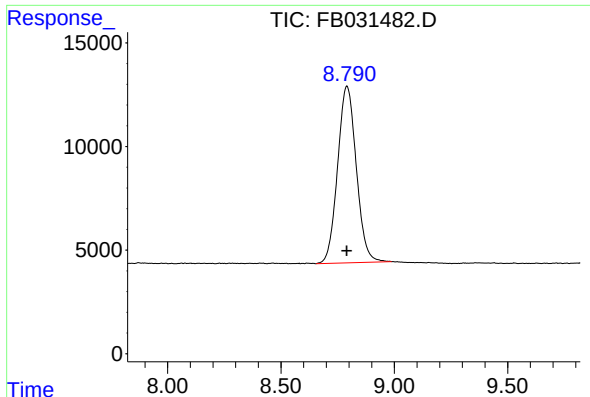

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: 0.002 min
Response: 488539
Conc: 20.48 ng/ml

Instrument :
FID_B
ClientSampleId :

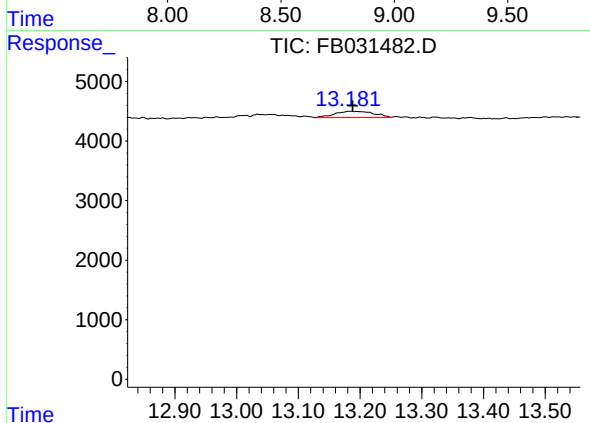


#8 m-Xylene

R.T.: 13.183 min
Delta R.T.: -0.005 min
Response: 4539
Conc: 0.12 ng/ml

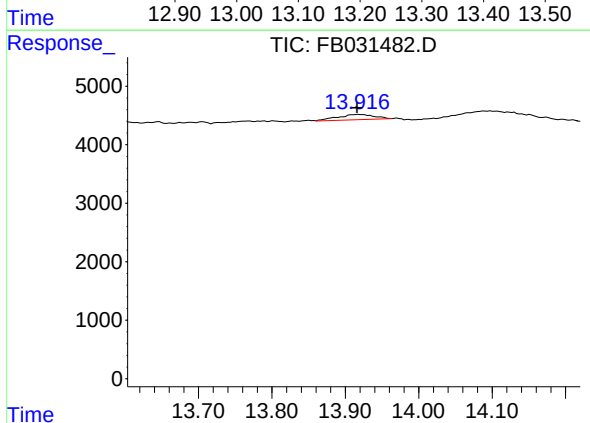

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.002 min
Response: 2973
Conc: 0.08 ng/ml

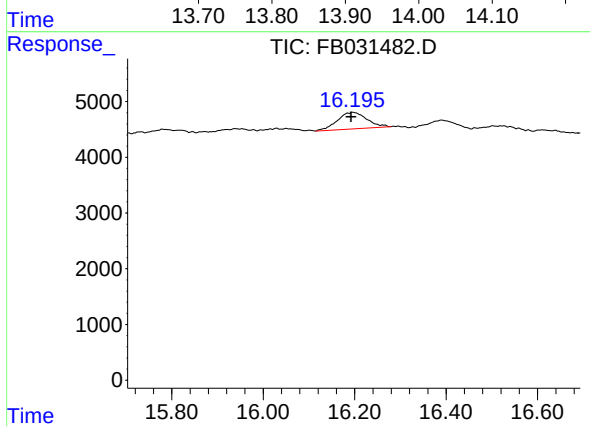

#10 1,2,4-Trimethylbenzene

R.T.: 16.197 min
Delta R.T.: 0.005 min
Response: 13229
Conc: 0.47 ng/ml