

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020819\
 Data File : FB019668.D
 Signal(s) : FID2B.CH
 Acq On : 8 Feb 2019 10:46
 Operator : MJ/SJ
 Sample : BSF0208S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Feb 08 23:08:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
 Quant Title :
 QLast Update : Tue Jan 29 12:07:12 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.042	216174	18.493 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.896	608519	35.148 ng/ml
2) t 2,2,4-Trimethylpentane	7.657	594536	35.851 ng/ml
3) t n-Heptane	7.997	183151	11.365 ng/ml
4) t Benzene	8.135	202859	10.755 ng/ml
6) t Toluene	10.890	527497	30.156 ng/ml
7) t Ethylbenzene	13.342	209520	9.547 ng/ml
8) t m-Xylene	13.475	432500	18.897 ng/ml
9) t O-Xylene	14.207	417031	18.672 ng/ml
10) t 1,2,4-Trimethylbenzene	16.493	429993	18.558 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020819\
Data File : FB019668.D
Signal(s) : FID2B.CH
Acq On : 8 Feb 2019 10:46
Operator : MJ/SJ
Sample : BSF0208S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Feb 08 23:08:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
Quant Title :
QLast Update : Tue Jan 29 12:07:12 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

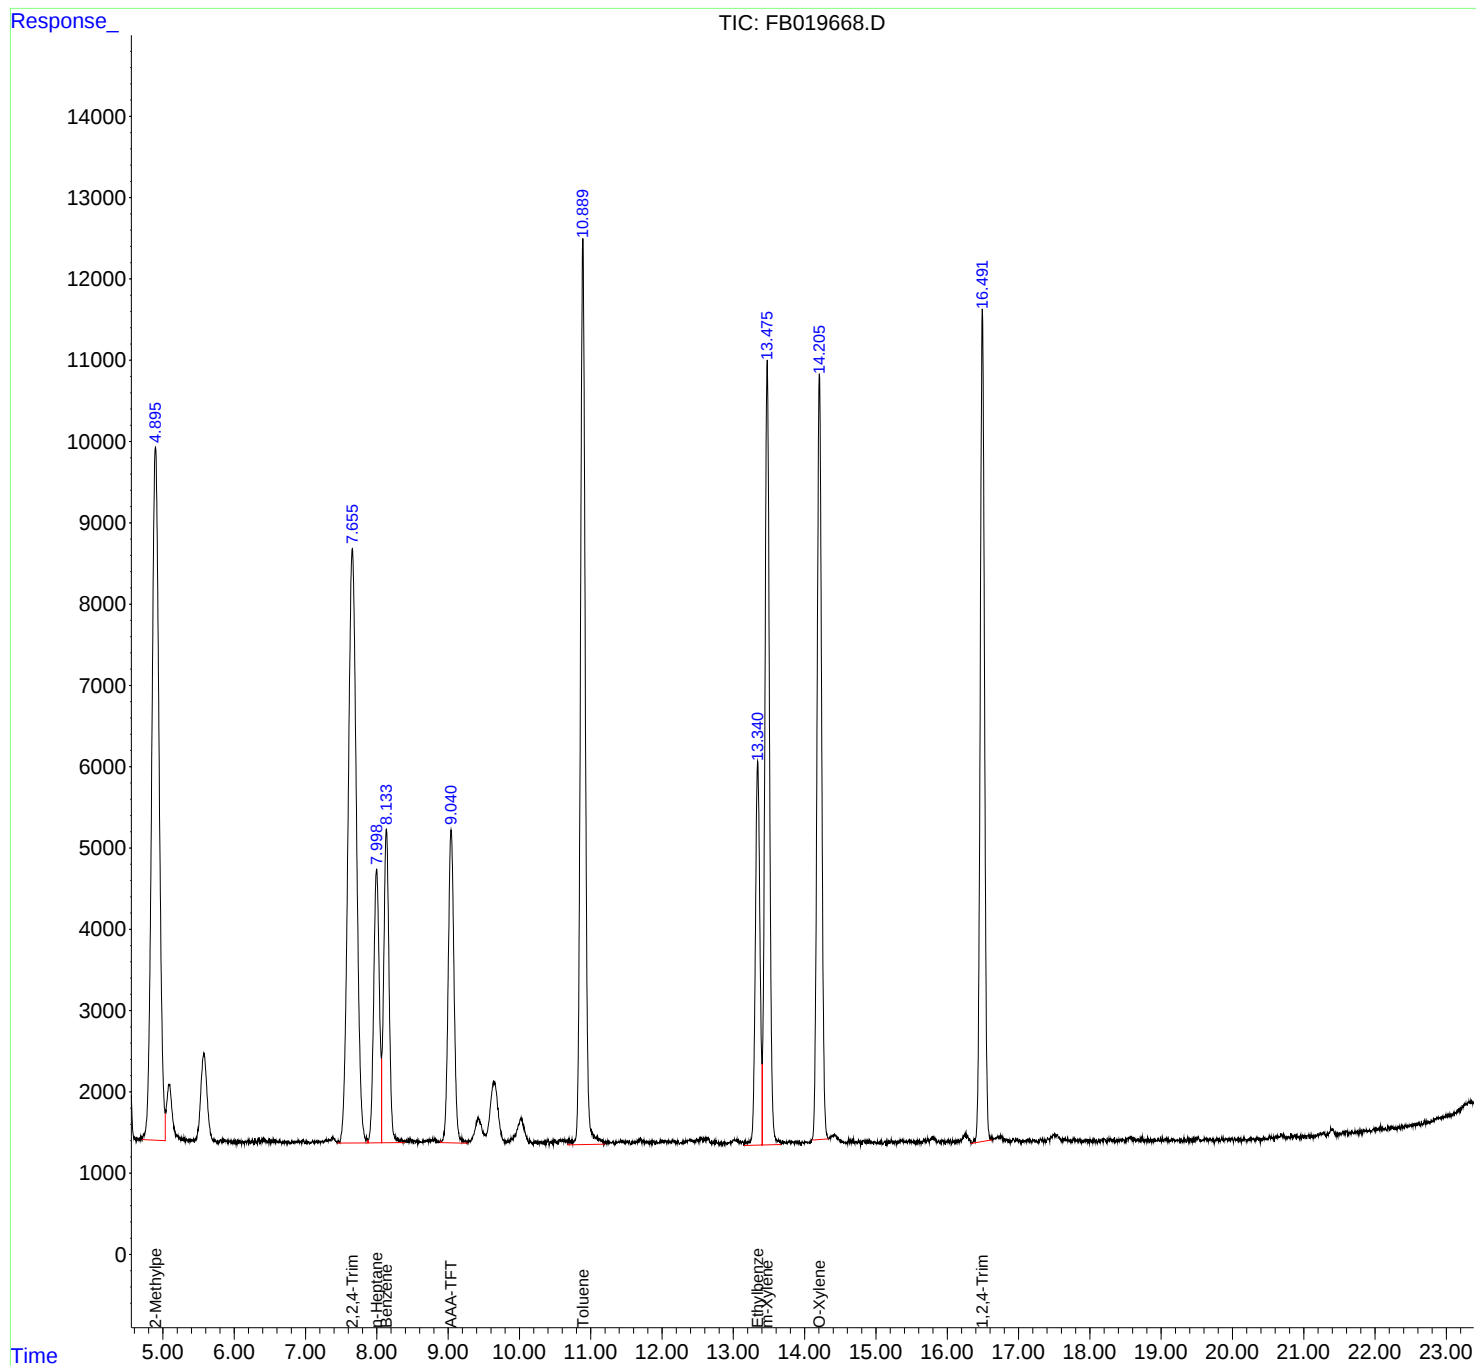


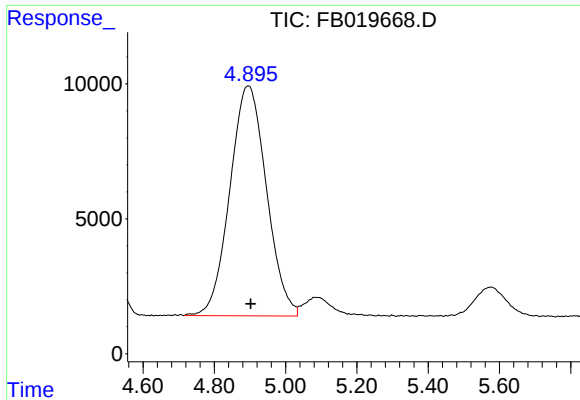

#1 2-Methylpentane


R.T.: 4.896 min
Delta R.T.: -0.006 min
Response: 608519
Conc: 35.15 ng/ml

Instrument :
FID_B
ClientSampleId :

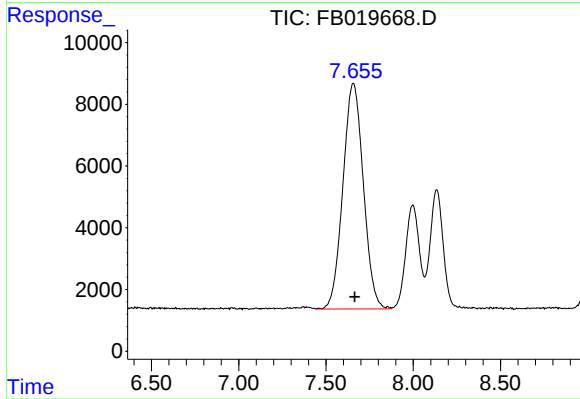


#2 2,2,4-Trimethylpentane

R.T.: 7.657 min
Delta R.T.: -0.008 min
Response: 594536
Conc: 35.85 ng/ml

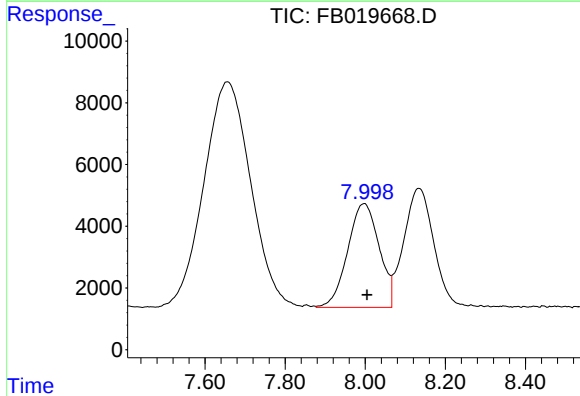


#3 n-Heptane

R.T.: 7.997 min
Delta R.T.: -0.007 min
Response: 183151
Conc: 11.37 ng/ml

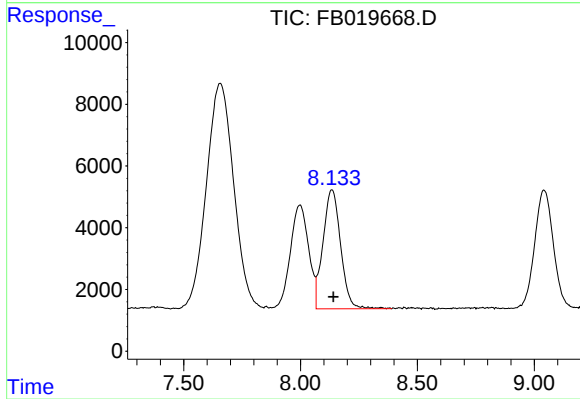

#4 Benzene


R.T.: 8.135 min
Delta R.T.: -0.007 min
Response: 202859
Conc: 10.76 ng/ml

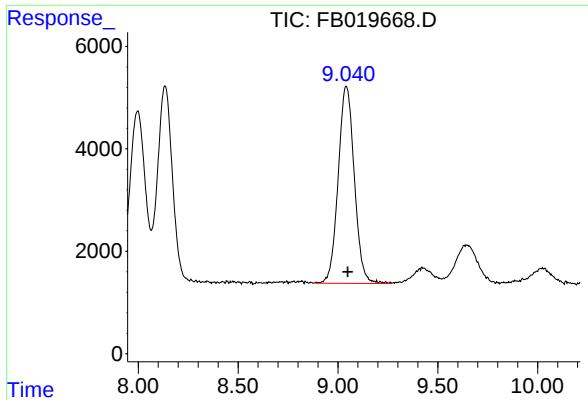

#5 AAA-TFT


R.T.: 9.042 min
Delta R.T.: -0.007 min
Response: 216174
Conc: 18.49 ng/ml

Instrument :
FID_B
ClientSampleId :

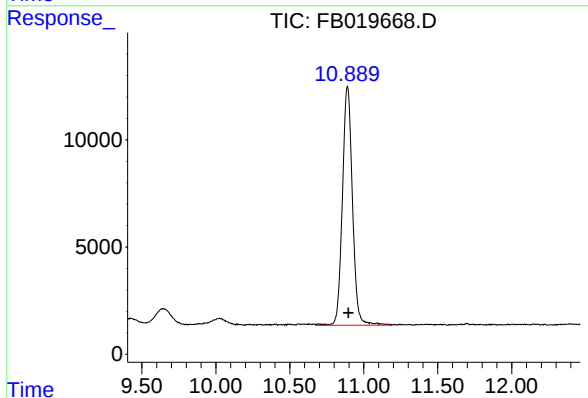


#6 Toluene

R.T.: 10.890 min
Delta R.T.: -0.007 min
Response: 527497
Conc: 30.16 ng/ml

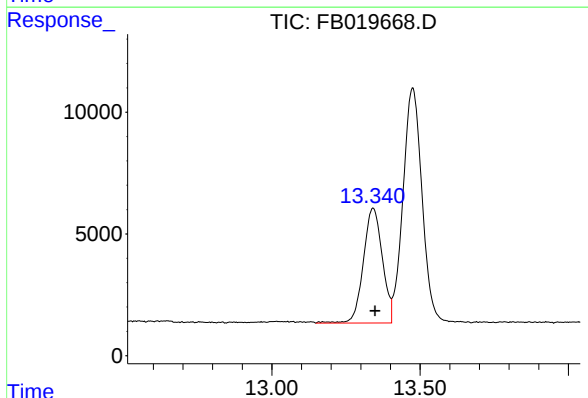


#7 Ethylbenzene

R.T.: 13.342 min
Delta R.T.: -0.007 min
Response: 209520
Conc: 9.55 ng/ml

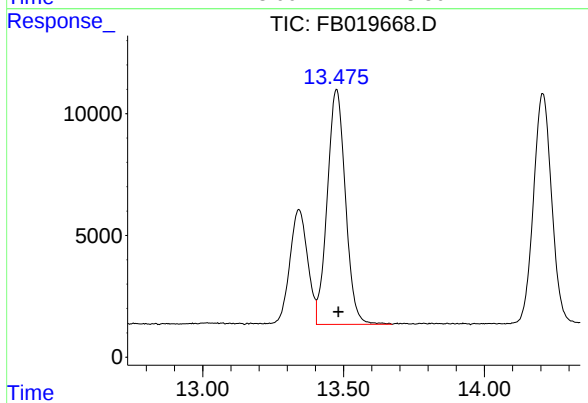

#8 m-Xylene


R.T.: 13.475 min
Delta R.T.: -0.007 min
Response: 432500
Conc: 18.90 ng/ml

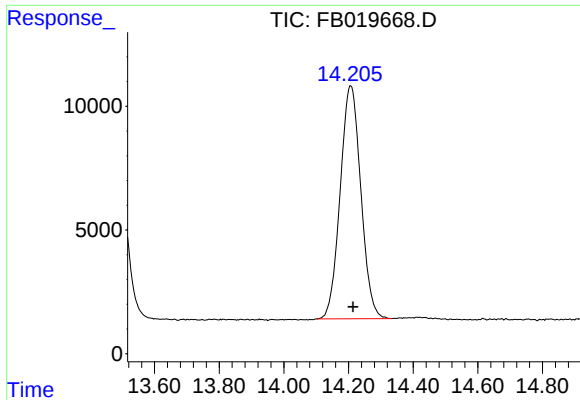

#9 O-Xylene

R.T.: 14.207 min
Delta R.T.: -0.006 min
Response: 417031
Conc: 18.67 ng/ml

Instrument :
FID_B
ClientSampleId :

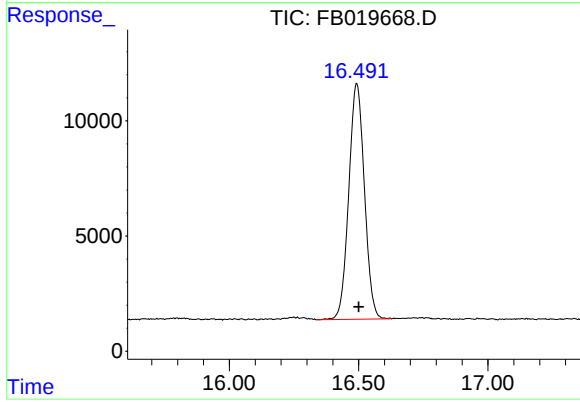

#10 1,2,4-Trimethylbenzene

R.T.: 16.493 min
Delta R.T.: -0.007 min
Response: 429993
Conc: 18.56 ng/ml